

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050619\
 Data File : VU031781.D
 Acq On : 06 May 2019 15:33
 Operator : JC/SP
 Sample : K2694-06
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFHF9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.395	88	95	106	rBV	374977	404734	13.20%	1.777%
2	1.678	175	183	198	rVB	316135	403745	13.17%	1.773%
3	2.270	356	367	380	rVB	626635	960155	31.31%	4.215%
4	2.460	423	426	428	rBV2	1250	818	0.03%	0.004%
5	2.572	457	461	466	rBV6	1774	1781	0.06%	0.008%
6	2.653	481	486	487	rBV3	1068	933	0.03%	0.004%
7	2.768	519	522	526	rVV3	1598	1094	0.04%	0.005%
8	2.839	531	544	554	rVV6	5357	12736	0.42%	0.056%
9	2.945	573	577	582	rBV4	1401	1369	0.04%	0.006%
10	3.048	606	609	613	rBV2	1149	852	0.03%	0.004%
11	3.167	638	646	649	rBV5	1469	1864	0.06%	0.008%
12	3.225	661	664	669	rVB3	1204	831	0.03%	0.004%
13	3.286	678	683	687	rBV3	1801	1817	0.06%	0.008%
14	3.312	688	691	695	rVV5	2103	1757	0.06%	0.008%
15	3.550	762	765	768	rVV2	1303	1053	0.03%	0.005%
16	3.575	768	773	777	rVV3	1086	1436	0.05%	0.006%
17	3.595	777	779	781	rVV2	1651	858	0.03%	0.004%
18	3.611	781	784	787	rVV	1461	904	0.03%	0.004%
19	3.704	809	813	817	rVB2	1163	1114	0.04%	0.005%
20	3.730	817	821	822	rBV2	970	747	0.02%	0.003%
21	3.743	822	825	828	rVB2	1231	761	0.02%	0.003%
22	3.810	841	846	849	rVB5	1091	854	0.03%	0.004%
23	3.887	867	870	873	rVB3	1268	769	0.03%	0.003%
24	3.907	873	876	880	rVB4	1532	1202	0.04%	0.005%
25	3.955	882	891	893	rBV3	1532	2133	0.07%	0.009%
26	4.013	897	909	913	rBV6	5044	8795	0.29%	0.039%
27	4.080	927	930	934	rBV4	1182	991	0.03%	0.004%
28	4.183	948	962	998	rBV	330726	1007685	32.87%	4.424%
29	4.395	1023	1028	1047	rVB3	15942	36630	1.19%	0.161%
30	4.643	1087	1105	1128	rBV	513446	1231018	40.15%	5.405%
31	4.913	1186	1189	1194	rVB5	2197	1832	0.06%	0.008%
32	5.122	1251	1254	1259	rBV4	1376	1181	0.04%	0.005%
33	5.170	1263	1269	1273	rVB6	931	1021	0.03%	0.004%
34	5.222	1282	1285	1290	rVB4	1352	1231	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050619\
 Data File : VU031781.D
 Acq On : 06 May 2019 15:33
 Operator : JC/SP
 Sample : K2694-06
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFHF9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	5.334	1295	1320	1357	rBV2	986216	3066123	100.00%	13.461%
36	5.595	1398	1401	1402	rBV3	1329	771	0.03%	0.003%
37	5.665	1420	1423	1429	rVB8	1351	1015	0.03%	0.004%
38	5.730	1440	1443	1446	rBV5	1498	1120	0.04%	0.005%
39	5.884	1476	1491	1523	rBV	837577	1757341	57.31%	7.715%
40	6.180	1572	1583	1597	rBV	15936	37942	1.24%	0.167%
41	6.328	1615	1629	1659	rBV	719929	1456231	47.49%	6.393%
42	6.713	1745	1749	1753	rVB3	1963	1553	0.05%	0.007%
43	6.823	1778	1783	1785	rBV3	1238	824	0.03%	0.004%
44	6.919	1811	1813	1818	rVB2	1261	921	0.03%	0.004%
45	7.025	1839	1846	1853	rBV5	1085	1574	0.05%	0.007%
46	7.119	1872	1875	1882	rBV5	1280	1195	0.04%	0.005%
47	7.225	1896	1908	1937	rBV	348103	665555	21.71%	2.922%
48	7.421	1966	1969	1972	rBV3	1343	1258	0.04%	0.006%
49	7.485	1985	1989	1994	rVB3	2422	2412	0.08%	0.011%
50	7.511	1994	1997	1999	rBV2	1189	878	0.03%	0.004%
51	7.562	2000	2013	2046	rBV	1096113	2021010	65.91%	8.873%
52	7.848	2091	2102	2131	rBV2	233460	442464	14.43%	1.943%
53	8.061	2166	2168	2173	rVB3	1209	790	0.03%	0.003%
54	8.176	2193	2204	2213	rBV2	15748	27887	0.91%	0.122%
55	8.312	2234	2246	2283	rBV2	1027557	2075663	67.70%	9.113%
56	8.607	2336	2338	2340	rBV3	1354	749	0.02%	0.003%
57	8.623	2341	2343	2347	rVB5	2462	1416	0.05%	0.006%
58	8.720	2367	2373	2375	rBV6	1549	1289	0.04%	0.006%
59	8.736	2375	2378	2382	rVB4	1652	1132	0.04%	0.005%
60	8.964	2442	2449	2453	rBV7	1211	1833	0.06%	0.008%
61	9.086	2471	2487	2515	rBV	1236920	2159359	70.43%	9.480%
62	9.289	2547	2550	2554	rBV4	1427	1418	0.05%	0.006%
63	9.408	2585	2587	2589	rBV2	1236	791	0.03%	0.003%
64	9.463	2601	2604	2608	rVB3	1386	805	0.03%	0.004%
65	9.582	2639	2641	2645	rVB2	1417	851	0.03%	0.004%
66	9.607	2645	2649	2651	rBV	1320	877	0.03%	0.004%
67	9.623	2651	2654	2657	rBV2	1672	1219	0.04%	0.005%
68	9.659	2662	2665	2668	rVB3	1214	795	0.03%	0.003%
69	9.684	2668	2673	2674	rBV2	2304	1738	0.06%	0.008%
70	9.842	2713	2722	2725	rBV5	1862	2149	0.07%	0.009%
71	9.877	2728	2733	2736	rVB6	1205	1137	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050619\
 Data File : VU031781.D
 Acq On : 06 May 2019 15:33
 Operator : JC/SP
 Sample : K2694-06
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFHF9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	9.919	2744	2746	2751	rVB4	1511	1286	0.04%	0.006%
73	10.045	2778	2785	2788	rBV7	4459	5221	0.17%	0.023%
74	10.173	2820	2825	2831	rBV4	1486	1795	0.06%	0.008%
75	10.295	2857	2863	2864	rBV3	1448	1414	0.05%	0.006%
76	10.427	2892	2904	2926	rBV	945714	1529752	49.89%	6.716%
77	10.604	2951	2959	2973	rVB3	15773	27849	0.91%	0.122%
78	10.749	3000	3004	3007	rBV4	1692	1624	0.05%	0.007%
79	10.787	3014	3016	3020	rVB3	1578	885	0.03%	0.004%
80	10.819	3021	3026	3031	rBV6	1474	1731	0.06%	0.008%
81	10.890	3045	3048	3050	rBV3	1633	1144	0.04%	0.005%
82	10.951	3065	3067	3071	rVB2	1340	778	0.03%	0.003%
83	11.154	3127	3130	3135	rVB3	1207	1125	0.04%	0.005%
84	11.276	3165	3168	3172	rVV4	1471	944	0.03%	0.004%
85	11.379	3187	3200	3212	rBV4	6617	19459	0.63%	0.085%
86	11.482	3220	3232	3250	rBV	996883	1626856	53.06%	7.143%
87	11.771	3316	3322	3325	rBV7	3157	3872	0.13%	0.017%
88	11.855	3336	3348	3369	rBV	998836	1678176	54.73%	7.368%
89	12.424	3516	3525	3530	rBV4	2981	5098	0.17%	0.022%
90	12.475	3534	3541	3549	rVV3	8434	14111	0.46%	0.062%
91	12.601	3574	3580	3583	rBV3	2235	2999	0.10%	0.013%
92	12.977	3693	3697	3702	rVB4	1883	1796	0.06%	0.008%
93	13.176	3756	3759	3760	rBV2	1378	784	0.03%	0.003%
94	13.257	3782	3784	3790	rVB6	1439	1124	0.04%	0.005%
95	13.286	3790	3793	3795	rBV2	1771	1141	0.04%	0.005%
96	13.401	3825	3829	3833	rBV3	1958	1859	0.06%	0.008%
97	13.498	3857	3859	3863	rBV3	1372	1114	0.04%	0.005%
98	13.630	3897	3900	3902	rBV4	2379	1444	0.05%	0.006%
99	14.266	4095	4098	4103	rBV6	2086	2059	0.07%	0.009%
100	14.803	4263	4265	4267	rBV2	1713	853	0.03%	0.004%


Sum of corrected areas: 22777079

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU050619\
Data File : VU031781.D
Acq On : 06 May 2019 15:33
Operator : JC/SP
Sample : K2694-06
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFHF9

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

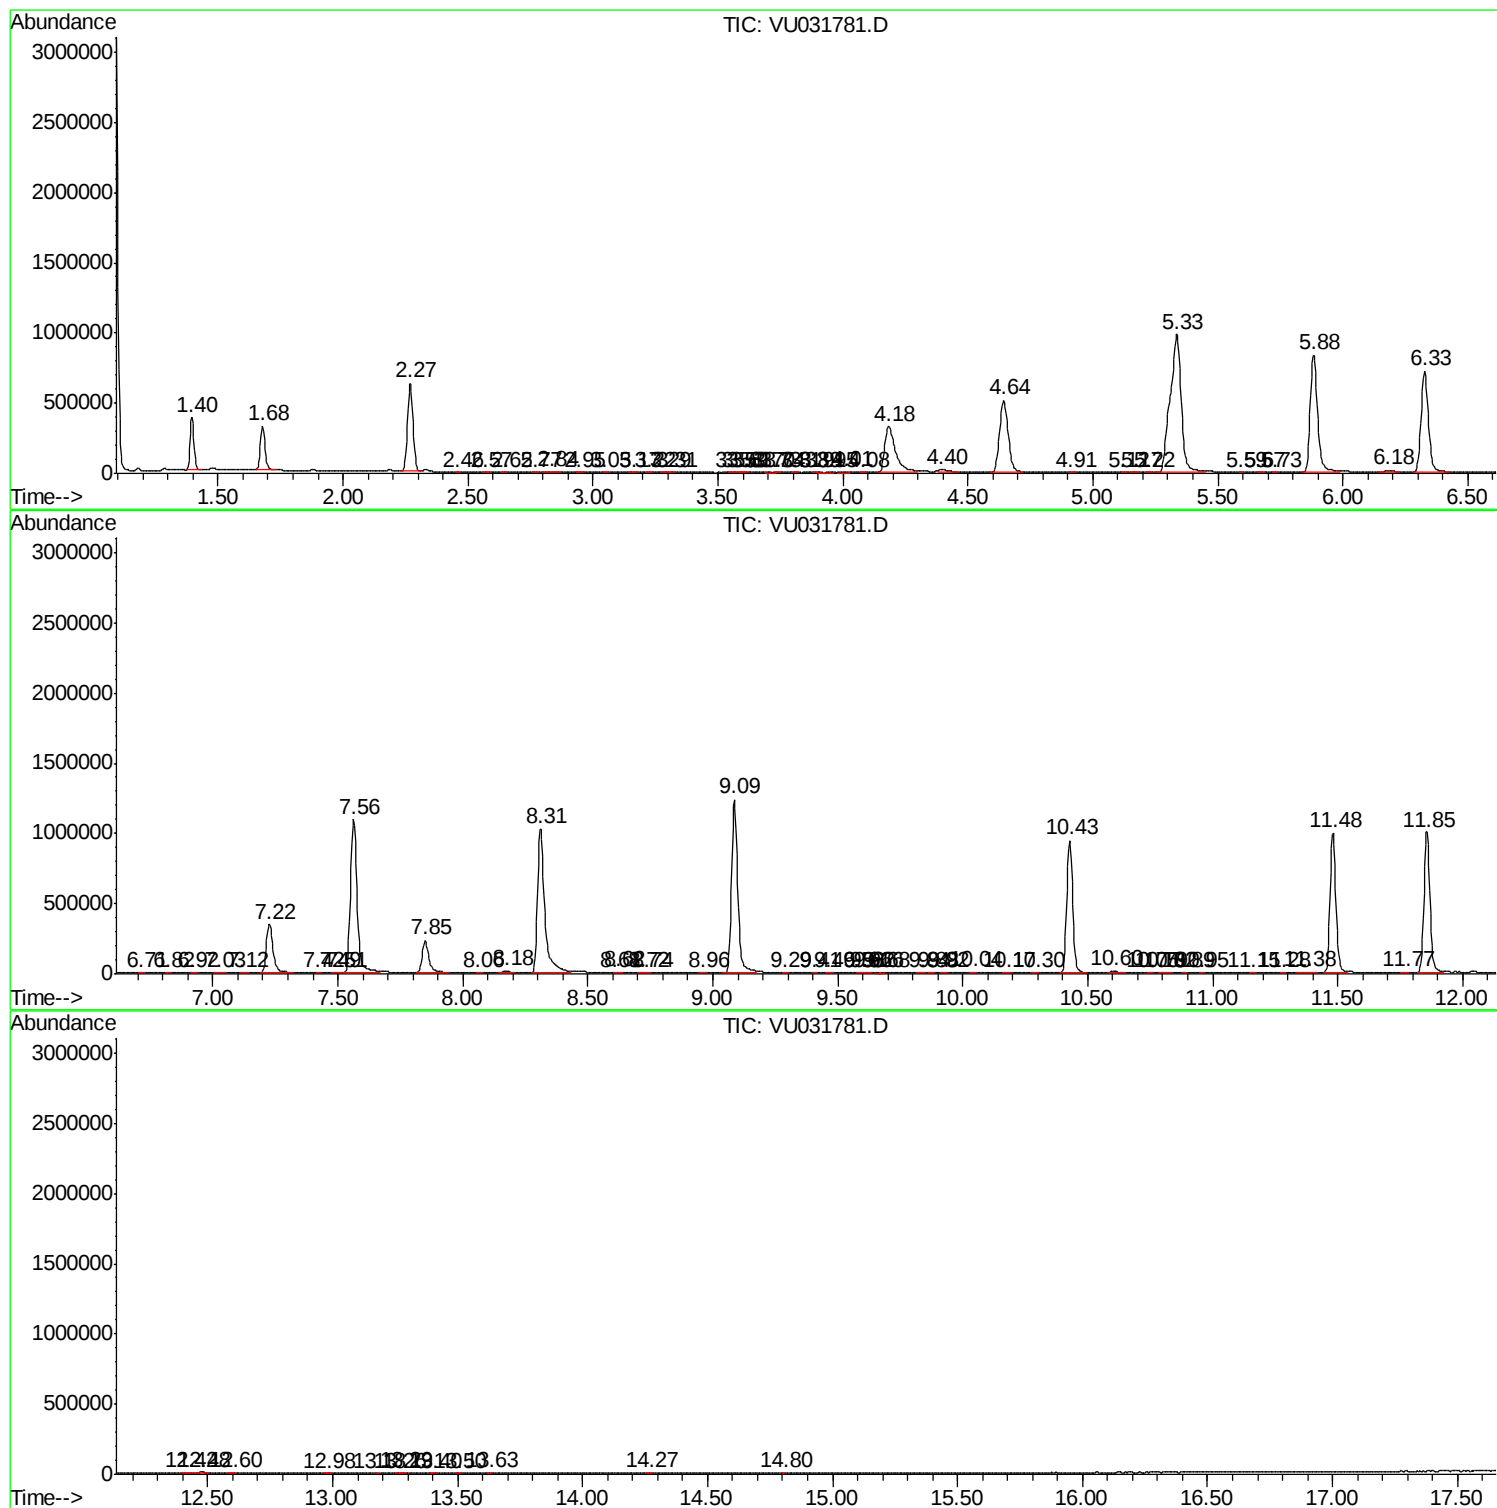

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU050619\
Data File : VU031781.D
Acq On : 06 May 2019 15:33
Operator : JC/SP
Sample : K2694-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFHF9

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU050619\
Data File : VU031781.D
Acq On : 06 May 2019 15:33
Operator : JC/SP
Sample : K2694-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFHF9

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc