

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050619\
 Data File : VU031788.D
 Acq On : 06 May 2019 18:39
 Operator : JC/SP
 Sample : VIBLK40
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK40

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	25	28	39	rVB4	15558	17171	0.58%	0.081%
2	1.395	88	95	105	rBV	364204	404096	13.56%	1.902%
3	1.675	175	182	195	rVB	327111	395532	13.27%	1.862%
4	2.267	356	366	381	rVB	633908	962447	32.29%	4.531%
5	2.453	420	424	426	rBV	1799	1491	0.05%	0.007%
6	2.630	475	479	481	rVV4	2042	1619	0.05%	0.008%
7	2.646	481	484	490	rVB4	2027	1567	0.05%	0.007%
8	2.698	498	500	503	rVB3	1958	1063	0.04%	0.005%
9	3.154	638	642	647	rVB2	1897	1744	0.06%	0.008%
10	3.183	647	651	653	rBV3	1427	1025	0.03%	0.005%
11	3.202	653	657	660	rVV3	1241	1005	0.03%	0.005%
12	3.225	662	664	668	rVB3	1069	836	0.03%	0.004%
13	3.247	668	671	674	rVB2	1501	720	0.02%	0.003%
14	3.302	684	688	690	rBV2	1211	1111	0.04%	0.005%
15	3.325	693	695	698	rVB3	1416	779	0.03%	0.004%
16	3.424	724	726	729	rBV2	1546	1215	0.04%	0.006%
17	3.482	742	744	750	rVB3	1186	933	0.03%	0.004%
18	3.524	753	757	763	rVB3	1416	1406	0.05%	0.007%
19	3.556	763	767	771	rBV2	1020	855	0.03%	0.004%
20	3.585	771	776	779	rVB3	1098	926	0.03%	0.004%
21	3.604	779	782	788	rBV3	1188	1170	0.04%	0.006%
22	3.640	788	793	796	rBV4	1117	1281	0.04%	0.006%
23	3.707	811	814	818	rVB2	1311	857	0.03%	0.004%
24	3.739	818	824	828	rBV6	1587	1751	0.06%	0.008%
25	3.800	837	843	847	rBV4	984	1030	0.03%	0.005%
26	3.829	847	852	855	rBV2	1185	1407	0.05%	0.007%
27	3.858	858	861	868	rVB5	802	815	0.03%	0.004%
28	3.942	881	887	888	rBV2	1449	1153	0.04%	0.005%
29	3.971	892	896	902	rVB5	1292	1486	0.05%	0.007%
30	4.009	902	908	909	rBV	1449	979	0.03%	0.005%
31	4.045	916	919	921	rBV	1229	905	0.03%	0.004%
32	4.093	928	934	940	rBV4	1139	1259	0.04%	0.006%
33	4.180	946	961	1000	rBV	321376	960515	32.22%	4.522%
34	4.488	1054	1057	1059	rBV2	1425	882	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050619\
 Data File : VU031788.D
 Acq On : 06 May 2019 18:39
 Operator : JC/SP
 Sample : VIBLK40
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK40

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	4.643	1087	1105	1125	rBV	505058	1199584	40.25%	5.647%
36	4.865	1170	1174	1177	rBV4	968	1013	0.03%	0.005%
37	5.106	1245	1249	1250	rBV2	1033	697	0.02%	0.003%
38	5.132	1255	1257	1259	rVV3	1905	1248	0.04%	0.006%
39	5.157	1263	1265	1270	rVB2	1403	814	0.03%	0.004%
40	5.193	1270	1276	1278	rBV3	1041	1048	0.04%	0.005%
41	5.334	1297	1320	1351	rBV2	970606	2980670	100.00%	14.032%
42	5.656	1417	1420	1422	rBV3	1046	719	0.02%	0.003%
43	5.742	1445	1447	1451	rVB3	1571	1108	0.04%	0.005%
44	5.884	1476	1491	1522	rBV	713217	1498528	50.27%	7.055%
45	6.112	1559	1562	1566	rVB3	2659	1745	0.06%	0.008%
46	6.183	1572	1584	1597	rBV9	23271	53719	1.80%	0.253%
47	6.328	1615	1629	1651	rBV	695279	1424983	47.81%	6.709%
48	6.591	1709	1711	1717	rVB5	2601	1988	0.07%	0.009%
49	6.771	1764	1767	1770	rVB3	1326	877	0.03%	0.004%
50	6.800	1770	1776	1781	rVB4	1690	1890	0.06%	0.009%
51	6.987	1830	1834	1836	rBV2	1402	990	0.03%	0.005%
52	7.099	1865	1869	1874	rVB5	1171	1018	0.03%	0.005%
53	7.225	1896	1908	1933	rBV	327922	626657	21.02%	2.950%
54	7.427	1967	1971	1975	rBV6	2100	1953	0.07%	0.009%
55	7.562	1997	2013	2047	rBV	1054376	1995046	66.93%	9.392%
56	7.848	2092	2102	2129	rBV	219331	407624	13.68%	1.919%
57	8.048	2161	2164	2166	rVB2	1940	1109	0.04%	0.005%
58	8.070	2166	2171	2173	rBV5	1809	1818	0.06%	0.009%
59	8.228	2210	2220	2233	rBV5	21774	41287	1.39%	0.194%
60	8.311	2235	2246	2283	rBV	980867	1960985	65.79%	9.232%
61	8.845	2409	2412	2416	rBV4	1308	1185	0.04%	0.006%
62	8.865	2416	2418	2425	rVB5	1354	1207	0.04%	0.006%
63	8.942	2438	2442	2446	rBV5	1370	1379	0.05%	0.006%
64	8.993	2456	2458	2461	rVB3	1749	900	0.03%	0.004%
65	9.016	2461	2465	2469	rBV5	1393	1065	0.04%	0.005%
66	9.086	2475	2487	2527	rBV	1039253	1840133	61.74%	8.663%
67	9.395	2581	2583	2587	rVB3	2126	1293	0.04%	0.006%
68	9.414	2587	2589	2594	rVB4	1340	776	0.03%	0.004%
69	9.598	2639	2646	2649	rBV4	2182	2769	0.09%	0.013%
70	9.652	2658	2663	2664	rBV4	1831	1580	0.05%	0.007%
71	9.684	2669	2673	2676	rBV	1296	1205	0.04%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050619\
 Data File : VU031788.D
 Acq On : 06 May 2019 18:39
 Operator : JC/SP
 Sample : VIBLK40
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK40

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	9.723	2683	2685	2692	rVB4	1717	1311	0.04%	0.006%
73	9.787	2698	2705	2707	rBV5	1998	2510	0.08%	0.012%
74	9.819	2713	2715	2718	rVB4	1969	1022	0.03%	0.005%
75	9.839	2718	2721	2726	rVB3	2773	2462	0.08%	0.012%
76	9.864	2726	2729	2731	rBV2	1376	946	0.03%	0.004%
77	9.884	2733	2735	2738	rVB2	2117	1131	0.04%	0.005%
78	9.909	2738	2743	2745	rBV3	1613	1588	0.05%	0.007%
79	10.016	2773	2776	2780	rVB3	1508	1084	0.04%	0.005%
80	10.096	2796	2801	2803	rBV2	1131	1121	0.04%	0.005%
81	10.366	2880	2885	2890	rBV2	1565	1680	0.06%	0.008%
82	10.427	2890	2904	2931	rVV	889072	1460632	49.00%	6.876%
83	10.601	2953	2958	2961	rBV4	3384	3008	0.10%	0.014%
84	10.672	2977	2980	2984	rBV4	1325	1036	0.03%	0.005%
85	10.794	3015	3018	3019	rBV2	1586	1049	0.04%	0.005%
86	10.900	3048	3051	3053	rBV	1416	867	0.03%	0.004%
87	11.028	3087	3091	3094	rBV3	1889	1424	0.05%	0.007%
88	11.044	3094	3096	3099	rBV3	1476	876	0.03%	0.004%
89	11.118	3117	3119	3121	rBV3	1261	776	0.03%	0.004%
90	11.289	3168	3172	3174	rBV3	1684	1397	0.05%	0.007%
91	11.340	3186	3188	3197	rBV4	1188	1059	0.04%	0.005%
92	11.482	3220	3232	3250	rBV	814833	1340554	44.97%	6.311%
93	11.858	3337	3349	3372	rBV	939767	1566527	52.56%	7.375%
94	12.604	3576	3581	3588	rBV5	2176	3184	0.11%	0.015%
95	12.636	3588	3591	3593	rBV2	1145	842	0.03%	0.004%
96	12.970	3688	3695	3698	rBV4	1858	2768	0.09%	0.013%
97	13.006	3702	3706	3711	rBV6	1486	2041	0.07%	0.010%
98	13.048	3716	3719	3721	rBV4	1569	1079	0.04%	0.005%
99	13.318	3800	3803	3805	rBV2	1364	697	0.02%	0.003%
100	13.388	3822	3825	3828	rVB2	1436	889	0.03%	0.004%


Sum of corrected areas: 21241201

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU050619\
Data File : VU031788.D
Acq On : 06 May 2019 18:39
Operator : JC/SP
Sample : VIBLK40
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK40

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

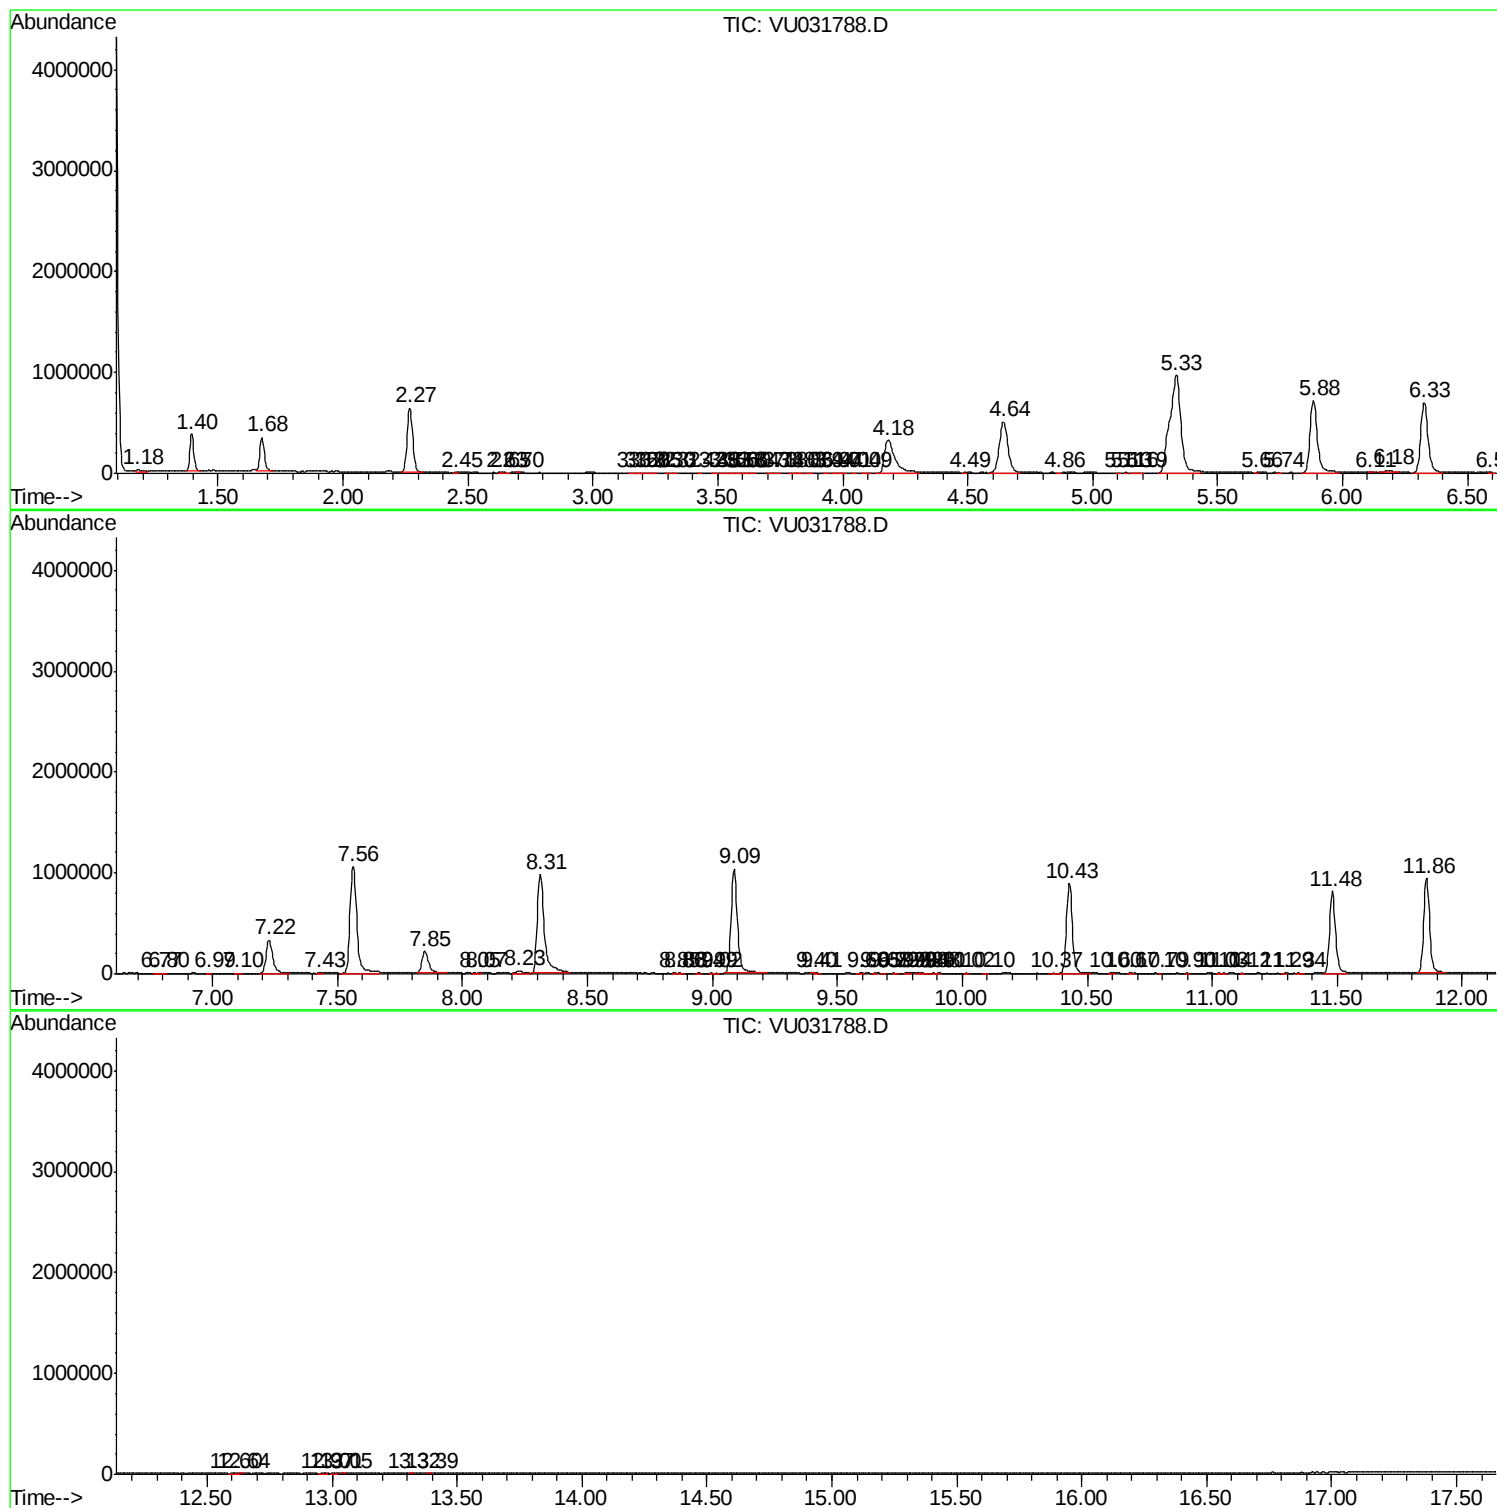

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU050619\
Data File : VU031788.D
Acq On : 06 May 2019 18:39
Operator : JC/SP
Sample : VIBLK40
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK40

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU050619\
Data File : VU031788.D
Acq On : 06 May 2019 18:39
Operator : JC/SP
Sample : VIBLK40
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK40

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc