


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050619\
 Data File : VU031763.D
 Acq On : 06 May 2019 08:25
 Operator : JC/SP
 Sample : BFB38
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB38

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis
 Last Update : Tue May 07 08:38:32 2019

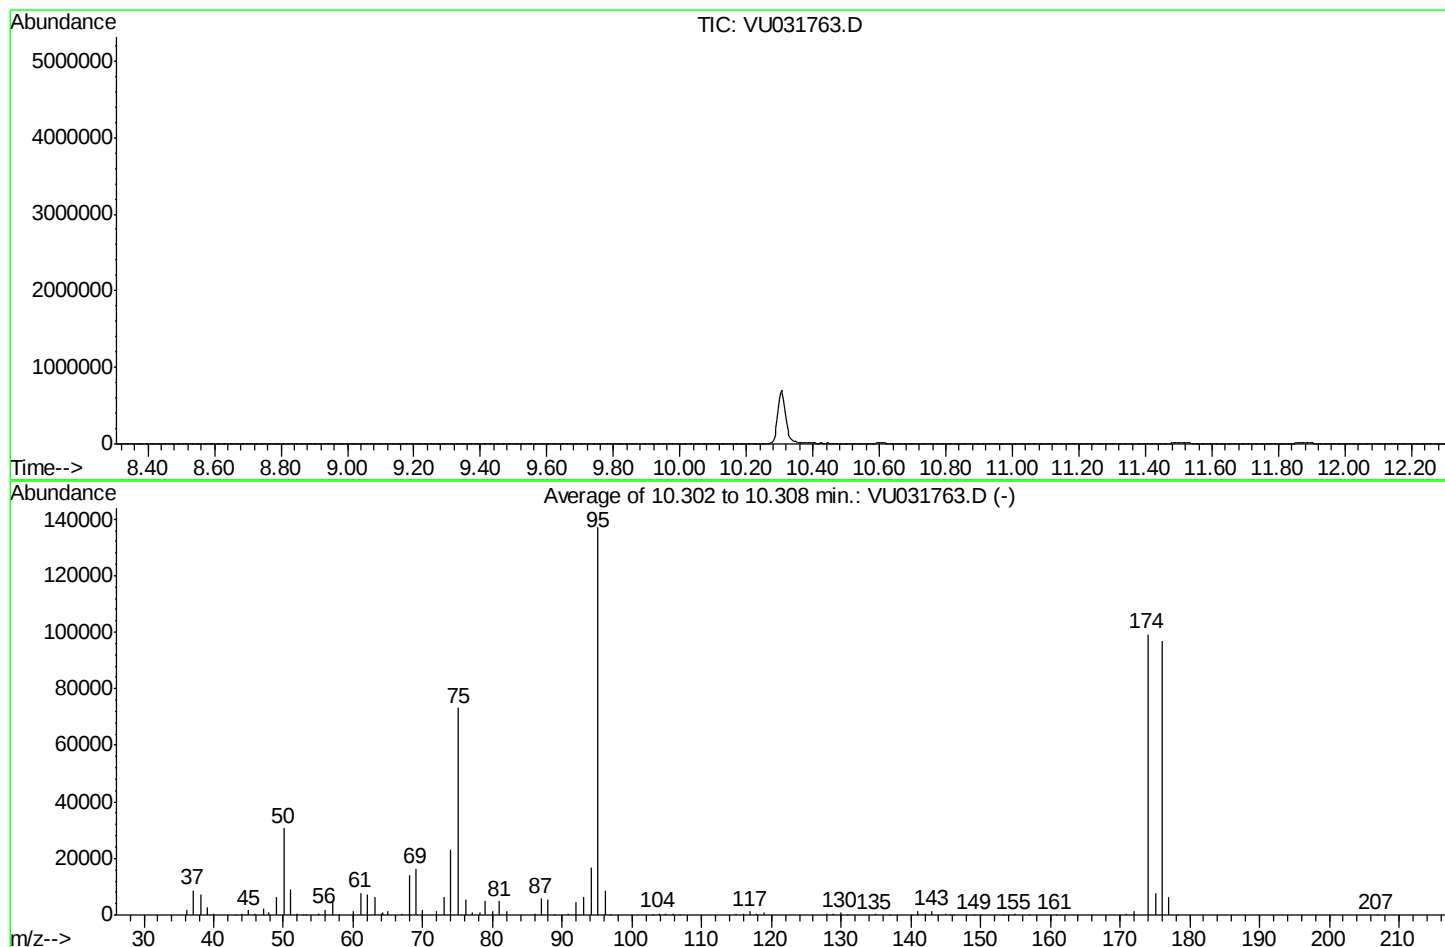

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2853

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.4	30682	PASS
75	95	30	80	53.5	73312	PASS
95	95	100	100	100.0	137088	PASS
96	95	5	9	6.2	8531	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	72.4	99232	PASS
175	174	5	9	7.6	7579	PASS
176	174	95	101	97.6	96858	PASS
177	176	5	9	6.6	6376	PASS

Scan 2853 (10.263 min): VU031763.D
BFB38

m/z	Abundance
39.00	106.0
40.00	4782.0
41.10	209.0
44.00	1233.0
77.30	163.0
78.20	187.0

Instrument :
MSVOA_U
ClientSampleId :
BFB38

m/z	Abundance
36.00	1828.0
37.00	8810.0
38.10	7624.0
39.00	3085.0
40.00	5395.0
41.10	104.0
43.20	146.0
44.10	1848.0
45.00	1680.0
45.90	340.0
47.10	2429.0
48.00	806.0
49.00	6396.0
50.10	30448.0
51.00	9164.0
52.00	574.0
52.90	235.0
55.00	393.0
55.90	1923.0
57.00	4521.0
57.90	163.0
60.00	1276.0
61.10	7875.0
62.00	7461.0
63.10	6280.0
64.00	788.0
64.20	790.0
65.10	1475.0
67.10	366.0
68.00	13611.0
69.00	15456.0
70.00	1582.0
72.00	1259.0
73.10	6606.0
74.00	23976.0
75.10	72608.0
76.10	5886.0
77.10	838.0
78.10	986.0
79.00	4807.0
80.00	1391.0
81.00	5055.0
81.90	1320.0
86.00	250.0
87.00	6106.0
88.00	5065.0
88.80	199.0
90.90	417.0
92.00	4655.0
93.00	5875.0
94.10	16416.0
95.10	134656.0
96.10	8913.0
96.90	105.0
103.00	128.0
103.90	643.0
104.80	210.0
105.90	584.0
106.90	190.0
115.00	265.0
116.00	616.0
116.90	1391.0
117.90	615.0
118.90	774.0
127.90	433.0
128.80	392.0
129.90	704.0
134.90	322.0
136.80	187.0
140.00	103.0
141.00	1337.0
142.10	203.0
143.00	1544.0
145.00	331.0
146.10	178.0
147.90	139.0
149.10	112.0
150.10	106.0
153.20	151.0
155.00	310.0
156.90	204.0
170.90	237.0
172.00	1348.0
174.00	95568.0
175.10	7855.0
176.00	93240.0
177.00	6355.0
178.10	325.0

Instrument :
MSVOA_U
ClientSampleId :
BFB38

m/z	Abundance
36.00	1828.0
37.00	9295.0
38.10	7562.0
39.00	3111.0
40.00	5259.0
41.10	126.0
43.00	113.0
44.10	1763.0
45.00	1759.0
46.00	355.0
47.10	2248.0
48.00	896.0
49.00	6599.0
50.10	31576.0
51.00	9281.0
52.00	553.0
52.90	142.0
55.00	490.0
55.90	1935.0
57.00	4700.0
57.90	197.0
60.00	1409.0
61.10	8114.0
62.00	7350.0
63.10	6634.0
64.20	923.0
65.10	1572.0
66.90	316.0
68.10	14512.0
69.00	17024.0
70.00	1679.0
72.00	1256.0
73.10	6757.0
74.10	23552.0
75.10	75240.0
76.10	5704.0
77.00	885.0
78.10	920.0
79.00	5060.0
80.00	1468.0
81.00	5090.0
82.00	1536.0
86.10	282.0
87.00	5925.0
88.00	5589.0
88.80	114.0
90.80	452.0
92.00	4537.0
93.00	6301.0
94.10	17264.0
95.10	141568.0
96.10	8695.0
103.00	146.0
103.80	722.0
104.70	280.0
105.90	724.0
106.90	160.0
115.00	275.0
116.00	585.0
116.90	1324.0
117.90	616.0
118.90	819.0
127.90	341.0
128.80	351.0
129.90	806.0
134.90	387.0
136.90	171.0
140.00	109.0
141.00	1373.0
142.10	289.0
143.00	1555.0
145.10	394.0
145.60	130.0
146.10	162.0
149.10	184.0
150.10	126.0
153.20	170.0
154.80	299.0
156.90	276.0
160.80	199.0
170.90	340.0
172.00	1312.0
174.00	102232.0
175.10	7816.0
176.00	100184.0
177.00	6596.0
178.20	184.0
206.80	132.0

Instrument :
MSVOA_U
ClientSampleId :
BFB38

m/z	Abundance
36.10	1565.0
37.00	8390.0
38.10	6841.0
39.10	2855.0
40.00	5018.0
41.10	133.0
43.00	184.0
44.00	1647.0
45.00	1748.0
46.00	318.0
47.10	1870.0
47.90	989.0
49.00	6254.0
50.10	30024.0
51.10	8783.0
52.00	458.0
53.20	105.0
55.00	459.0
56.00	1793.0
57.00	4402.0
57.90	173.0
60.00	1358.0
61.00	7572.0
62.10	6687.0
63.10	6227.0
64.20	864.0
65.00	1486.0
67.00	258.0
68.10	14608.0
69.00	16432.0
70.00	1561.0
72.00	1076.0
73.10	6137.0
74.10	21832.0
75.10	72088.0
76.10	5148.0
77.00	800.0
78.10	796.0
79.00	4977.0
80.00	1389.0
81.00	4533.0
82.00	1501.0
86.10	243.0
87.00	5296.0
88.00	5826.0
90.90	454.0
92.00	3967.0
93.00	6219.0
94.10	16156.0
95.10	135040.0
96.10	7985.0
97.00	120.0
103.00	103.0
103.80	706.0
104.70	290.0
105.90	674.0
106.70	125.0
114.90	224.0
116.00	438.0
117.00	1086.0
117.90	483.0
119.00	802.0
128.00	306.0
128.80	236.0
129.90	711.0
130.90	112.0
134.90	380.0
136.90	147.0
141.00	1247.0
142.10	296.0
143.00	1509.0
145.10	396.0
146.00	139.0
147.90	136.0
149.10	191.0
150.00	133.0
153.20	100.0
154.80	322.0
157.00	235.0
160.80	252.0
170.90	384.0
172.00	1205.0
174.00	99896.0
175.10	7066.0
176.00	97152.0
177.00	6178.0
178.20	128.0
206.80	152.0

Instrument :
MSVOA_U
ClientSampleId :
BFB38