

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050622\
 Data File : VU048466.D
 Acq On : 06 May 2022 19:41
 Operator : SY/MD
 Sample : N2710-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXLA1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M

Title : VOC Analysis

Signal : TIC: VU048466.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	40	45	51	rVV2	4866	5411	0.33%	0.046%
2	1.520	53	56	65	rVB2	3340	3925	0.24%	0.033%
3	1.601	73	81	102	rBV	194965	253839	15.40%	2.149%
4	1.900	165	174	185	rBV	123239	181481	11.01%	1.536%
5	2.565	368	381	398	rBV	350622	582513	35.34%	4.931%
6	2.732	430	433	435	rBV3	585	390	0.02%	0.003%
7	2.771	436	445	447	rBV3	3508	4515	0.27%	0.038%
8	2.874	474	477	480	rVB3	661	412	0.02%	0.003%
9	2.951	499	501	505	rBV	320	326	0.02%	0.003%
10	2.996	513	515	519	rVB3	531	315	0.02%	0.003%
11	3.044	525	530	540	rVB4	1329	2170	0.13%	0.018%
12	3.186	560	574	593	rVB	11184	25580	1.55%	0.217%
13	3.353	619	626	631	rBV4	1922	2841	0.17%	0.024%
14	3.440	650	653	657	rVB2	417	299	0.02%	0.003%
15	3.462	657	660	665	rBV2	311	328	0.02%	0.003%
16	3.546	683	686	693	rBV2	374	416	0.03%	0.004%
17	3.826	766	773	778	rBV	410	365	0.02%	0.003%
18	3.864	779	785	786	rBV2	369	330	0.02%	0.003%
19	4.620	1007	1020	1046	rBV	190667	460433	27.93%	3.898%
20	4.970	1126	1129	1132	rBV	649	457	0.03%	0.004%
21	5.063	1141	1158	1185	rBV	288406	631454	38.31%	5.345%
22	5.186	1194	1196	1201	rVB2	579	382	0.02%	0.003%
23	5.372	1251	1254	1256	rBV	543	393	0.02%	0.003%
24	5.391	1258	1260	1265	rVB3	976	762	0.05%	0.006%
25	5.526	1294	1302	1304	rVV3	940	961	0.06%	0.008%
26	5.726	1342	1364	1397	rBV2	612744	1648422	100.00%	13.954%
27	6.108	1480	1483	1489	rBV	396	395	0.02%	0.003%
28	6.250	1511	1527	1548	rBV	488717	932823	56.59%	7.896%
29	6.539	1608	1617	1626	rBV8	2377	4923	0.30%	0.042%
30	6.690	1648	1664	1683	rBV	382446	743556	45.11%	6.294%
31	7.105	1785	1793	1803	rVB2	1215	2010	0.12%	0.017%
32	7.176	1807	1815	1830	rVV9	3631	7388	0.45%	0.063%
33	7.565	1923	1936	1959	rBV	205668	358190	21.73%	3.032%
34	7.687	1970	1974	1979	rBV4	1442	1446	0.09%	0.012%
35	7.796	2000	2008	2018	rVB6	2232	3735	0.23%	0.032%
36	7.838	2018	2021	2025	rVB2	295	275	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050622\
 Data File : VU048466.D
 Acq On : 06 May 2022 19:41
 Operator : SY/MD
 Sample : N2710-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXLA1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

37	7.899	2025	2040	2056	rBV	719158	1247836	75.70%	10.563%
38	8.179	2114	2127	2149	rBV	143061	241413	14.65%	2.044%
39	8.398	2192	2195	2199	rBV4	714	500	0.03%	0.004%
40	8.459	2211	2214	2215	rBV2	520	307	0.02%	0.003%
41	8.555	2237	2244	2251	rVB5	3789	5377	0.33%	0.046%
42	8.636	2256	2269	2309	rBV2	544472	1032192	62.62%	8.737%
43	9.092	2408	2411	2416	rBV2	576	541	0.03%	0.005%
44	9.163	2429	2433	2436	rVB2	465	358	0.02%	0.003%
45	9.417	2499	2512	2529	rBV	683051	1142745	69.32%	9.673%
46	9.571	2553	2560	2572	rVB4	2349	3763	0.23%	0.032%
47	9.693	2591	2598	2612	rVB4	2706	4472	0.27%	0.038%
48	9.999	2687	2693	2696	rBV3	377	386	0.02%	0.003%
49	10.105	2717	2726	2743	rBV6	3064	6415	0.39%	0.054%
50	10.295	2780	2785	2789	rVB3	413	418	0.03%	0.004%
51	10.436	2823	2829	2832	rBV2	431	442	0.03%	0.004%
52	10.484	2835	2844	2853	rVB7	1923	3091	0.19%	0.026%
53	10.671	2895	2902	2909	rVB3	2367	3099	0.19%	0.026%
54	10.758	2915	2929	2945	rBV	439032	687450	41.70%	5.819%
55	10.867	2960	2963	2966	rBV3	537	413	0.03%	0.003%
56	10.944	2980	2987	2990	rBV2	266	366	0.02%	0.003%
57	11.086	3027	3031	3038	rBV2	842	1289	0.08%	0.011%
58	11.121	3039	3042	3047	rVB4	756	645	0.04%	0.005%
59	11.330	3102	3107	3112	rVB2	440	413	0.03%	0.003%
60	11.359	3112	3116	3122	rBV2	470	517	0.03%	0.004%
61	11.398	3122	3128	3130	rBV2	303	290	0.02%	0.002%
62	11.465	3140	3149	3150	rBV4	2463	2500	0.15%	0.021%
63	11.578	3180	3184	3190	rVB2	681	554	0.03%	0.005%
64	11.603	3190	3192	3199	rVB2	252	277	0.02%	0.002%
65	11.648	3199	3206	3209	rBV2	469	392	0.02%	0.003%
66	11.700	3215	3222	3224	rBV3	596	602	0.04%	0.005%
67	11.751	3228	3238	3244	rBV4	2128	3384	0.21%	0.029%
68	11.812	3244	3257	3277	rBV	456919	725124	43.99%	6.138%
69	11.970	3303	3306	3313	rVB4	1024	979	0.06%	0.008%
70	12.028	3320	3324	3331	rBV	349	302	0.02%	0.003%
71	12.192	3361	3375	3395	rBV	456940	750194	45.51%	6.350%
72	12.272	3395	3400	3402	rBV2	574	436	0.03%	0.004%
73	12.336	3416	3420	3425	rVB3	610	630	0.04%	0.005%
74	12.404	3437	3441	3444	rVB	437	350	0.02%	0.003%
75	12.430	3444	3449	3455	rVB2	347	433	0.03%	0.004%
76	12.471	3459	3462	3464	rBV2	458	324	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050622\
 Data File : VU048466.D
 Acq On : 06 May 2022 19:41
 Operator : SY/MD
 Sample : N2710-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXLA1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

77	12.610	3502	3505	3507	rBV	415	309	0.02%	0.003%
78	12.680	3524	3527	3535	rVB2	433	443	0.03%	0.004%
79	12.725	3535	3541	3545	rBV2	410	436	0.03%	0.004%
80	12.748	3545	3548	3551	rBV	418	278	0.02%	0.002%
81	12.770	3551	3555	3558	rVV3	549	422	0.03%	0.004%
82	12.803	3561	3565	3570	rBV3	393	375	0.02%	0.003%
83	12.951	3608	3611	3614	rVB2	521	347	0.02%	0.003%
84	12.979	3617	3620	3622	rVV	417	307	0.02%	0.003%
85	13.002	3625	3627	3633	rVV2	934	753	0.05%	0.006%
86	13.034	3633	3637	3639	rVV3	389	328	0.02%	0.003%
87	13.050	3640	3642	3646	rVV2	542	411	0.02%	0.003%
88	13.073	3646	3649	3652	rVV2	563	421	0.03%	0.004%
89	13.147	3669	3672	3674	rVV2	581	399	0.02%	0.003%
90	13.172	3678	3680	3688	rVV2	605	555	0.03%	0.005%
91	13.224	3690	3696	3705	rVB6	3035	4627	0.28%	0.039%
92	13.375	3738	3743	3744	rBV	540	433	0.03%	0.004%
93	13.446	3762	3765	3769	rVB3	483	325	0.02%	0.003%
94	13.478	3769	3775	3781	rBV2	625	709	0.04%	0.006%
95	13.799	3869	3875	3877	rBV2	613	614	0.04%	0.005%
96	13.844	3880	3889	3901	rVV5	9168	14268	0.87%	0.121%
97	14.063	3953	3957	3958	rBV2	791	538	0.03%	0.005%
98	14.092	3958	3966	3983	rVB2	20597	34464	2.09%	0.292%
99	14.333	4032	4041	4049	rBV3	10279	16709	1.01%	0.141%
100	14.475	4083	4085	4088	rVB3	644	316	0.02%	0.003%




Sum of corrected areas: 11813467

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050622\
Data File : VU048466.D
Acq On : 06 May 2022 19:41
Operator : SY/MD
Sample : N2710-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXLA1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

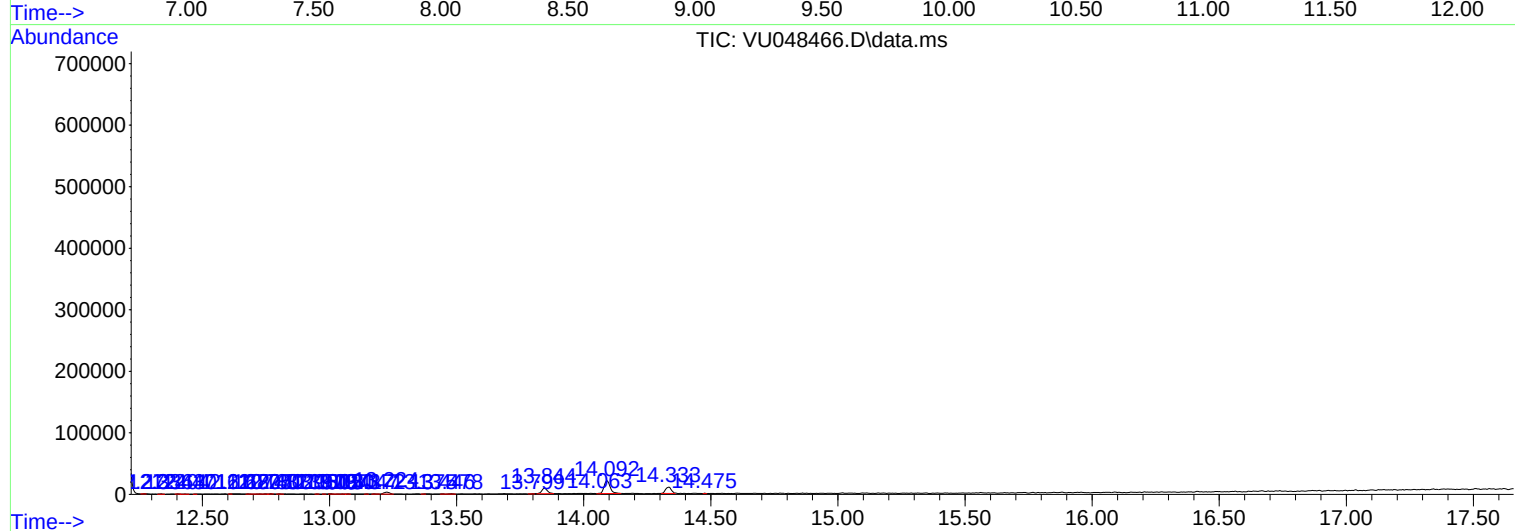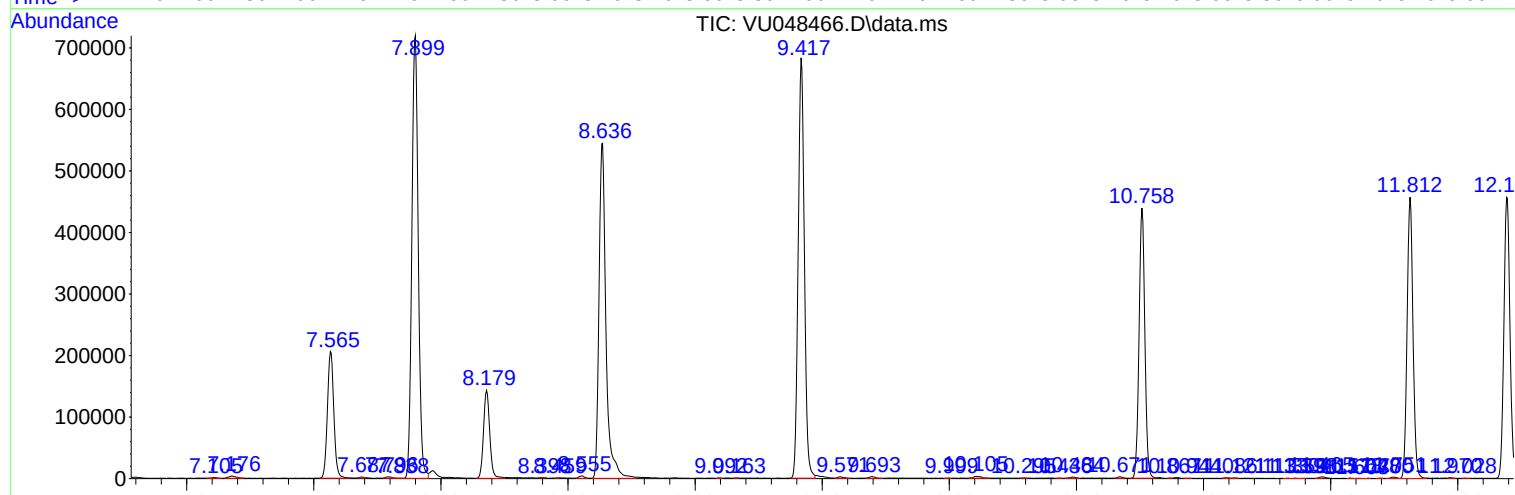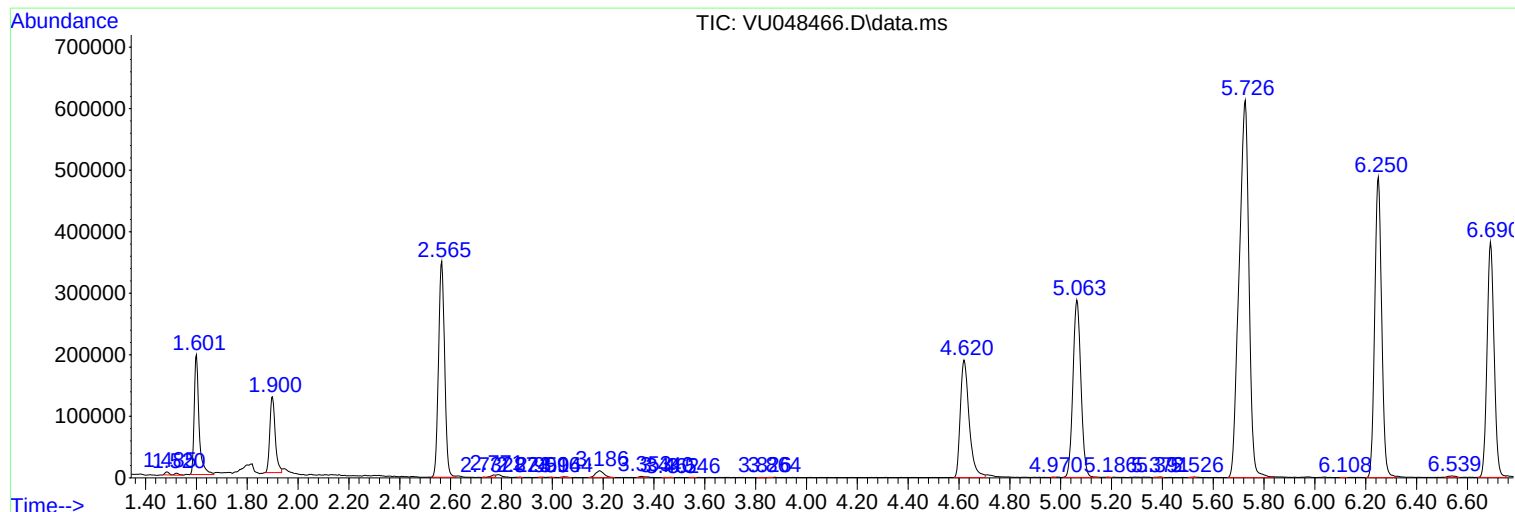

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050622\
Data File : VU048466.D
Acq On : 06 May 2022 19:41
Operator : SY/MD
Sample : N2710-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXLA1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050622\
Data File : VU048466.D
Acq On : 06 May 2022 19:41
Operator : SY/MD
Sample : N2710-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXLA1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------