

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050622\
 Data File : VU048467.D
 Acq On : 06 May 2022 20:05
 Operator : SY/MD
 Sample : N2710-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXLA2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

Signal : TIC: VU048467.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	100	rVB	183430	239435	14.26%	1.941%
2	1.906	169	176	200	rVB	134573	204316	12.17%	1.656%
3	2.565	368	381	401	rBV	362049	594422	35.39%	4.819%
4	3.025	520	524	527	rBV2	401	280	0.02%	0.002%
5	3.044	527	530	531	rBV	557	284	0.02%	0.002%
6	3.115	547	552	553	rBV	344	187	0.01%	0.002%
7	3.195	559	577	584	rBV4	4500	10957	0.65%	0.089%
8	3.350	621	625	628	rBV2	625	516	0.03%	0.004%
9	3.414	642	645	647	rBV	313	181	0.01%	0.001%
10	3.452	654	657	660	rVB2	328	205	0.01%	0.002%
11	3.475	660	664	669	rVB2	373	275	0.02%	0.002%
12	3.501	669	672	678	rBV2	327	360	0.02%	0.003%
13	3.533	678	682	685	rBV	426	316	0.02%	0.003%
14	3.642	711	716	718	rBV2	206	198	0.01%	0.002%
15	3.674	724	726	728	rVB	256	104	0.01%	0.001%
16	3.713	734	738	742	rVB2	383	287	0.02%	0.002%
17	3.739	742	746	749	rBV2	225	188	0.01%	0.002%
18	3.796	761	764	768	rVB2	269	205	0.01%	0.002%
19	3.912	797	800	805	rVB	261	207	0.01%	0.002%
20	3.941	805	809	812	rBV2	171	108	0.01%	0.001%
21	3.967	814	817	821	rBV	285	206	0.01%	0.002%
22	4.057	840	845	848	rBV2	176	150	0.01%	0.001%
23	4.128	862	867	870	rBV2	322	262	0.02%	0.002%
24	4.147	870	873	874	rBV	158	86	0.01%	0.001%
25	4.214	890	894	898	rBV2	242	205	0.01%	0.002%
26	4.276	911	913	916	rBV2	247	175	0.01%	0.001%
27	4.317	922	926	930	rBV2	299	247	0.01%	0.002%
28	4.401	949	952	957	rVB2	294	233	0.01%	0.002%
29	4.443	963	965	968	rVB	199	90	0.01%	0.001%
30	4.536	991	994	996	rBV3	165	103	0.01%	0.001%
31	4.565	1002	1003	1006	rBV	208	102	0.01%	0.001%
32	4.629	1009	1023	1062	rBV	185990	486526	28.97%	3.944%
33	5.063	1141	1158	1180	rBV	298933	652662	38.86%	5.291%
34	5.295	1222	1230	1232	rBV4	698	1000	0.06%	0.008%
35	5.340	1242	1244	1247	rVV	232	120	0.01%	0.001%
36	5.369	1250	1253	1256	rBV	249	124	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050622\
 Data File : VU048467.D
 Acq On : 06 May 2022 20:05
 Operator : SY/MD
 Sample : N2710-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXLA2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

37	5.398	1259	1262	1263	rBV	254	147	0.01%	0.001%
38	5.407	1263	1265	1268	rVB2	324	106	0.01%	0.001%
39	5.462	1276	1282	1287	rBV3	228	226	0.01%	0.002%
40	5.523	1299	1301	1304	rVB	308	138	0.01%	0.001%
41	5.626	1330	1333	1335	rVB2	165	91	0.01%	0.001%
42	5.642	1335	1338	1341	rVB	204	126	0.01%	0.001%
43	5.726	1341	1364	1390	rBV2	625657	1679396	100.00%	13.614%
44	5.970	1436	1440	1443	rBV3	689	656	0.04%	0.005%
45	6.041	1456	1462	1464	rBV3	586	564	0.03%	0.005%
46	6.166	1498	1501	1507	rVB	390	283	0.02%	0.002%
47	6.250	1512	1527	1553	rBV	472284	902904	53.76%	7.319%
48	6.507	1602	1607	1608	rBV2	339	233	0.01%	0.002%
49	6.536	1608	1616	1625	rVV6	2245	3633	0.22%	0.029%
50	6.632	1642	1646	1649	rVB3	428	290	0.02%	0.002%
51	6.690	1649	1664	1685	rBV	383165	758455	45.16%	6.148%
52	6.861	1715	1717	1720	rBV2	170	107	0.01%	0.001%
53	7.044	1770	1774	1775	rBV2	371	225	0.01%	0.002%
54	7.089	1785	1788	1793	rVB2	378	303	0.02%	0.002%
55	7.153	1802	1808	1810	rBV2	303	274	0.02%	0.002%
56	7.185	1810	1818	1825	rBV5	3548	5703	0.34%	0.046%
57	7.240	1833	1835	1836	rBV5	276	111	0.01%	0.001%
58	7.295	1849	1852	1855	rBV2	300	169	0.01%	0.001%
59	7.382	1876	1879	1882	rBV2	196	131	0.01%	0.001%
60	7.452	1898	1901	1903	rBV	229	124	0.01%	0.001%
61	7.517	1918	1921	1922	rBV	352	200	0.01%	0.002%
62	7.565	1924	1936	1958	rVV	201172	356347	21.22%	2.889%
63	7.748	1991	1993	1997	rBV2	189	111	0.01%	0.001%
64	7.771	1998	2000	2003	rBV3	384	167	0.01%	0.001%
65	7.793	2005	2007	2009	rBV2	636	322	0.02%	0.003%
66	7.899	2025	2040	2057	rBV	729539	1268255	75.52%	10.281%
67	8.179	2114	2127	2143	rBV	138063	239069	14.24%	1.938%
68	8.433	2203	2206	2208	rBV3	390	237	0.01%	0.002%
69	8.507	2227	2229	2232	rBV2	314	259	0.02%	0.002%
70	8.552	2232	2243	2256	rVB3	27204	46805	2.79%	0.379%
71	8.636	2256	2269	2298	rBV2	550178	1039255	61.88%	8.425%
72	8.873	2340	2343	2347	rBV2	576	462	0.03%	0.004%
73	8.970	2371	2373	2379	rVB2	351	218	0.01%	0.002%
74	9.021	2387	2389	2390	rBV	325	124	0.01%	0.001%
75	9.060	2397	2401	2405	rBV3	517	409	0.02%	0.003%
76	9.156	2426	2431	2437	rBV4	869	944	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050622\
 Data File : VU048467.D
 Acq On : 06 May 2022 20:05
 Operator : SY/MD
 Sample : N2710-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXLA2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

77	9.201	2443	2445	2449	rBV2	236	172	0.01%	0.001%
78	9.417	2499	2512	2536	rBV	637060	1071722	63.82%	8.688%
79	9.574	2558	2561	2567	rVB3	1159	1117	0.07%	0.009%
80	9.645	2579	2583	2588	rBV	576	612	0.04%	0.005%
81	9.735	2609	2611	2612	rBV	256	121	0.01%	0.001%
82	9.764	2617	2620	2624	rVB3	309	235	0.01%	0.002%
83	9.928	2669	2671	2674	rVB2	226	134	0.01%	0.001%
84	9.960	2678	2681	2685	rVB2	402	260	0.02%	0.002%
85	10.098	2718	2724	2726	rBV2	787	767	0.05%	0.006%
86	10.343	2797	2800	2802	rBV	232	113	0.01%	0.001%
87	10.635	2886	2891	2895	rBV2	385	472	0.03%	0.004%
88	10.671	2898	2902	2910	rVB5	2704	3260	0.19%	0.026%
89	10.758	2916	2929	2947	rBV	515231	842660	50.18%	6.831%
90	10.864	2956	2962	2964	rBV2	546	626	0.04%	0.005%
91	11.089	3027	3032	3035	rBV2	675	654	0.04%	0.005%
92	11.150	3049	3051	3054	rVB2	375	145	0.01%	0.001%
93	11.208	3064	3069	3070	rBV	402	317	0.02%	0.003%
94	11.301	3094	3098	3102	rBV	458	439	0.03%	0.004%
95	11.690	3216	3219	3228	rBV4	1149	1333	0.08%	0.011%
96	11.748	3231	3237	3241	rBV4	1535	1792	0.11%	0.015%
97	11.812	3245	3257	3274	rBV	570079	904271	53.85%	7.330%
98	12.195	3362	3376	3394	rBV	598214	985686	58.69%	7.990%
99	12.825	3570	3572	3574	rBV	273	149	0.01%	0.001%
100	14.092	3958	3966	3974	rBV2	10491	15781	0.94%	0.128%




Sum of corrected areas: 12335739

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050622\
Data File : VU048467.D
Acq On : 06 May 2022 20:05
Operator : SY/MD
Sample : N2710-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXLA2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

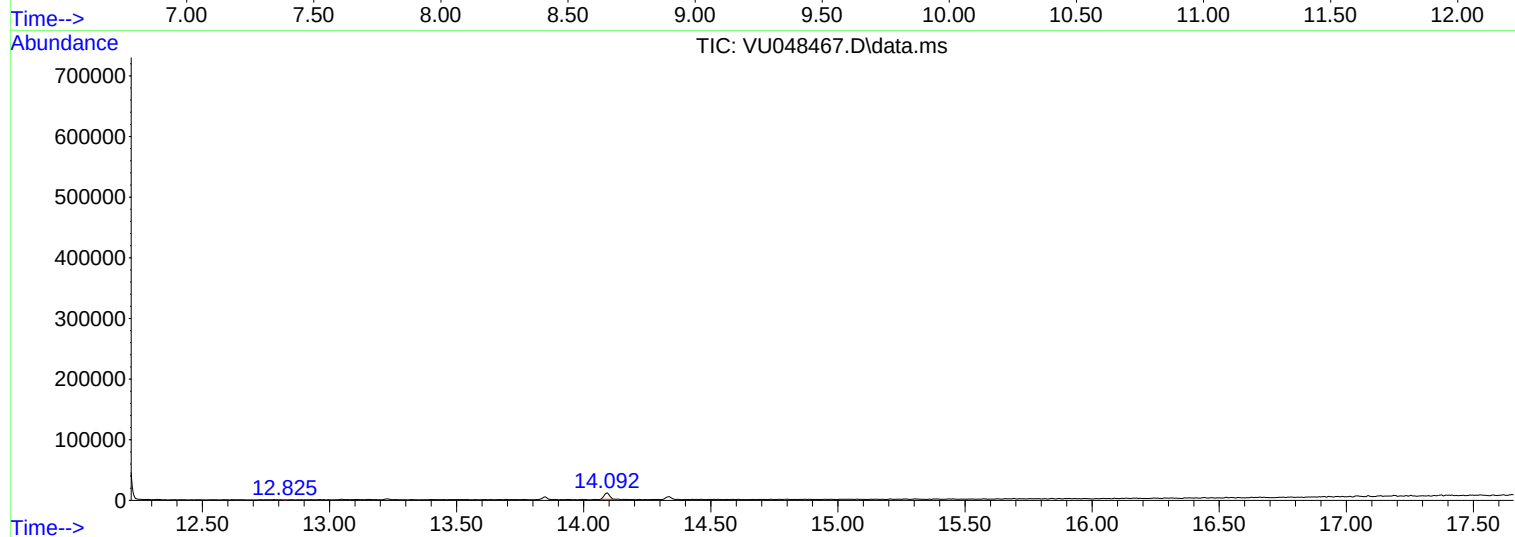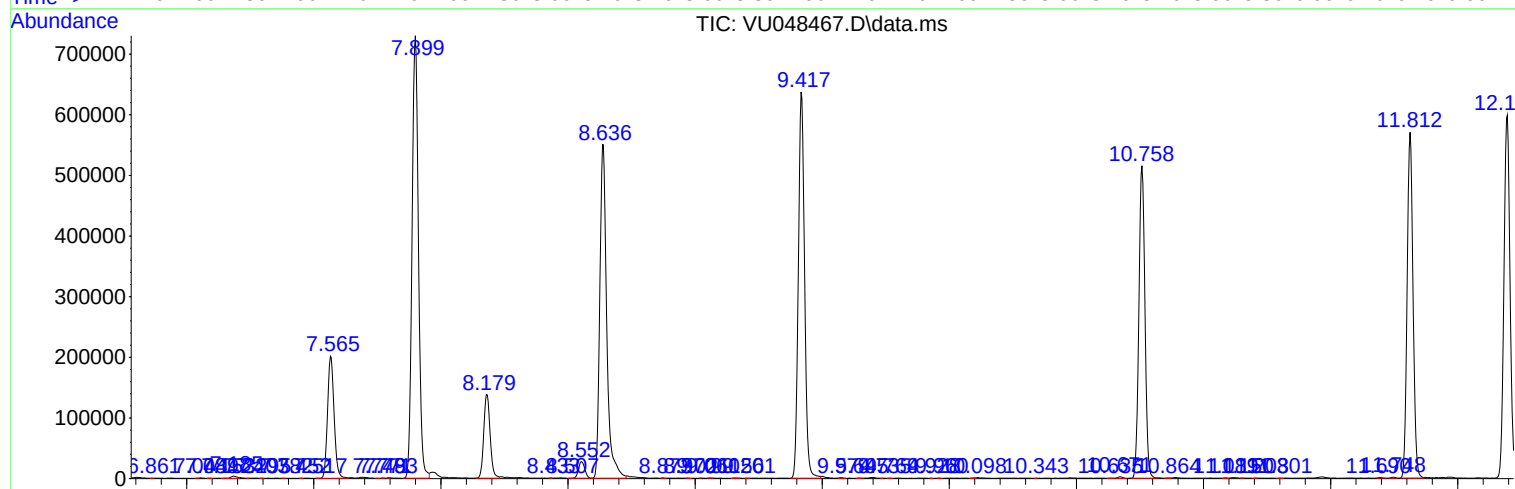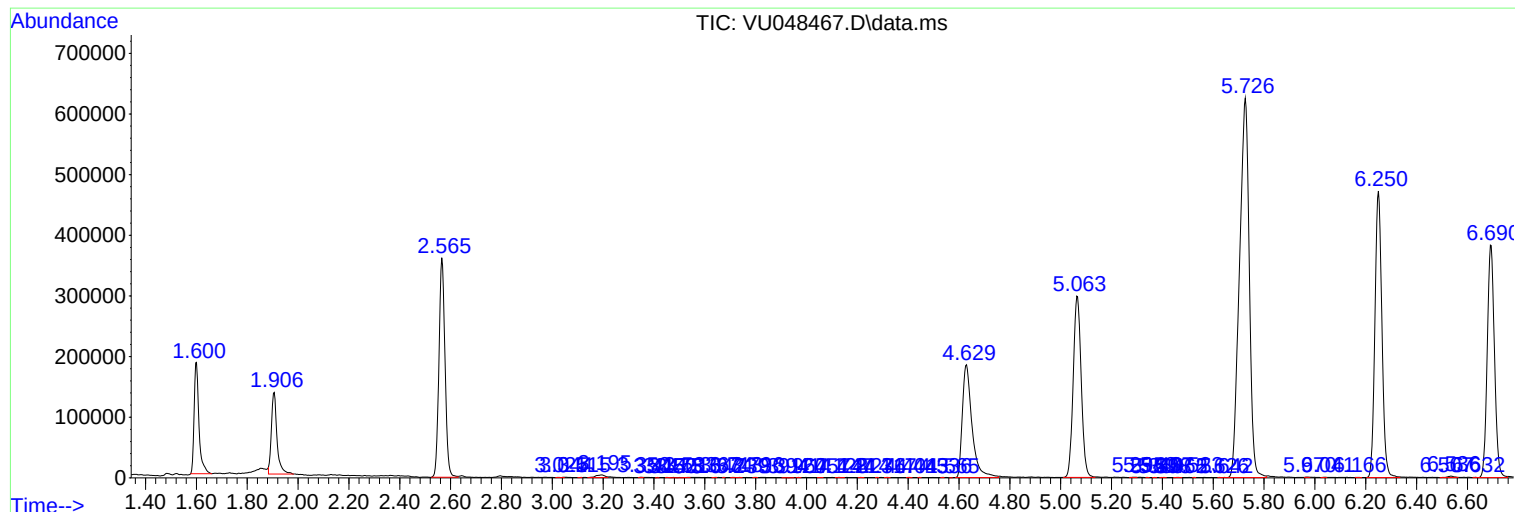

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050622\
Data File : VU048467.D
Acq On : 06 May 2022 20:05
Operator : SY/MD
Sample : N2710-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXLA2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050622\
Data File : VU048467.D
Acq On : 06 May 2022 20:05
Operator : SY/MD
Sample : N2710-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXLA2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc