

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050622\
 Data File : VU048468.D
 Acq On : 06 May 2022 20:29
 Operator : SY/MD
 Sample : N2710-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXLA3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

Signal : TIC: VU048468.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	103	rBV	183756	242170	14.64%	1.932%
2	1.906	170	176	201	rVB	132766	194855	11.78%	1.555%
3	2.408	326	332	334	rBV4	867	802	0.05%	0.006%
4	2.565	368	381	400	rBV	352656	585050	35.38%	4.668%
5	2.697	420	422	425	rBV	367	209	0.01%	0.002%
6	2.774	443	446	447	rBV2	427	216	0.01%	0.002%
7	3.044	527	530	534	rBV3	860	699	0.04%	0.006%
8	3.099	545	547	551	rVB2	493	230	0.01%	0.002%
9	3.186	562	574	590	rBV3	3722	9097	0.55%	0.073%
10	3.266	596	599	602	rBV	326	236	0.01%	0.002%
11	3.308	605	612	614	rBV	313	389	0.02%	0.003%
12	3.417	645	646	650	rBV2	184	124	0.01%	0.001%
13	3.514	674	676	680	rVB2	218	124	0.01%	0.001%
14	3.565	688	692	693	rBV	290	156	0.01%	0.001%
15	3.610	704	706	707	rBV	287	108	0.01%	0.001%
16	3.674	723	726	728	rBV2	201	100	0.01%	0.001%
17	3.735	743	745	747	rBV	141	74	0.00%	0.001%
18	3.748	747	749	754	rBV	226	203	0.01%	0.002%
19	3.829	770	774	777	rBV	196	176	0.01%	0.001%
20	3.864	782	785	789	rVB2	189	136	0.01%	0.001%
21	3.883	789	791	794	rBV2	406	196	0.01%	0.002%
22	4.018	831	833	835	rVB2	245	100	0.01%	0.001%
23	4.092	854	856	859	rBV	149	67	0.00%	0.001%
24	4.108	859	861	862	rVB	131	50	0.00%	0.000%
25	4.121	862	865	866	rBV	122	61	0.00%	0.000%
26	4.137	866	870	872	rVB	298	211	0.01%	0.002%
27	4.160	872	877	880	rBV	304	291	0.02%	0.002%
28	4.292	914	918	922	rBV2	415	372	0.02%	0.003%
29	4.359	934	939	942	rBV2	257	297	0.02%	0.002%
30	4.382	942	946	949	rVV2	292	244	0.01%	0.002%
31	4.427	957	960	962	rBV2	185	117	0.01%	0.001%
32	4.443	962	965	969	rVV2	191	182	0.01%	0.001%
33	4.530	988	992	995	rBV2	411	335	0.02%	0.003%
34	4.629	1008	1023	1062	rBV	185310	494627	29.91%	3.947%
35	5.067	1142	1159	1177	rBV	292000	643071	38.89%	5.131%
36	5.269	1221	1222	1225	rBV	239	132	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050622\
 Data File : VU048468.D
 Acq On : 06 May 2022 20:29
 Operator : SY/MD
 Sample : N2710-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXLA3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

37	5.337	1241	1243	1246	rVB	459	159	0.01%	0.001%
38	5.356	1246	1249	1252	rBV	323	168	0.01%	0.001%
39	5.411	1264	1266	1268	rBV	223	85	0.01%	0.001%
40	5.449	1276	1278	1279	rBV	136	43	0.00%	0.000%
41	5.497	1289	1293	1295	rBV2	248	229	0.01%	0.002%
42	5.533	1301	1304	1306	rBV	201	96	0.01%	0.001%
43	5.562	1311	1313	1318	rBV2	245	183	0.01%	0.001%
44	5.726	1342	1364	1385	rBV2	618130	1653621	100.00%	13.195%
45	6.038	1458	1461	1464	rBV2	651	549	0.03%	0.004%
46	6.108	1480	1483	1486	rBV2	526	294	0.02%	0.002%
47	6.147	1491	1495	1498	rBV3	607	476	0.03%	0.004%
48	6.250	1513	1527	1555	rBV	503138	951151	57.52%	7.590%
49	6.530	1608	1614	1616	rBV2	1669	1603	0.10%	0.013%
50	6.690	1649	1664	1686	rBV	376520	746620	45.15%	5.958%
51	6.970	1748	1751	1752	rBV2	107	60	0.00%	0.000%
52	7.079	1783	1785	1788	rBV	293	203	0.01%	0.002%
53	7.185	1810	1818	1819	rBV4	2641	2864	0.17%	0.023%
54	7.253	1836	1839	1841	rBV	273	185	0.01%	0.001%
55	7.298	1851	1853	1854	rBV	165	54	0.00%	0.000%
56	7.507	1915	1918	1920	rBV2	246	185	0.01%	0.001%
57	7.565	1924	1936	1959	rVV	198229	350196	21.18%	2.794%
58	7.832	2016	2019	2022	rVB2	354	245	0.01%	0.002%
59	7.899	2026	2040	2056	rBV	713393	1247976	75.47%	9.958%
60	8.179	2115	2127	2156	rBV	135802	239111	14.46%	1.908%
61	8.452	2207	2212	2213	rBV2	458	363	0.02%	0.003%
62	8.501	2225	2227	2230	rBV2	283	136	0.01%	0.001%
63	8.552	2232	2243	2258	rBV	109085	187224	11.32%	1.494%
64	8.639	2258	2270	2305	rBV2	545833	1046018	63.26%	8.347%
65	8.861	2335	2339	2341	rBV2	473	362	0.02%	0.003%
66	8.954	2366	2368	2370	rBV	165	77	0.00%	0.001%
67	8.980	2372	2376	2377	rBV2	521	383	0.02%	0.003%
68	9.002	2381	2383	2385	rVB3	366	169	0.01%	0.001%
69	9.034	2390	2393	2394	rBV3	458	218	0.01%	0.002%
70	9.066	2401	2403	2405	rBV	345	202	0.01%	0.002%
71	9.137	2422	2425	2427	rBV	390	190	0.01%	0.002%
72	9.192	2441	2442	2443	rBV	241	62	0.00%	0.000%
73	9.224	2450	2452	2454	rBV2	191	107	0.01%	0.001%
74	9.259	2460	2463	2467	rBV2	350	324	0.02%	0.003%
75	9.417	2499	2512	2536	rBV	668626	1138494	68.85%	9.084%
76	9.642	2578	2582	2584	rBV2	438	378	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050622\
 Data File : VU048468.D
 Acq On : 06 May 2022 20:29
 Operator : SY/MD
 Sample : N2710-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXLA3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

77	9.780	2622	2625	2629	rVB2	401	276	0.02%	0.002%
78	9.825	2637	2639	2643	rBV2	288	224	0.01%	0.002%
79	9.880	2653	2656	2659	rBV	335	263	0.02%	0.002%
80	10.291	2781	2784	2787	rBV2	299	212	0.01%	0.002%
81	10.359	2800	2805	2807	rBV2	385	288	0.02%	0.002%
82	10.671	2892	2902	2912	rBV4	2407	3894	0.24%	0.031%
83	10.758	2917	2929	2955	rVB	520097	836244	50.57%	6.673%
84	10.973	2991	2996	2999	rBV3	587	552	0.03%	0.004%
85	11.185	3059	3062	3063	rBV	380	213	0.01%	0.002%
86	11.362	3115	3117	3118	rBV	213	68	0.00%	0.001%
87	11.520	3164	3166	3169	rVB	391	170	0.01%	0.001%
88	11.578	3182	3184	3186	rBV2	287	143	0.01%	0.001%
89	11.812	3244	3257	3279	rBV	604674	956355	57.83%	7.631%
90	12.073	3336	3338	3341	rBV	400	238	0.01%	0.002%
91	12.195	3361	3376	3394	rBV	598753	978060	59.15%	7.804%
92	13.626	3818	3821	3824	rBV2	573	420	0.03%	0.003%
93	13.690	3840	3841	3845	rBV	473	344	0.02%	0.003%
94	14.092	3960	3966	3979	rBV3	5201	7859	0.48%	0.063%




Sum of corrected areas: 12532393

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050622\
Data File : VU048468.D
Acq On : 06 May 2022 20:29
Operator : SY/MD
Sample : N2710-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXLA3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

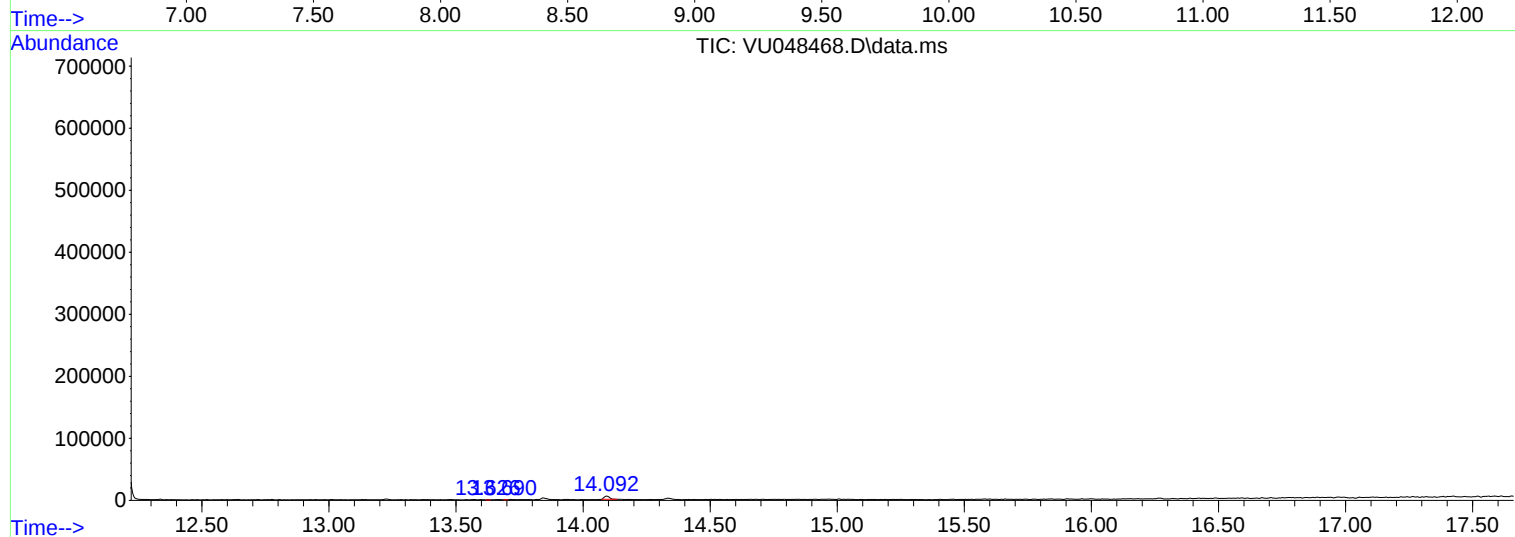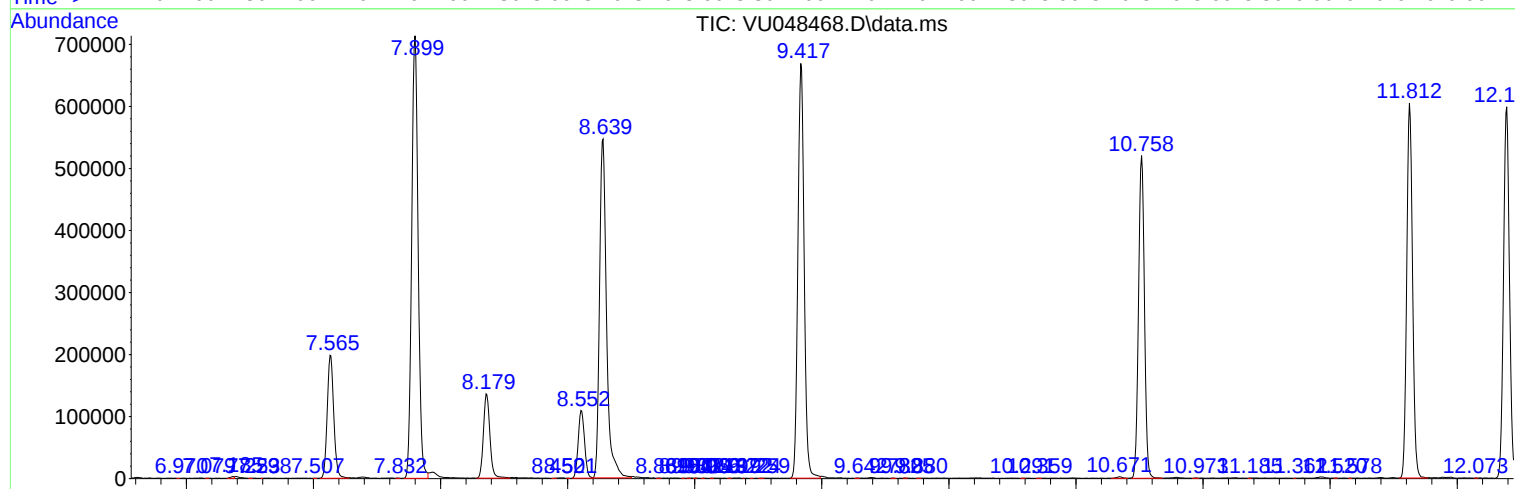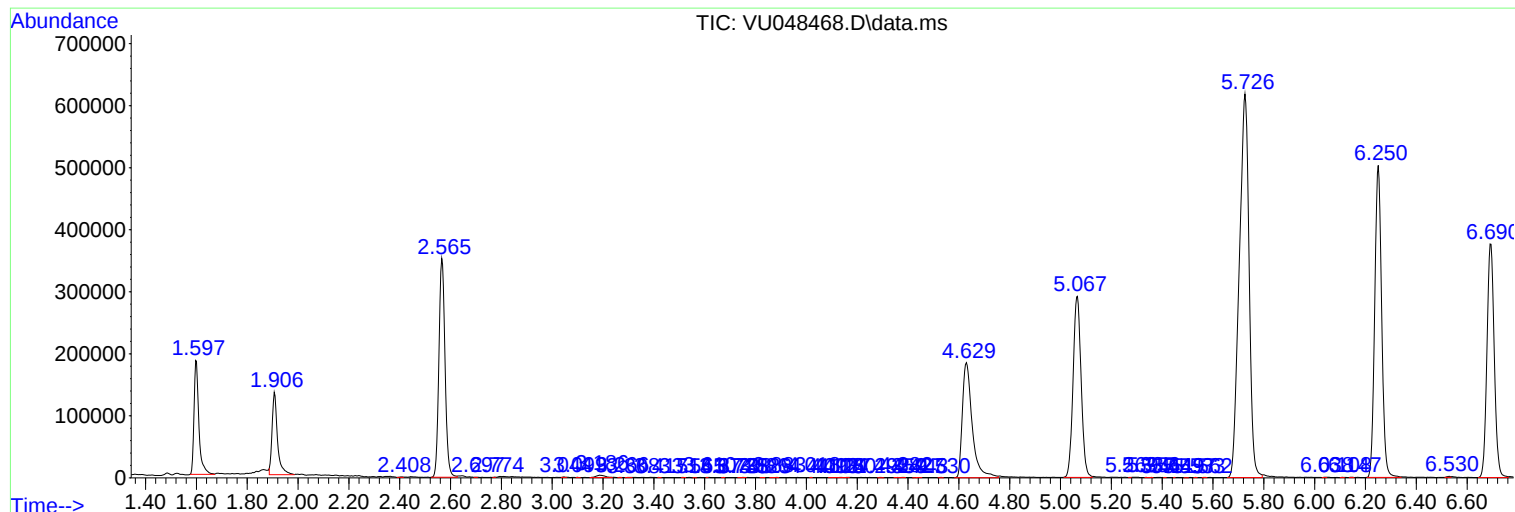

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050622\
Data File : VU048468.D
Acq On : 06 May 2022 20:29
Operator : SY/MD
Sample : N2710-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXLA3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050622\
Data File : VU048468.D
Acq On : 06 May 2022 20:29
Operator : SY/MD
Sample : N2710-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXLA3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc