

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050622\
 Data File : VU048469.D
 Acq On : 06 May 2022 20:53
 Operator : SY/MD
 Sample : N2710-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXLA4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

Signal : TIC: VU048469.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	100	rBV	192217	248277	15.31%	2.031%
2	1.900	166	174	199	rVB	122402	192619	11.88%	1.576%
3	2.565	367	381	397	rBV	350153	573491	35.36%	4.691%
4	2.729	428	432	434	rBV2	846	622	0.04%	0.005%
5	2.771	435	445	462	rVB3	4902	12366	0.76%	0.101%
6	2.896	480	484	488	rVV3	451	347	0.02%	0.003%
7	2.964	502	505	508	rVB2	583	402	0.02%	0.003%
8	3.054	527	533	536	rVB4	731	606	0.04%	0.005%
9	3.109	546	550	554	rVB2	260	226	0.01%	0.002%
10	3.189	559	575	591	rBV2	11110	27125	1.67%	0.222%
11	3.363	621	629	632	rBV2	234	317	0.02%	0.003%
12	4.179	877	883	885	rVV	299	265	0.02%	0.002%
13	4.240	895	902	905	rBV2	317	361	0.02%	0.003%
14	4.302	919	921	926	rVB	359	268	0.02%	0.002%
15	4.337	926	932	936	rBV2	651	898	0.06%	0.007%
16	4.620	1004	1020	1048	rBV	196806	477337	29.43%	3.904%
17	4.839	1085	1088	1092	rVB2	695	470	0.03%	0.004%
18	4.861	1092	1095	1100	rBV3	334	336	0.02%	0.003%
19	4.974	1127	1130	1132	rBV	464	290	0.02%	0.002%
20	5.064	1141	1158	1177	rBV	285141	628416	38.75%	5.140%
21	5.199	1196	1200	1203	rVB3	427	365	0.02%	0.003%
22	5.282	1223	1226	1229	rBV3	558	470	0.03%	0.004%
23	5.411	1263	1266	1268	rBV2	345	205	0.01%	0.002%
24	5.578	1316	1318	1321	rVV	465	196	0.01%	0.002%
25	5.726	1341	1364	1396	rBV2	596952	1621694	100.00%	13.265%
26	5.916	1421	1423	1426	rVB2	381	219	0.01%	0.002%
27	5.974	1437	1441	1445	rBV4	759	634	0.04%	0.005%
28	5.993	1445	1447	1449	rVB	504	237	0.01%	0.002%
29	6.015	1449	1454	1457	rBV3	341	300	0.02%	0.002%
30	6.038	1457	1461	1466	rBV3	498	473	0.03%	0.004%
31	6.067	1466	1470	1475	rVB2	408	293	0.02%	0.002%
32	6.163	1494	1500	1503	rBV3	447	572	0.04%	0.005%
33	6.195	1507	1510	1512	rBV	443	263	0.02%	0.002%
34	6.247	1512	1526	1550	rBV	479137	918176	56.62%	7.510%
35	6.478	1594	1598	1602	rBV4	528	526	0.03%	0.004%
36	6.539	1607	1617	1630	rVB9	7747	15647	0.96%	0.128%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050622\
 Data File : VU048469.D
 Acq On : 06 May 2022 20:53
 Operator : SY/MD
 Sample : N2710-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXLA4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

37	6.691	1650	1664	1682	rBV	377693	733568	45.23%	6.000%
38	6.861	1713	1717	1720	rVB2	439	298	0.02%	0.002%
39	6.880	1720	1723	1726	rBV2	429	293	0.02%	0.002%
40	7.047	1772	1775	1781	rVB3	316	352	0.02%	0.003%
41	7.179	1808	1816	1826	rVV5	3187	5652	0.35%	0.046%
42	7.218	1826	1828	1832	rVB	514	325	0.02%	0.003%
43	7.343	1863	1867	1869	rBV2	358	245	0.02%	0.002%
44	7.398	1881	1884	1890	rBV2	421	379	0.02%	0.003%
45	7.475	1903	1908	1911	rVB2	304	222	0.01%	0.002%
46	7.520	1919	1922	1924	rBV	355	256	0.02%	0.002%
47	7.565	1924	1936	1953	rVV	196920	344849	21.26%	2.821%
48	7.687	1968	1974	1975	rBV	1143	915	0.06%	0.007%
49	7.900	2025	2040	2056	rBV	699258	1222749	75.40%	10.002%
50	8.179	2115	2127	2141	rBV	137320	231497	14.28%	1.894%
51	8.440	2206	2208	2213	rBV2	318	366	0.02%	0.003%
52	8.514	2228	2231	2234	rBV2	317	218	0.01%	0.002%
53	8.549	2234	2242	2250	rVB6	1234	1839	0.11%	0.015%
54	8.633	2255	2268	2308	rBV2	544872	1038703	64.05%	8.496%
55	8.912	2352	2355	2358	rBV3	720	541	0.03%	0.004%
56	8.983	2374	2377	2379	rBV	487	227	0.01%	0.002%
57	9.054	2396	2399	2404	rBV2	295	291	0.02%	0.002%
58	9.276	2463	2468	2473	rBV2	254	354	0.02%	0.003%
59	9.417	2496	2512	2535	rBV	663748	1111088	68.51%	9.088%
60	9.559	2553	2556	2558	rBV3	451	267	0.02%	0.002%
61	9.639	2577	2581	2588	rVB2	612	594	0.04%	0.005%
62	9.684	2591	2595	2596	rBV2	664	447	0.03%	0.004%
63	9.803	2630	2632	2635	rVB	470	214	0.01%	0.002%
64	9.909	2661	2665	2668	rBV2	324	262	0.02%	0.002%
65	10.112	2720	2728	2730	rBV3	691	789	0.05%	0.006%
66	10.163	2739	2744	2752	rVB2	385	431	0.03%	0.004%
67	10.218	2759	2761	2764	rVB2	448	211	0.01%	0.002%
68	10.311	2787	2790	2793	rVB2	394	242	0.01%	0.002%
69	10.333	2794	2797	2800	rBV2	261	228	0.01%	0.002%
70	10.414	2819	2822	2826	rBV2	353	267	0.02%	0.002%
71	10.581	2870	2874	2877	rBV3	373	305	0.02%	0.002%
72	10.668	2894	2901	2910	rBV7	1978	2750	0.17%	0.022%
73	10.758	2915	2929	2949	rBV	524002	854301	52.68%	6.988%
74	10.864	2959	2962	2965	rBV2	653	414	0.03%	0.003%
75	10.890	2965	2970	2973	rBV4	1589	1412	0.09%	0.012%
76	10.954	2987	2990	2993	rBV2	451	220	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050622\
 Data File : VU048469.D
 Acq On : 06 May 2022 20:53
 Operator : SY/MD
 Sample : N2710-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXLA4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

77	11.051	3017	3020	3024	rBV2	342	255	0.02%	0.002%
78	11.105	3036	3037	3040	rBV	549	372	0.02%	0.003%
79	11.411	3128	3132	3135	rBV3	543	413	0.03%	0.003%
80	11.459	3141	3147	3159	rVB7	1979	3487	0.22%	0.029%
81	11.514	3159	3164	3167	rBV2	234	271	0.02%	0.002%
82	11.571	3180	3182	3187	rBV3	399	373	0.02%	0.003%
83	11.697	3219	3221	3224	rVB4	1075	608	0.04%	0.005%
84	11.813	3243	3257	3273	rBV	595741	945932	58.33%	7.737%
85	11.970	3302	3306	3318	rVB5	1558	2424	0.15%	0.020%
86	12.195	3360	3376	3398	rBV	601231	978809	60.36%	8.006%
87	12.388	3433	3436	3439	rBV2	432	300	0.02%	0.002%
88	12.404	3439	3441	3443	rBV	469	231	0.01%	0.002%
89	12.456	3454	3457	3458	rBV	416	220	0.01%	0.002%
90	12.581	3493	3496	3499	rBV	415	235	0.01%	0.002%
91	12.671	3521	3524	3526	rVB2	533	318	0.02%	0.003%
92	12.771	3548	3555	3559	rBV3	669	952	0.06%	0.008%
93	12.935	3603	3606	3610	rBV3	543	494	0.03%	0.004%
94	13.192	3683	3686	3691	rBV3	707	713	0.04%	0.006%
95	13.780	3866	3869	3871	rBV	666	356	0.02%	0.003%
96	14.102	3963	3969	3977	rVB5	2666	3564	0.22%	0.029%
97	14.333	4038	4041	4042	rBV2	1001	619	0.04%	0.005%
98	14.549	4106	4108	4111	rBV2	486	263	0.02%	0.002%
99	14.632	4132	4134	4137	rVB2	578	275	0.02%	0.002%
100	15.529	4411	4413	4416	rBV	671	278	0.02%	0.002%


Sum of corrected areas: 12225652

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050622\
Data File : VU048469.D
Acq On : 06 May 2022 20:53
Operator : SY/MD
Sample : N2710-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXLA4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

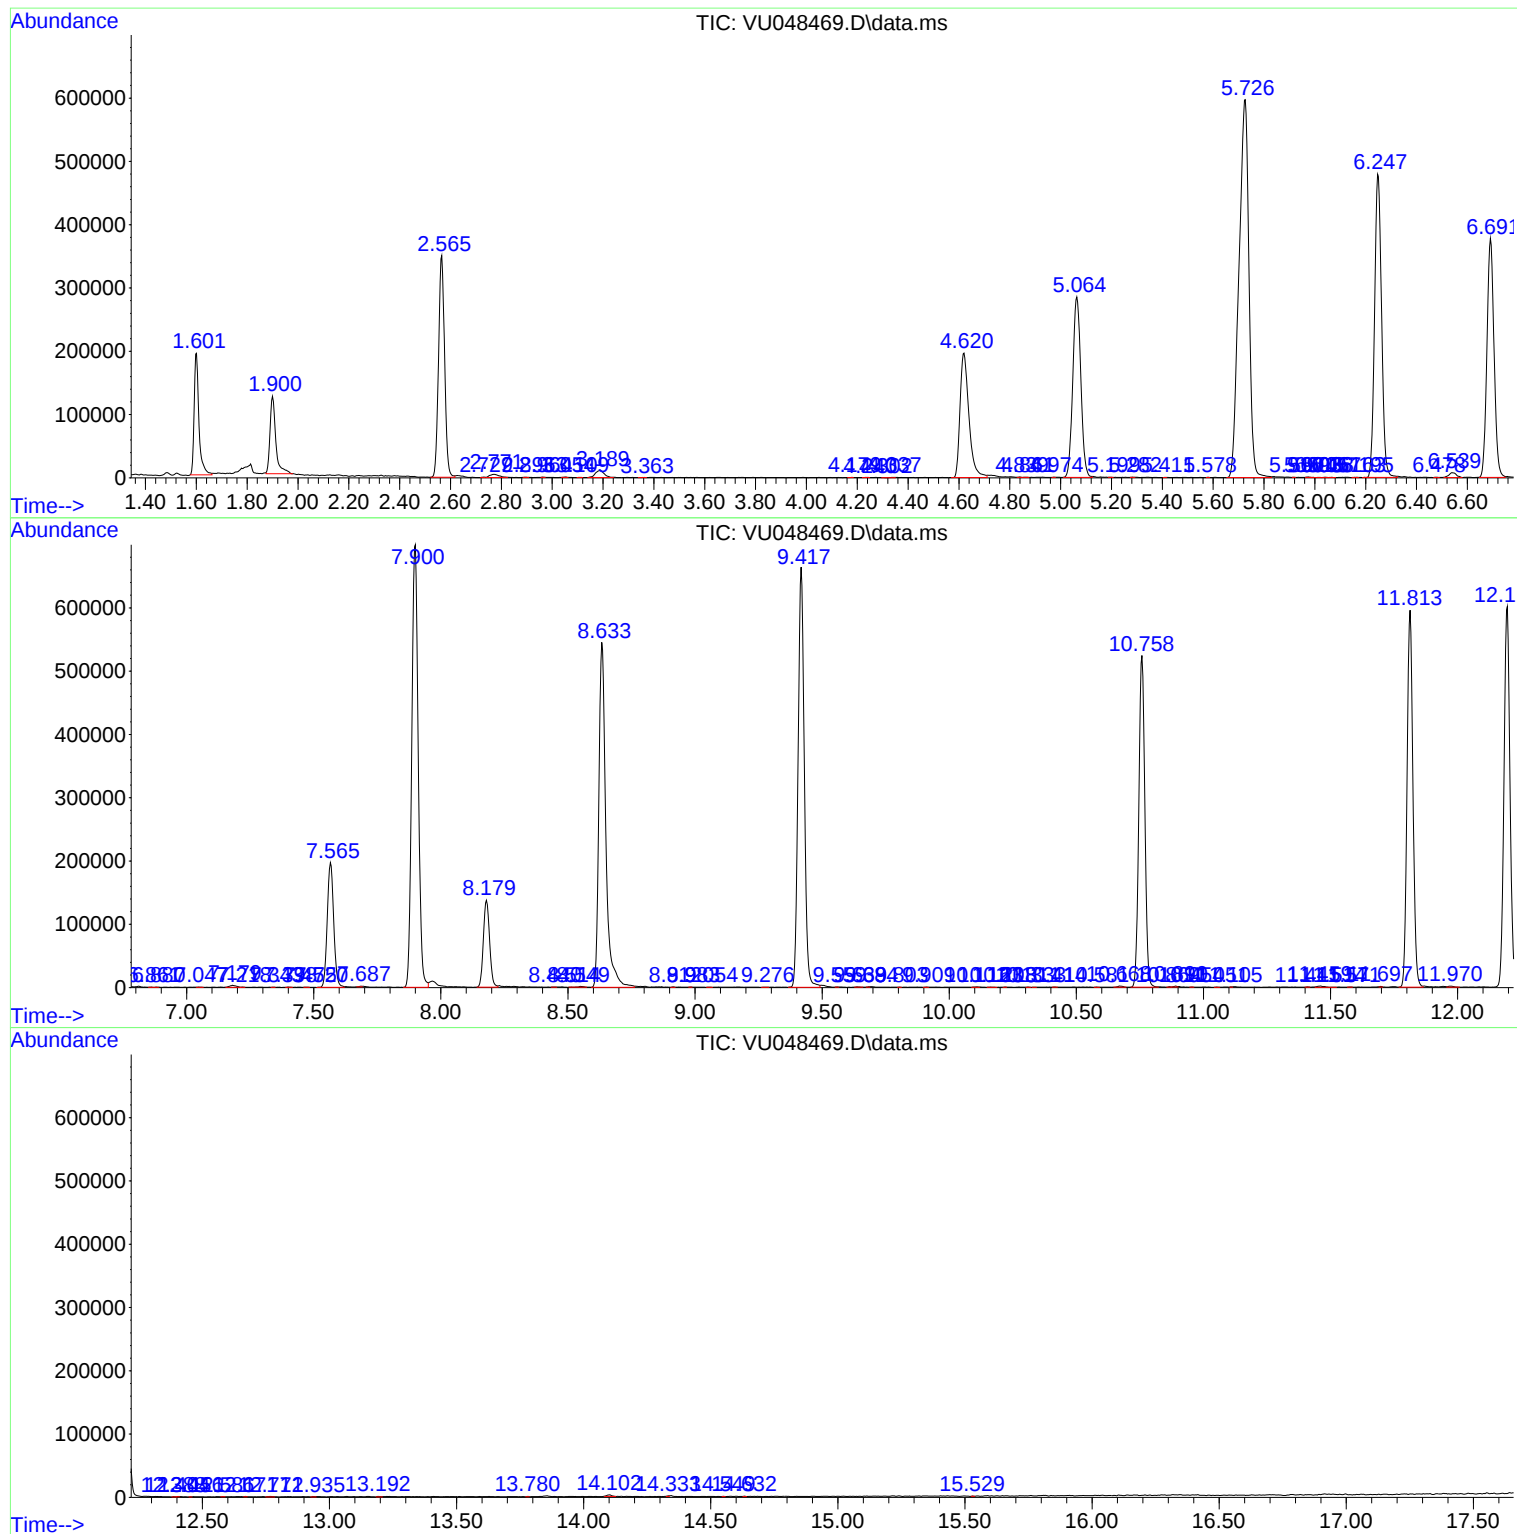

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050622\
Data File : VU048469.D
Acq On : 06 May 2022 20:53
Operator : SY/MD
Sample : N2710-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXLA4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050622\
Data File : VU048469.D
Acq On : 06 May 2022 20:53
Operator : SY/MD
Sample : N2710-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXLA4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc