

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050622\
 Data File : VU048473.D
 Acq On : 06 May 2022 22:28
 Operator : SY/MD
 Sample : N2710-20
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXLA9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

Signal : TIC: VU048473.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	98	rBV	185432	235977	14.93%	2.090%
2	1.912	170	178	206	rVB	135046	196607	12.43%	1.742%
3	2.456	344	347	354	rVB5	1209	1101	0.07%	0.010%
4	2.568	369	382	398	rBV	336984	554514	35.07%	4.912%
5	2.793	446	452	453	rBV4	1344	1329	0.08%	0.012%
6	3.047	528	531	534	rBV	747	563	0.04%	0.005%
7	3.093	539	545	548	rBV2	268	317	0.02%	0.003%
8	3.183	566	573	574	rBV3	2195	2276	0.14%	0.020%
9	3.388	633	637	640	rBV2	342	241	0.02%	0.002%
10	3.623	706	710	714	rBV2	291	334	0.02%	0.003%
11	3.707	734	736	743	rVB2	317	231	0.01%	0.002%
12	3.777	755	758	765	rVB2	270	227	0.01%	0.002%
13	4.160	874	877	882	rVB2	231	240	0.02%	0.002%
14	4.250	901	905	910	rBV2	245	252	0.02%	0.002%
15	4.276	910	913	917	rVB	422	300	0.02%	0.003%
16	4.308	917	923	928	rBV	526	701	0.04%	0.006%
17	4.626	1009	1022	1059	rBV	163633	440682	27.87%	3.904%
18	4.877	1096	1100	1104	rBV2	504	462	0.03%	0.004%
19	4.928	1113	1116	1118	rBV2	330	238	0.02%	0.002%
20	5.067	1142	1159	1185	rBV	284038	621035	39.28%	5.501%
21	5.401	1261	1263	1270	rVB2	329	259	0.02%	0.002%
22	5.539	1304	1306	1310	rBV2	268	241	0.02%	0.002%
23	5.726	1342	1364	1392	rBV2	580170	1581079	100.00%	14.005%
24	5.932	1425	1428	1430	rBV2	335	251	0.02%	0.002%
25	6.118	1482	1486	1489	rBV2	564	496	0.03%	0.004%
26	6.150	1493	1496	1501	rVB3	479	347	0.02%	0.003%
27	6.250	1512	1527	1553	rBV	469447	898856	56.85%	7.962%
28	6.433	1582	1584	1589	rVB2	574	472	0.03%	0.004%
29	6.462	1590	1593	1597	rBV2	315	223	0.01%	0.002%
30	6.526	1609	1613	1620	rVV6	1561	2258	0.14%	0.020%
31	6.604	1635	1637	1640	rVB2	625	341	0.02%	0.003%
32	6.690	1648	1664	1690	rBV	364312	721088	45.61%	6.387%
33	7.186	1811	1818	1828	rVV6	2019	3275	0.21%	0.029%
34	7.231	1830	1832	1838	rVB2	443	256	0.02%	0.002%
35	7.366	1871	1874	1877	rBV	320	227	0.01%	0.002%
36	7.568	1924	1937	1958	rBV	186246	333591	21.10%	2.955%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050622\
 Data File : VU048473.D
 Acq On : 06 May 2022 22:28
 Operator : SY/MD
 Sample : N2710-20
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXLA9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

37	7.690	1967	1975	1988	rBV7	1667	3125	0.20%	0.028%
38	7.761	1995	1997	2000	rVB2	604	305	0.02%	0.003%
39	7.800	2006	2009	2014	rVB4	322	300	0.02%	0.003%
40	7.899	2025	2040	2057	rBV	678101	1194708	75.56%	10.583%
41	8.128	2107	2111	2114	rBV4	468	340	0.02%	0.003%
42	8.179	2116	2127	2152	rVV	129985	227158	14.37%	2.012%
43	8.327	2171	2173	2177	rBV2	346	242	0.02%	0.002%
44	8.475	2212	2219	2222	rBV4	996	1187	0.08%	0.011%
45	8.517	2229	2232	2234	rVB	425	233	0.01%	0.002%
46	8.555	2234	2244	2254	rBV2	17058	29462	1.86%	0.261%
47	8.636	2256	2269	2295	rBV2	471349	950811	60.14%	8.422%
48	8.854	2334	2337	2341	rVB4	378	291	0.02%	0.003%
49	8.919	2353	2357	2362	rBV3	347	345	0.02%	0.003%
50	8.973	2370	2374	2379	rVB2	409	343	0.02%	0.003%
51	9.166	2429	2434	2436	rBV2	623	540	0.03%	0.005%
52	9.417	2499	2512	2532	rBV	644288	1094057	69.20%	9.691%
53	9.645	2581	2583	2587	rVB3	618	350	0.02%	0.003%
54	9.690	2591	2597	2600	rBV3	967	855	0.05%	0.008%
55	10.105	2723	2726	2728	rBV3	364	233	0.01%	0.002%
56	10.382	2807	2812	2817	rBV2	368	456	0.03%	0.004%
57	10.581	2869	2874	2879	rBV2	260	272	0.02%	0.002%
58	10.645	2892	2894	2897	rVV	312	240	0.02%	0.002%
59	10.674	2899	2903	2911	rVB4	1530	1658	0.10%	0.015%
60	10.758	2914	2929	2949	rBV	390610	628023	39.72%	5.563%
61	10.899	2965	2973	2976	rVB4	1517	1729	0.11%	0.015%
62	10.957	2985	2991	2995	rVB2	317	345	0.02%	0.003%
63	11.111	3037	3039	3043	rVB2	377	224	0.01%	0.002%
64	11.134	3043	3046	3052	rVB	375	288	0.02%	0.003%
65	11.282	3087	3092	3095	rBV2	261	236	0.01%	0.002%
66	11.362	3114	3117	3121	rVB	297	246	0.02%	0.002%
67	11.388	3121	3125	3128	rBV2	243	237	0.01%	0.002%
68	11.459	3137	3147	3157	rVB5	1310	2339	0.15%	0.021%
69	11.677	3212	3215	3219	rBV2	428	361	0.02%	0.003%
70	11.700	3220	3222	3228	rVB3	560	410	0.03%	0.004%
71	11.738	3229	3234	3236	rBV3	529	420	0.03%	0.004%
72	11.751	3236	3238	3243	rVB2	537	416	0.03%	0.004%
73	11.812	3243	3257	3274	rBV	444709	701287	44.35%	6.212%
74	11.912	3286	3288	3292	rBV2	593	499	0.03%	0.004%
75	11.973	3303	3307	3314	rVB3	1073	1273	0.08%	0.011%
76	12.115	3348	3351	3353	rBV2	383	245	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050622\
 Data File : VU048473.D
 Acq On : 06 May 2022 22:28
 Operator : SY/MD
 Sample : N2710-20
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXLA9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

77	12.195	3361	3376	3393	rBV	519988	831761	52.61%	7.368%
78	12.311	3409	3412	3417	rVB3	553	472	0.03%	0.004%
79	12.340	3417	3421	3423	rBV2	722	538	0.03%	0.005%
80	12.394	3431	3438	3441	rBV2	820	824	0.05%	0.007%
81	12.414	3441	3444	3448	rVV	476	357	0.02%	0.003%
82	12.455	3454	3457	3461	rBV3	433	349	0.02%	0.003%
83	12.536	3479	3482	3484	rBV2	478	310	0.02%	0.003%
84	12.552	3485	3487	3490	rVB3	521	287	0.02%	0.003%
85	12.677	3524	3526	3529	rBV	452	299	0.02%	0.003%
86	12.806	3563	3566	3571	rBV2	301	287	0.02%	0.003%
87	13.144	3669	3671	3675	rBV3	374	288	0.02%	0.003%
88	13.211	3689	3692	3696	rBV3	333	268	0.02%	0.002%
89	13.443	3761	3764	3765	rBV2	372	229	0.01%	0.002%
90	13.510	3782	3785	3787	rBV2	610	392	0.02%	0.003%
91	13.578	3804	3806	3809	rBV	347	225	0.01%	0.002%
92	13.690	3838	3841	3845	rVB3	453	258	0.02%	0.002%
93	13.861	3886	3894	3901	rBV5	1031	1881	0.12%	0.017%
94	14.015	3939	3942	3944	rBV2	396	289	0.02%	0.003%
95	14.330	4036	4040	4041	rBV2	890	605	0.04%	0.005%
96	14.468	4080	4083	4085	rBV2	633	342	0.02%	0.003%
97	14.925	4223	4225	4229	rBV3	556	370	0.02%	0.003%
98	15.240	4320	4323	4325	rBV2	720	413	0.03%	0.004%
99	15.433	4381	4383	4386	rBV3	757	443	0.03%	0.004%
100	15.661	4451	4454	4458	rBV3	946	826	0.05%	0.007%




Sum of corrected areas: 11289289

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050622\
Data File : VU048473.D
Acq On : 06 May 2022 22:28
Operator : SY/MD
Sample : N2710-20
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXLA9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

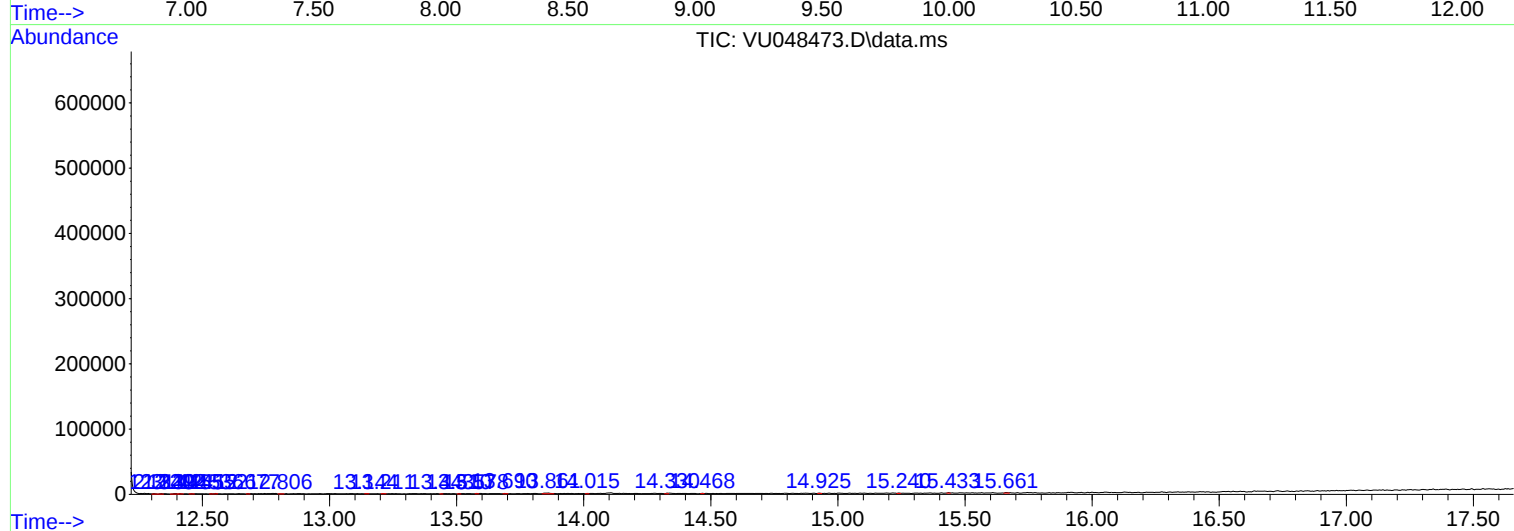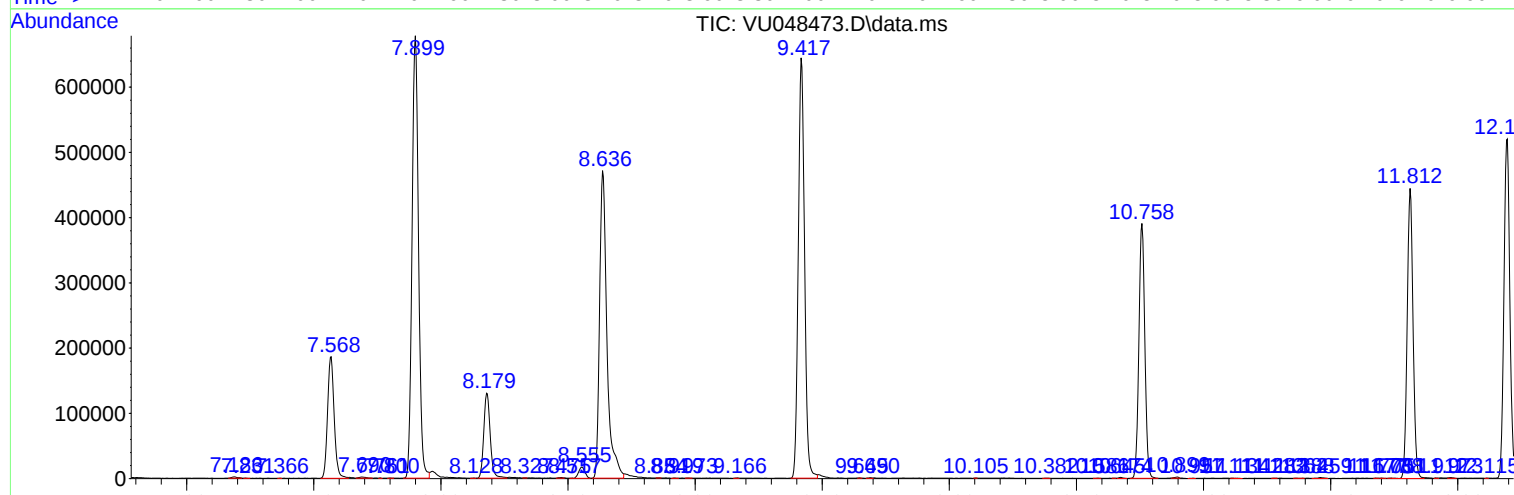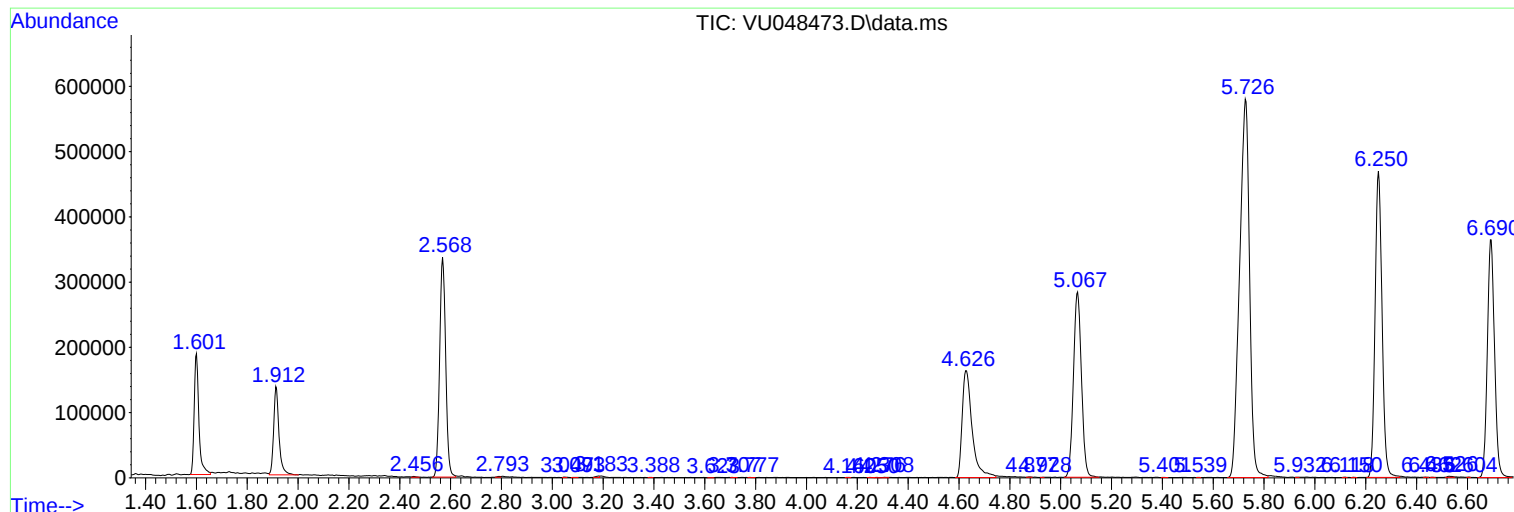

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050622\
Data File : VU048473.D
Acq On : 06 May 2022 22:28
Operator : SY/MD
Sample : N2710-20
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXLA9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050622\
Data File : VU048473.D
Acq On : 06 May 2022 22:28
Operator : SY/MD
Sample : N2710-20
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXLA9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------