

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050622\
 Data File : VU048474.D
 Acq On : 06 May 2022 22:52
 Operator : SY/MD
 Sample : N2710-21
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXLB0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

Signal : TIC: VU048474.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	102	rBV	197762	247847	15.48%	2.129%
2	1.916	170	179	202	rVB	137273	200499	12.53%	1.723%
3	2.436	338	341	344	rVB4	906	606	0.04%	0.005%
4	2.459	345	348	352	rBV4	794	608	0.04%	0.005%
5	2.568	367	382	397	rBV	344866	562302	35.13%	4.831%
6	2.745	433	437	441	rBV2	622	495	0.03%	0.004%
7	2.793	449	452	458	rVB2	679	751	0.05%	0.006%
8	3.038	525	528	530	rBV3	474	318	0.02%	0.003%
9	3.102	544	548	552	rVB2	370	348	0.02%	0.003%
10	3.128	552	556	558	rBV	355	287	0.02%	0.002%
11	3.372	628	632	635	rBV2	301	243	0.02%	0.002%
12	3.420	644	647	649	rBV2	340	208	0.01%	0.002%
13	3.530	677	681	682	rBV2	322	206	0.01%	0.002%
14	3.562	687	691	695	rVB2	473	371	0.02%	0.003%
15	3.793	759	763	766	rBV	269	205	0.01%	0.002%
16	4.530	986	992	995	rVB2	257	246	0.02%	0.002%
17	4.620	1005	1020	1049	rBV	169451	417226	26.06%	3.585%
18	5.067	1138	1159	1184	rBV	284709	626916	39.16%	5.386%
19	5.279	1223	1225	1228	rBV3	446	317	0.02%	0.003%
20	5.295	1228	1230	1235	rVB2	590	438	0.03%	0.004%
21	5.436	1267	1274	1278	rBV2	369	420	0.03%	0.004%
22	5.597	1322	1324	1329	rVB2	401	249	0.02%	0.002%
23	5.726	1342	1364	1400	rBV2	586627	1600747	100.00%	13.753%
24	5.970	1436	1440	1443	rBV3	488	393	0.02%	0.003%
25	5.993	1445	1447	1450	rVB	713	357	0.02%	0.003%
26	6.015	1450	1454	1457	rVB2	278	216	0.01%	0.002%
27	6.034	1457	1460	1463	rBV2	534	419	0.03%	0.004%
28	6.086	1473	1476	1480	rVB2	326	231	0.01%	0.002%
29	6.112	1480	1484	1488	rBV4	489	407	0.03%	0.003%
30	6.137	1488	1492	1494	rVB3	355	231	0.01%	0.002%
31	6.185	1504	1507	1510	rBV2	278	205	0.01%	0.002%
32	6.250	1511	1527	1556	rBV	480769	919407	57.44%	7.899%
33	6.411	1574	1577	1583	rVV3	412	380	0.02%	0.003%
34	6.446	1586	1588	1596	rVB2	564	503	0.03%	0.004%
35	6.533	1608	1615	1620	rBV5	1402	1934	0.12%	0.017%
36	6.610	1637	1639	1645	rVB4	651	446	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050622\
 Data File : VU048474.D
 Acq On : 06 May 2022 22:52
 Operator : SY/MD
 Sample : N2710-21
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXLB0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

37	6.694	1647	1665	1686	rBV	368453	728821	45.53%	6.262%
38	6.796	1694	1697	1699	rBV4	671	445	0.03%	0.004%
39	7.044	1772	1774	1781	rVB3	554	471	0.03%	0.004%
40	7.079	1781	1785	1789	rBV2	425	366	0.02%	0.003%
41	7.189	1810	1819	1829	rVV4	2674	4227	0.26%	0.036%
42	7.311	1853	1857	1859	rBV2	372	272	0.02%	0.002%
43	7.362	1871	1873	1880	rVB2	338	277	0.02%	0.002%
44	7.446	1896	1899	1903	rVB2	358	275	0.02%	0.002%
45	7.568	1924	1937	1960	rBV	189268	338423	21.14%	2.908%
46	7.687	1969	1974	1975	rBV3	904	769	0.05%	0.007%
47	7.745	1990	1992	1996	rVV2	461	253	0.02%	0.002%
48	7.899	2025	2040	2057	rBV	691259	1208552	75.50%	10.384%
49	8.179	2116	2127	2145	rBV	131109	223809	13.98%	1.923%
50	8.462	2211	2215	2216	rBV3	381	274	0.02%	0.002%
51	8.555	2231	2244	2257	rBV	181916	304763	19.04%	2.619%
52	8.632	2257	2268	2307	rVV2	433808	904506	56.51%	7.771%
53	8.848	2334	2335	2343	rVB2	851	643	0.04%	0.006%
54	9.163	2429	2433	2435	rBV	443	297	0.02%	0.003%
55	9.218	2446	2450	2451	rBV2	293	221	0.01%	0.002%
56	9.362	2487	2495	2499	rBV2	485	663	0.04%	0.006%
57	9.417	2499	2512	2533	rBV	665982	1122498	70.12%	9.644%
58	9.571	2555	2560	2565	rVB5	819	934	0.06%	0.008%
59	10.095	2720	2723	2726	rVB2	505	333	0.02%	0.003%
60	10.185	2748	2751	2754	rBV2	230	214	0.01%	0.002%
61	10.291	2781	2784	2787	rVB2	372	240	0.01%	0.002%
62	10.484	2842	2844	2847	rVB2	454	240	0.01%	0.002%
63	10.565	2865	2869	2871	rBV	310	265	0.02%	0.002%
64	10.758	2916	2929	2945	rBV	492119	795462	49.69%	6.835%
65	10.835	2950	2953	2959	rBV	252	301	0.02%	0.003%
66	10.886	2965	2969	2970	rBV	852	489	0.03%	0.004%
67	10.896	2970	2972	2984	rVB4	1338	1426	0.09%	0.012%
68	11.176	3053	3059	3060	rBV	292	196	0.01%	0.002%
69	11.217	3070	3072	3076	rBV2	321	233	0.01%	0.002%
70	11.333	3101	3108	3113	rBV2	304	402	0.03%	0.003%
71	11.459	3143	3147	3149	rBV4	793	599	0.04%	0.005%
72	11.571	3179	3182	3189	rBV2	327	393	0.02%	0.003%
73	11.610	3189	3194	3197	rBV2	408	442	0.03%	0.004%
74	11.684	3213	3217	3220	rBV	366	401	0.03%	0.003%
75	11.812	3245	3257	3278	rBV	432650	690905	43.16%	5.936%
76	11.912	3285	3288	3293	rVB3	814	717	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050622\
 Data File : VU048474.D
 Acq On : 06 May 2022 22:52
 Operator : SY/MD
 Sample : N2710-21
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXLB0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

77	11.941	3293	3297	3300	rBV2	954	846	0.05%	0.007%
78	11.973	3304	3307	3311	rVV3	379	342	0.02%	0.003%
79	12.041	3324	3328	3330	rBV	290	213	0.01%	0.002%
80	12.073	3330	3338	3345	rBV3	2326	3461	0.22%	0.030%
81	12.195	3362	3376	3393	rBV	433900	704574	44.02%	6.054%
82	12.365	3425	3429	3430	rBV	534	382	0.02%	0.003%
83	12.423	3444	3447	3452	rVB3	520	407	0.03%	0.003%
84	12.526	3475	3479	3481	rBV2	230	202	0.01%	0.002%
85	12.603	3500	3503	3507	rVB2	434	305	0.02%	0.003%
86	12.902	3594	3596	3602	rVB	415	355	0.02%	0.003%
87	12.934	3602	3606	3611	rBV4	660	733	0.05%	0.006%
88	12.992	3621	3624	3627	rBV2	425	283	0.02%	0.002%
89	13.089	3651	3654	3656	rBV	405	241	0.02%	0.002%
90	13.153	3672	3674	3677	rBV2	277	209	0.01%	0.002%
91	13.417	3754	3756	3760	rVB2	664	489	0.03%	0.004%
92	13.439	3760	3763	3764	rBV	407	224	0.01%	0.002%
93	13.574	3803	3805	3809	rBV	424	294	0.02%	0.003%
94	13.806	3874	3877	3881	rBV3	399	325	0.02%	0.003%
95	13.950	3917	3922	3926	rBV3	572	708	0.04%	0.006%
96	14.021	3940	3944	3949	rBV3	408	623	0.04%	0.005%
97	14.262	4017	4019	4021	rBV2	392	224	0.01%	0.002%
98	14.507	4093	4095	4097	rBV2	477	195	0.01%	0.002%
99	14.844	4197	4200	4204	rBV	597	437	0.03%	0.004%
100	15.429	4379	4382	4388	rBV4	771	765	0.05%	0.007%




Sum of corrected areas: 11638836

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050622\
Data File : VU048474.D
Acq On : 06 May 2022 22:52
Operator : SY/MD
Sample : N2710-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXLB0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

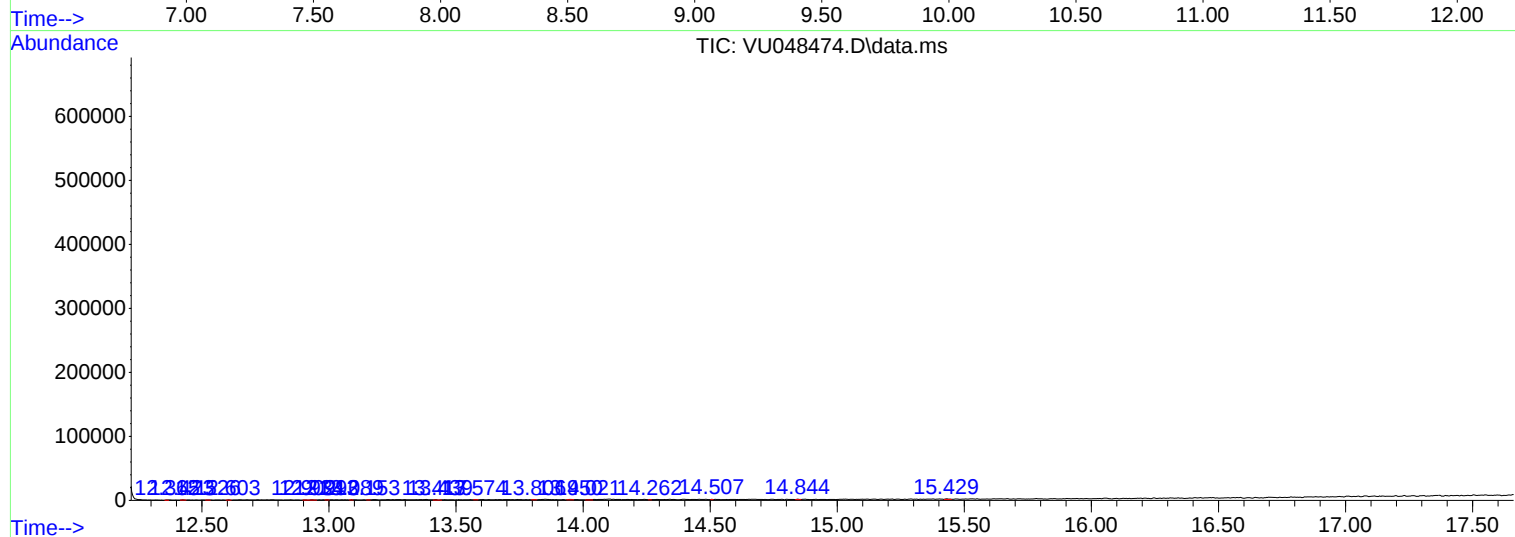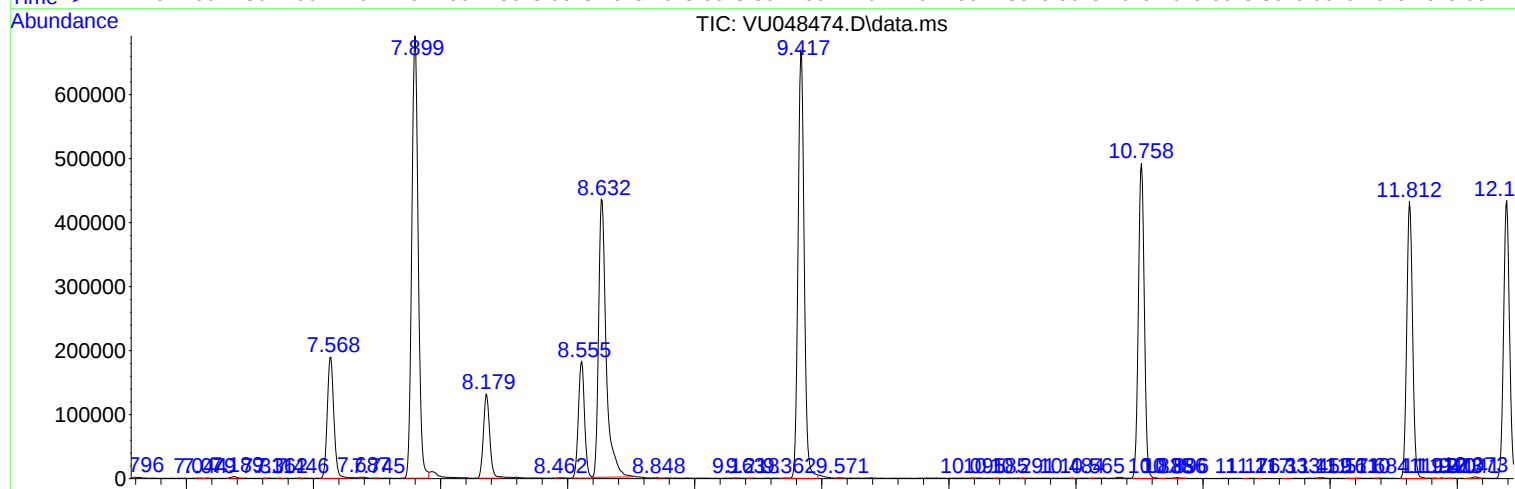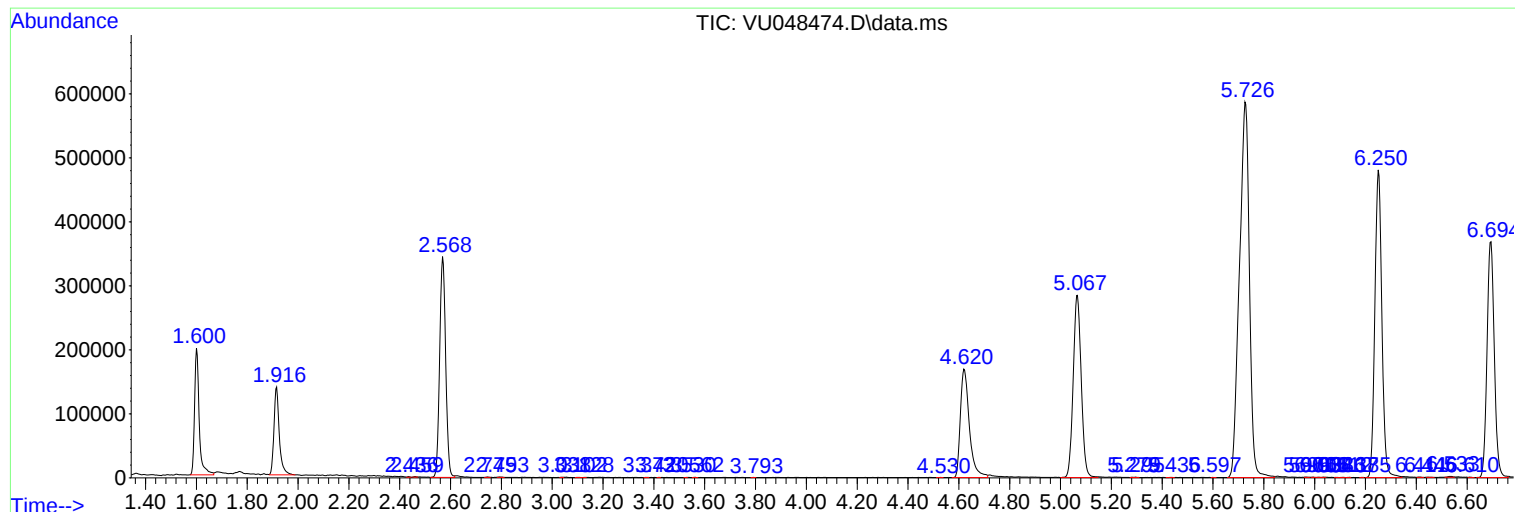

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050622\
Data File : VU048474.D
Acq On : 06 May 2022 22:52
Operator : SY/MD
Sample : N2710-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXLB0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050622\
Data File : VU048474.D
Acq On : 06 May 2022 22:52
Operator : SY/MD
Sample : N2710-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXLB0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------