

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050622\
 Data File : VU048476.D
 Acq On : 06 May 2022 23:40
 Operator : SY/MD
 Sample : N2710-23
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXLB2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

Signal : TIC: VU048476.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	105	rBV	106725	145285	14.12%	1.843%
2	1.913	171	178	194	rVB	78094	108149	10.51%	1.372%
3	2.568	370	382	396	rBV	223336	361878	35.16%	4.592%
4	2.784	436	449	453	rBV4	2040	3754	0.36%	0.048%
5	2.861	468	473	480	rVB2	459	527	0.05%	0.007%
6	2.903	480	486	491	rBV2	381	460	0.04%	0.006%
7	2.954	499	502	505	rBV	264	196	0.02%	0.002%
8	3.080	539	541	543	rBV	198	137	0.01%	0.002%
9	3.183	566	573	576	rBV2	2130	2657	0.26%	0.034%
10	3.257	592	596	600	rVB	407	327	0.03%	0.004%
11	3.282	600	604	608	rBV	350	386	0.04%	0.005%
12	3.311	610	613	615	rBV	243	148	0.01%	0.002%
13	3.466	657	661	663	rBV	333	278	0.03%	0.004%
14	3.494	667	670	671	rBV	214	129	0.01%	0.002%
15	3.565	690	692	694	rVB	164	79	0.01%	0.001%
16	3.607	704	705	708	rBV	254	134	0.01%	0.002%
17	3.630	708	712	713	rBV2	191	133	0.01%	0.002%
18	3.671	722	725	731	rVB2	337	288	0.03%	0.004%
19	3.707	732	736	737	rVV	148	85	0.01%	0.001%
20	3.726	737	742	745	rVV2	328	348	0.03%	0.004%
21	3.748	746	749	752	rVB2	403	304	0.03%	0.004%
22	3.771	753	756	757	rBV	188	128	0.01%	0.002%
23	3.896	792	795	798	rVB2	287	208	0.02%	0.003%
24	3.916	798	801	805	rBV	194	141	0.01%	0.002%
25	3.941	805	809	810	rBV2	247	173	0.02%	0.002%
26	3.999	822	827	829	rBV	200	241	0.02%	0.003%
27	4.070	846	849	852	rBV	177	117	0.01%	0.001%
28	4.093	853	856	859	rVB2	293	170	0.02%	0.002%
29	4.112	859	862	867	rBV2	189	223	0.02%	0.003%
30	4.211	887	893	895	rBV2	293	313	0.03%	0.004%
31	4.289	915	917	919	rBV	255	141	0.01%	0.002%
32	4.353	932	937	939	rBV2	216	235	0.02%	0.003%
33	4.469	968	973	976	rBV2	323	345	0.03%	0.004%
34	4.568	1000	1004	1008	rBV2	290	253	0.02%	0.003%
35	4.623	1008	1021	1047	rBV	106820	264118	25.66%	3.351%
36	5.064	1144	1158	1179	rBV	192815	424168	41.22%	5.382%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050622\
 Data File : VU048476.D
 Acq On : 06 May 2022 23:40
 Operator : SY/MD
 Sample : N2710-23
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXLB2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

37	5.250	1211	1216	1217	rBV	247	203	0.02%	0.003%
38	5.276	1222	1224	1226	rVV	177	90	0.01%	0.001%
39	5.295	1226	1230	1233	rBV2	452	462	0.04%	0.006%
40	5.337	1239	1243	1245	rBV	361	305	0.03%	0.004%
41	5.501	1292	1294	1297	rVB	300	132	0.01%	0.002%
42	5.546	1305	1308	1311	rVB2	334	233	0.02%	0.003%
43	5.565	1311	1314	1319	rBV2	387	516	0.05%	0.007%
44	5.620	1328	1331	1334	rVB	275	215	0.02%	0.003%
45	5.642	1334	1338	1340	rBV	192	174	0.02%	0.002%
46	5.726	1342	1364	1384	rBV3	373493	1029130	100.00%	13.058%
47	5.973	1439	1441	1446	rVB2	378	246	0.02%	0.003%
48	5.996	1446	1448	1450	rBV2	271	132	0.01%	0.002%
49	6.038	1459	1461	1467	rBV2	264	317	0.03%	0.004%
50	6.121	1484	1487	1489	rBV2	187	131	0.01%	0.002%
51	6.137	1489	1492	1497	rVB2	548	402	0.04%	0.005%
52	6.173	1498	1503	1505	rBV	450	288	0.03%	0.004%
53	6.189	1505	1508	1511	rBV	139	82	0.01%	0.001%
54	6.250	1511	1527	1550	rBV	320703	611752	59.44%	7.762%
55	6.443	1584	1587	1591	rBV	475	388	0.04%	0.005%
56	6.539	1605	1617	1627	rVB6	2721	5009	0.49%	0.064%
57	6.604	1635	1637	1641	rVB	360	210	0.02%	0.003%
58	6.639	1644	1648	1649	rBV	423	292	0.03%	0.004%
59	6.690	1650	1664	1691	rVV	232500	461854	44.88%	5.860%
60	6.806	1698	1700	1710	rVB3	903	990	0.10%	0.013%
61	6.845	1710	1712	1714	rVB2	308	144	0.01%	0.002%
62	6.861	1714	1717	1719	rBV	213	161	0.02%	0.002%
63	6.896	1725	1728	1730	rVB	181	107	0.01%	0.001%
64	6.944	1740	1743	1745	rBV	330	199	0.02%	0.003%
65	7.002	1758	1761	1764	rBV2	215	171	0.02%	0.002%
66	7.163	1808	1811	1812	rBV2	388	219	0.02%	0.003%
67	7.179	1813	1816	1824	rVB4	1087	1376	0.13%	0.017%
68	7.353	1867	1870	1873	rBV	233	225	0.02%	0.003%
69	7.395	1880	1883	1886	rBV	262	138	0.01%	0.002%
70	7.411	1886	1888	1892	rVV	320	179	0.02%	0.002%
71	7.430	1892	1894	1899	rVV2	346	248	0.02%	0.003%
72	7.568	1924	1937	1952	rBV	123393	220285	21.40%	2.795%
73	7.790	2001	2006	2007	rBV	409	252	0.02%	0.003%
74	7.899	2026	2040	2057	rBV	448762	782193	76.01%	9.925%
75	8.179	2116	2127	2145	rBV	90179	154350	15.00%	1.958%
76	8.430	2202	2205	2207	rBV2	262	195	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050622\
 Data File : VU048476.D
 Acq On : 06 May 2022 23:40
 Operator : SY/MD
 Sample : N2710-23
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXLB2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

77	8.446	2207	2210	2211	rBV2	377	214	0.02%	0.003%
78	8.555	2232	2244	2256	rVV2	51361	85479	8.31%	1.085%
79	8.636	2257	2269	2303	rBV3	299211	586752	57.01%	7.445%
80	8.925	2357	2359	2362	rBV	273	131	0.01%	0.002%
81	8.948	2362	2366	2369	rBV2	402	385	0.04%	0.005%
82	9.417	2499	2512	2531	rBV	439585	745044	72.40%	9.453%
83	9.610	2569	2572	2575	rBV2	253	240	0.02%	0.003%
84	9.723	2605	2607	2611	rBV	178	138	0.01%	0.002%
85	9.948	2671	2677	2681	rBV2	349	509	0.05%	0.006%
86	10.018	2696	2699	2702	rBV2	268	188	0.02%	0.002%
87	10.157	2739	2742	2748	rBV2	334	343	0.03%	0.004%
88	10.276	2776	2779	2784	rVB2	303	244	0.02%	0.003%
89	10.301	2785	2787	2790	rBV2	197	103	0.01%	0.001%
90	10.317	2790	2792	2793	rBV	292	122	0.01%	0.002%
91	10.575	2870	2872	2874	rBV	244	152	0.01%	0.002%
92	10.758	2916	2929	2946	rBV	323020	518970	50.43%	6.585%
93	10.858	2958	2960	2963	rBV2	218	170	0.02%	0.002%
94	11.436	3135	3140	3141	rBV	386	275	0.03%	0.003%
95	11.513	3160	3164	3166	rBV	330	286	0.03%	0.004%
96	11.745	3233	3236	3238	rBV2	322	203	0.02%	0.003%
97	11.812	3245	3257	3276	rBV	416133	673676	65.46%	8.548%
98	12.073	3335	3338	3341	rBV2	337	277	0.03%	0.004%
99	12.195	3363	3376	3397	rBV	412320	676139	65.70%	8.579%
100	12.883	3585	3590	3592	rBV2	447	466	0.05%	0.006%




Sum of corrected areas: 7881157

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050622\
Data File : VU048476.D
Acq On : 06 May 2022 23:40
Operator : SY/MD
Sample : N2710-23
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXLB2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

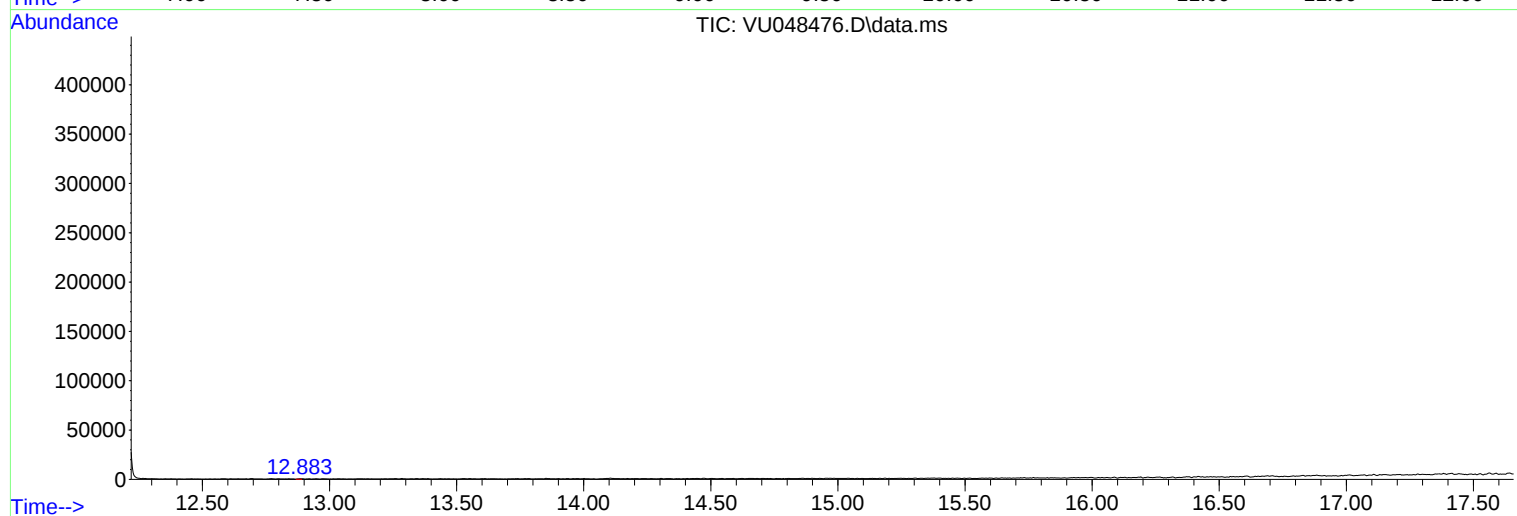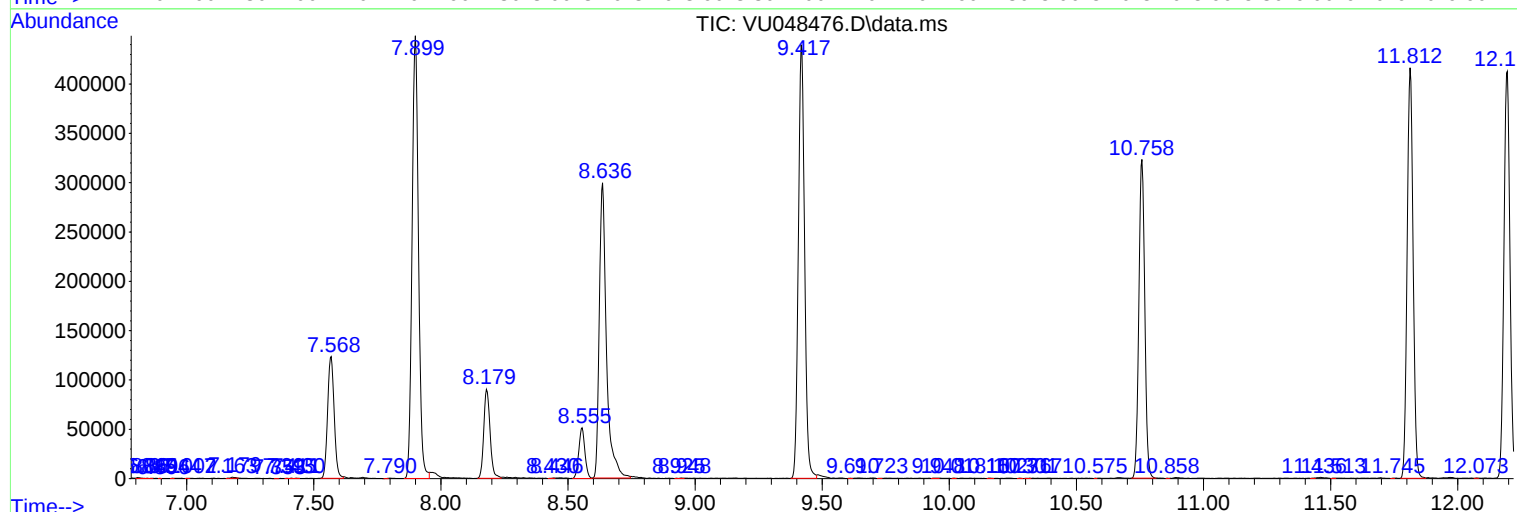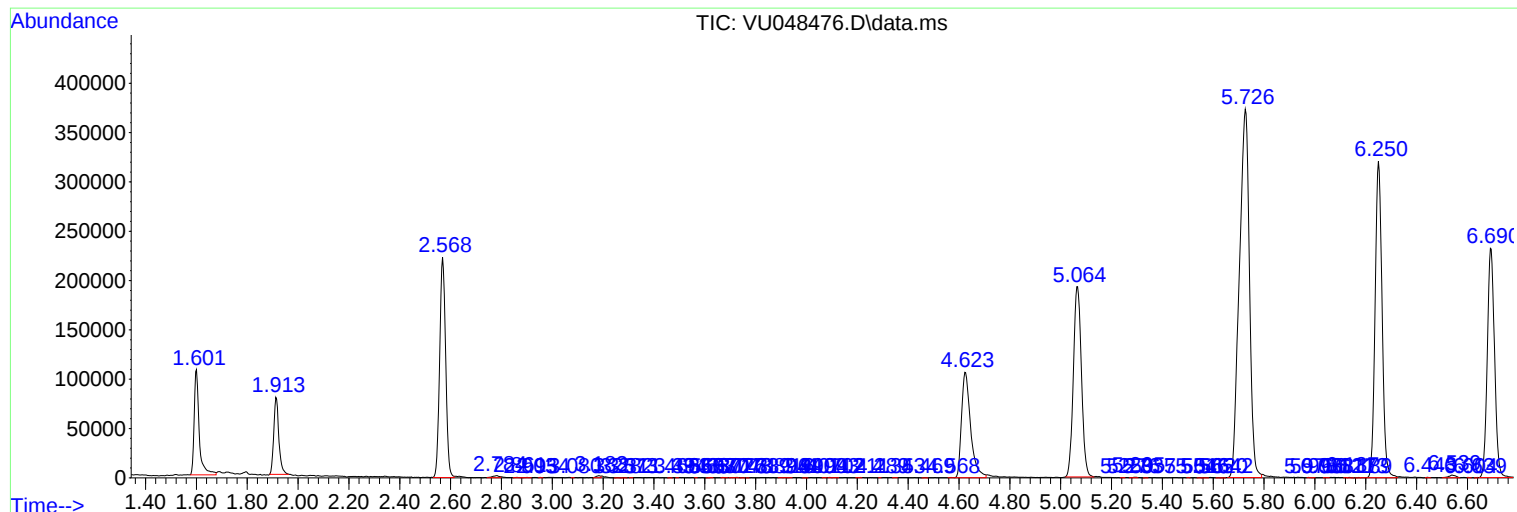

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050622\
Data File : VU048476.D
Acq On : 06 May 2022 23:40
Operator : SY/MD
Sample : N2710-23
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXLB2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050622\
Data File : VU048476.D
Acq On : 06 May 2022 23:40
Operator : SY/MD
Sample : N2710-23
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXLB2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc