


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050622\
 Data File : VU048450.D
 Acq On : 06 May 2022 11:31
 Operator : SY/MD
 Sample : BFB081
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB081

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis
 Last Update : Mon May 09 13:04:47 2022

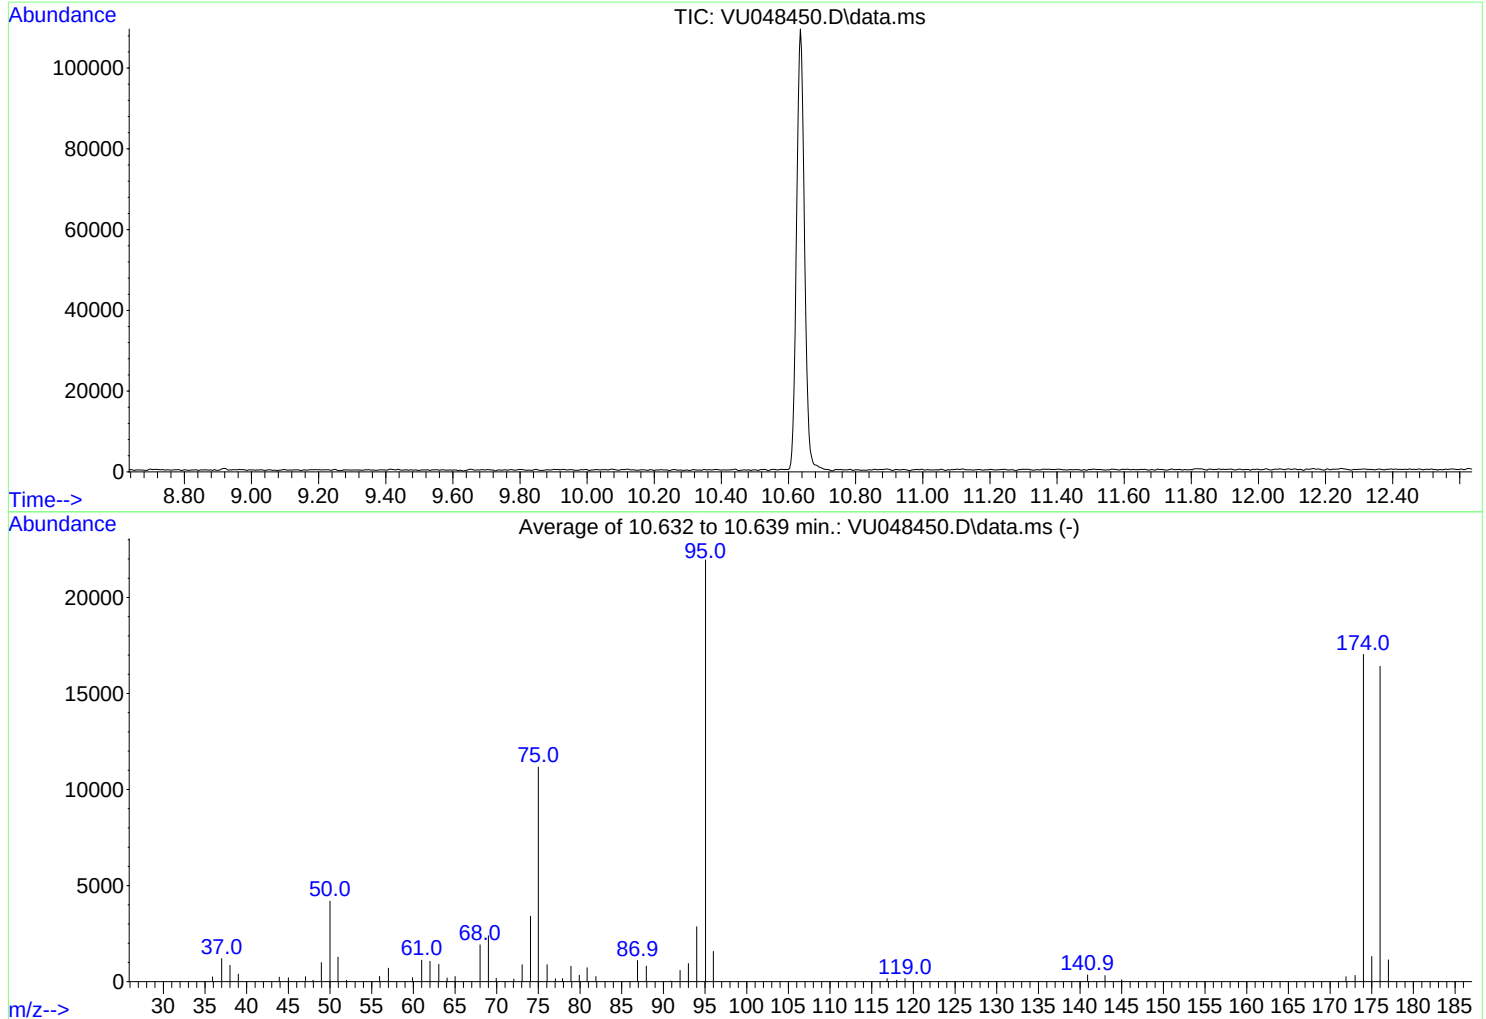

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	4191	PASS
75	95	30	80	50.9	11171	PASS
95	95	100	100	100.0	21955	PASS
96	95	5	9	7.2	1571	PASS
173	174	0.00	2	1.9	327	PASS
174	95	50	120	77.6	17029	PASS
175	174	5	9	7.7	1311	PASS
176	174	95	101	96.4	16418	PASS
177	176	5	9	6.9	1135	PASS

m/z	Abundance
39.90	216.0
43.90	379.0

Instrument :
MSVOA_U
ClientSampleId :
BFB081

m/z	Abundance
35.00	238.0
37.00	1191.0
38.00	898.0
39.00	396.0
40.00	151.0
43.00	653.0
45.00	193.0
47.00	288.0
48.00	112.0
48.00	1040.0
50.00	4214.0
51.00	1326.0
52.00	113.0
55.00	261.0
57.00	685.0
59.00	165.0
61.00	1098.0
62.00	955.0
63.10	1006.0
64.00	200.0
65.00	339.0
68.00	2085.0
69.00	2245.0
70.00	191.0
72.10	106.0
73.10	829.0
74.10	3412.0
75.00	10899.0
76.10	937.0
77.00	170.0
77.00	199.0
78.00	778.0
79.00	313.0
80.00	691.0
81.00	268.0
86.00	1026.0
87.00	777.0
92.00	576.0
93.00	1008.0
94.00	2688.0
95.00	21624.0
96.00	1695.0
116.00	148.0
119.00	138.0
140.00	292.0
143.10	336.0
145.00	159.0
171.00	217.0
173.00	285.0
174.00	16440.0
175.00	1344.0
176.00	15935.0
177.00	1139.0

Instrument :
MSVOA_U
ClientSampleId :
BFB081

m/z	Abundance
35.00	256.0
37.00	1228.0
38.00	866.0
39.00	405.0
40.00	186.0
44.00	619.0
45.00	197.0
47.10	272.0
47.90	107.0
48.90	1016.0
50.00	4371.0
51.00	1284.0
52.00	112.0
55.90	274.0
57.00	736.0
59.90	223.0
61.00	1187.0
62.00	1063.0
63.00	946.0
64.00	202.0
65.00	263.0
68.00	1935.0
69.00	2492.0
70.00	180.0
72.10	148.0
73.00	919.0
74.00	3500.0
75.00	11552.0
76.10	900.0
77.10	159.0
77.90	165.0
78.90	831.0
79.90	347.0
80.90	749.0
81.90	278.0
86.90	1159.0
88.00	849.0
92.00	607.0
93.00	961.0
94.00	2981.0
95.00	22776.0
96.00	1594.0
116.90	157.0
118.00	103.0
119.00	169.0
140.90	355.0
143.00	314.0
145.00	111.0
171.90	266.0
173.00	344.0
174.00	17544.0
175.00	1319.0
176.00	16888.0
177.00	1184.0

Instrument :
MSVOA_U
ClientSampleId :
BFB081

m/z	Abundance
35.90	247.0
37.00	1180.0
38.00	781.0
39.00	377.0
40.00	192.0
44.00	560.0
45.00	198.0
47.10	218.0
49.00	920.0
50.00	3987.0
50.90	1214.0
56.00	289.0
57.00	689.0
59.90	228.0
61.00	1075.0
62.00	1163.0
63.00	754.0
64.10	173.0
65.00	198.0
68.00	1729.0
69.00	2445.0
69.90	167.0
72.00	153.0
73.00	904.0
74.00	3309.0
75.00	11063.0
76.00	801.0
77.10	121.0
77.90	109.0
78.90	788.0
79.90	337.0
80.80	737.0
81.90	244.0
86.90	1102.0
88.00	796.0
90.90	101.0
92.00	575.0
93.00	851.0
94.00	2894.0
95.10	21464.0
96.00	1424.0
116.90	167.0
118.00	112.0
119.00	171.0
140.90	398.0
142.90	296.0
171.90	300.0
173.00	352.0
174.00	17104.0
175.00	1270.0
176.00	16432.0
177.00	1082.0

Instrument :
MSVOA_U
ClientSampleId :
BFB081