
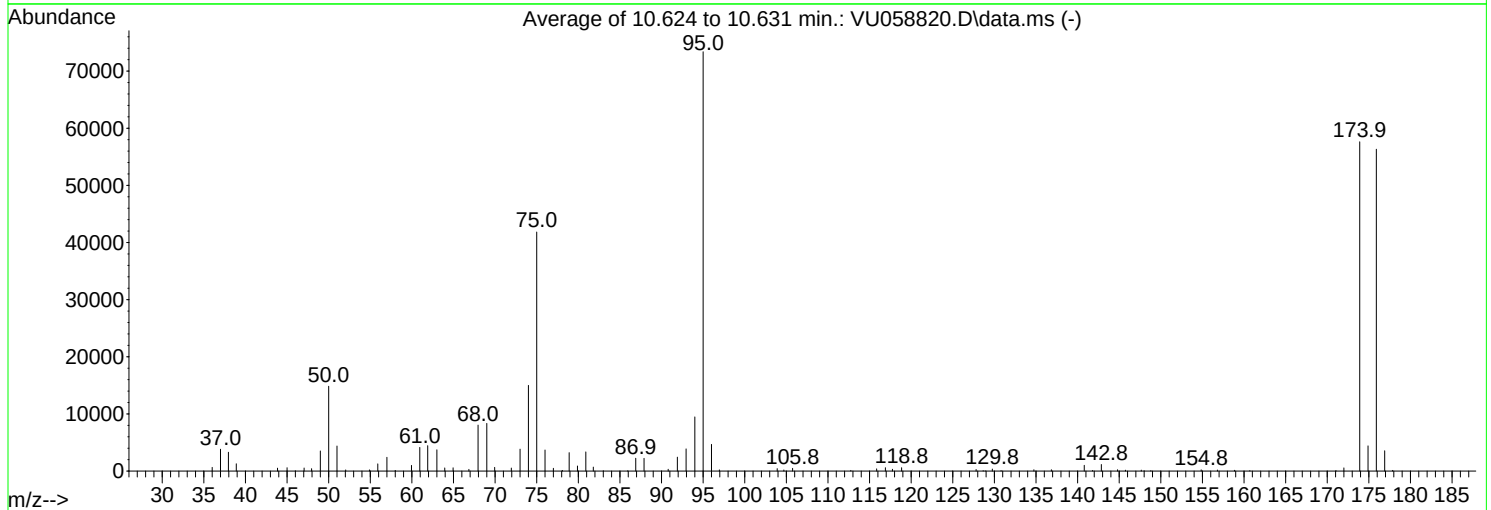


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050624\
Data File : VU058820.D
Acq On : 06 May 2024 08:30
Operator : MD/SY
Sample : BFB151
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB151

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042224WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue May 07 01:07:14 2024

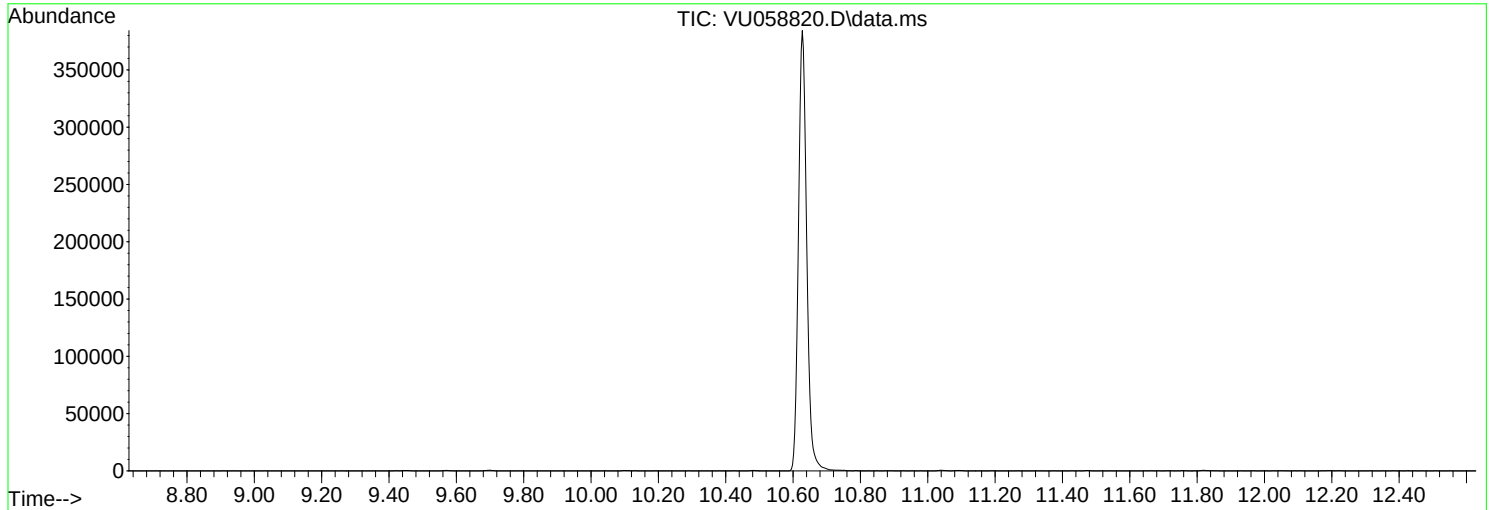

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	14847	PASS
75	95	30	80	57.0	41837	PASS
95	95	100	100	100.0	73392	PASS
96	95	5	9	6.4	4668	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	78.5	57629	PASS
175	174	5	9	7.7	4415	PASS
176	174	95	101	97.7	56328	PASS
177	176	5	9	6.3	3552	PASS

Instrument :
MSVOA_U
ClientSampleId :
BFB151

m/z	Abundance
36.00	624.0
37.00	3671.0
38.00	3304.0
38.90	1280.0
43.90	557.0
45.00	635.0
46.00	101.0
47.10	563.0
47.90	448.0
49.00	3482.0
50.00	14885.0
51.00	4369.0
52.00	217.0
54.90	163.0
55.90	1200.0
57.00	2466.0
58.00	107.0
60.00	963.0
60.90	4156.0
61.90	4408.0
63.00	3629.0
64.00	524.0
64.90	559.0
66.80	317.0
68.00	8080.0
69.00	8434.0
69.90	585.0
72.00	552.0
73.00	3715.0
74.00	14733.0
75.00	41152.0
76.00	3824.0
77.00	512.0
78.90	3244.0
79.90	917.0
80.90	3331.0
81.80	708.0
85.90	106.0
86.90	2192.0
87.90	2184.0
90.80	328.0
91.90	2356.0
93.00	3843.0
94.00	9255.0
95.00	71912.0
96.00	4587.0
96.90	198.0
103.90	436.0
104.70	194.0
105.70	429.0
112.80	107.0
115.90	353.0
116.90	570.0
117.80	329.0
118.90	566.0
127.80	265.0
128.60	106.0
129.80	351.0
130.80	136.0
134.80	215.0
136.80	212.0
140.80	948.0
141.80	120.0
142.90	1163.0
144.80	232.0
145.70	137.0
147.60	144.0
148.00	124.0
148.80	100.0
154.80	232.0
156.80	187.0
158.90	122.0
160.70	142.0
171.10	107.0
172.00	578.0
173.90	55480.0
174.90	4485.0
175.90	54880.0
176.90	3418.0
177.90	124.0

Instrument :
MSVOA_U
ClientSampleId :
BFB151

m/z	Abundance
36.00	683.0
37.00	3973.0
38.00	3387.0
38.90	1301.0
43.90	516.0
45.00	585.0
47.00	552.0
47.90	421.0
49.00	3646.0
50.00	15364.0
51.00	4501.0
52.00	206.0
54.90	216.0
55.90	1309.0
57.00	2510.0
58.00	119.0
59.90	1016.0
60.90	4275.0
61.90	4637.0
63.00	3861.0
64.00	584.0
64.90	589.0
66.80	318.0
68.00	8184.0
69.00	8565.0
70.00	696.0
72.00	555.0
73.00	3932.0
74.00	15438.0
75.00	43016.0
76.00	3817.0
77.00	518.0
78.10	320.0
78.90	3337.0
79.90	900.0
80.90	3461.0
81.80	725.0
86.90	2322.0
87.90	2327.0
90.80	317.0
91.90	2525.0
92.90	4019.0
94.00	9799.0
95.00	75728.0
96.00	4781.0
97.00	211.0
103.90	443.0
104.70	216.0
105.80	501.0
112.80	123.0
115.90	411.0
116.90	598.0
117.80	318.0
118.80	612.0
127.80	286.0
128.70	117.0
129.80	372.0
130.80	121.0
134.80	237.0
136.90	248.0
140.80	1043.0
141.90	114.0
142.80	1186.0
144.80	243.0
145.70	168.0
147.70	178.0
148.80	116.0
154.80	230.0
156.80	193.0
158.80	158.0
160.70	110.0
172.00	575.0
173.90	59144.0
174.90	4540.0
175.90	57808.0
176.90	3666.0
177.80	123.0

Instrument :
MSVOA_U
ClientSampleId :
BFB151

m/z	Abundance
36.00	637.0
37.00	3833.0
37.90	3200.0
38.90	1262.0
43.80	485.0
45.00	545.0
47.00	494.0
48.00	409.0
49.00	3425.0
50.00	14291.0
51.00	4288.0
52.10	184.0
54.90	250.0
55.90	1276.0
57.00	2263.0
58.00	108.0
59.90	1001.0
61.00	4002.0
61.90	4294.0
63.00	3674.0
63.90	532.0
65.00	563.0
66.90	270.0
67.90	7894.0
69.00	8031.0
70.00	661.0
71.90	484.0
73.00	3875.0
74.00	14825.0
75.00	41344.0
76.00	3434.0
77.00	436.0
78.90	3099.0
79.90	865.0
80.90	3262.0
81.80	660.0
83.00	106.0
86.90	2227.0
87.90	2167.0
90.80	307.0
91.90	2433.0
92.90	3781.0
94.00	9396.0
95.00	72536.0
96.00	4637.0
97.00	220.0
103.90	415.0
104.70	170.0
105.80	518.0
112.70	118.0
115.80	406.0
116.90	600.0
117.70	322.0
118.80	605.0
127.80	294.0
128.90	107.0
129.70	353.0
134.70	244.0
136.80	254.0
140.80	1047.0
141.70	100.0
142.90	1115.0
144.80	224.0
145.80	192.0
147.70	200.0
154.90	196.0
156.80	194.0
158.80	146.0
171.00	108.0
172.00	521.0
173.90	58264.0
174.90	4221.0
175.90	56296.0
176.90	3572.0
177.80	122.0

Instrument :
MSVOA_U
ClientSampleId :
BFB151