

Data Path : W:\HPCHEM1\MSVOA U\DATA\VU050718\
 Data File : VU023687.D
 Acq On : 07 May 2018 12:50
 Operator : MD/SY
 Sample : J2627-18
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Quant Time: May 07 14:35:46 2018
 Quant Method : W:\HPCHEM1\MSVOA_U\METHOD\SOMULM050118WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon May 07 00:51:10 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	346407	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	331719	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.49	152	156669	50.00	ug/L	0.00

System Monitoring Compounds


4) Vinyl Chloride-d3	1.40	65	108330	44.12	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	88.24%
7) Chloroethane-d5	1.68	69	90394	48.30	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	96.60%
11) 1,1-Dichloroethene-d2	2.27	63	160567	33.54	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	67.08%
21) 2-Butanone-d5	4.18	46	197640	116.51	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	116.51%
24) Chloroform-d	4.65	84	207298	51.06	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	102.12%
26) 1,2-Dichloroethane-d4	5.31	65	141578	50.14	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	100.28%
32) Benzene-d6	5.35	84	441838	49.64	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.28%
36) 1,2-Dichloropropane-d6	6.34	67	148641	49.86	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	99.72%
41) Toluene-d8	7.57	98	391837	47.75	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	95.50%
43) trans-1,3-Dichloropropene-	7.85	79	60656	47.26	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	94.52%
47) 2-Hexanone-d5	8.31	63	141440	124.94	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	124.94%
57) 1,1,2,2-Tetrachloroethane-	10.44	84	202706	52.57	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	105.14%
64) 1,2-Dichlorobenzene-d4	11.86	152	163962	53.65	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	107.30%


Target Compounds					Ovalue
59) 1,2,3-Trichloropropane	11.49	75	18028	4.874 ug/L	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA U\DATA\VU050718\
Data File : VU023687.D
Acq On : 07 May 2018 12:50
Operator : MD/SY
Sample : J2627-18
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 7 Sample Multiplier: 1

Quant Time: May 07 14:35:46 2018
Quant Method : W:\HPCHEM1\MSVOA_U\METHOD\SOMULM050118WMA.M
Quant Title : VOC Analysis
QLast Update : Mon May 07 00:51:10 2018
Response via : Initial Calibration

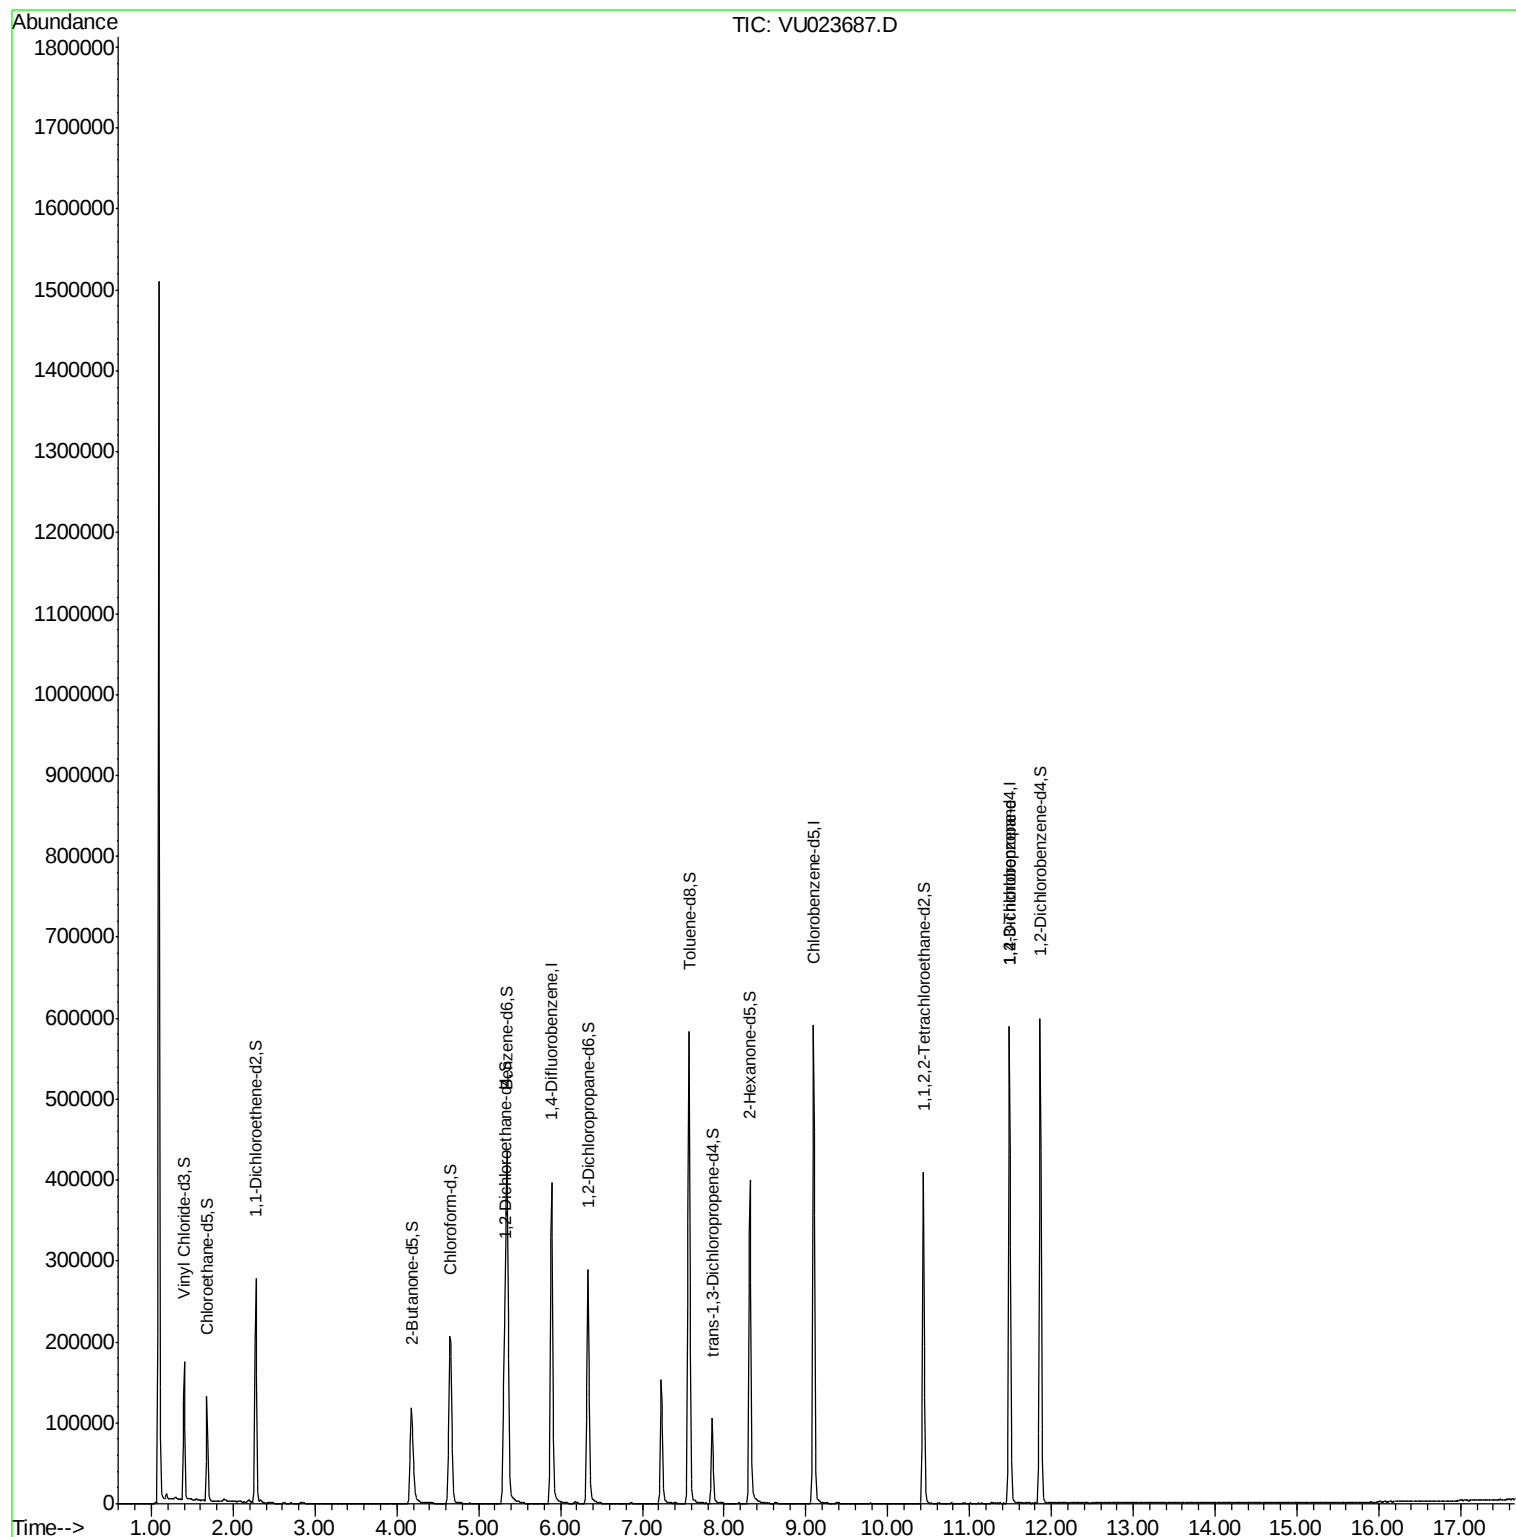

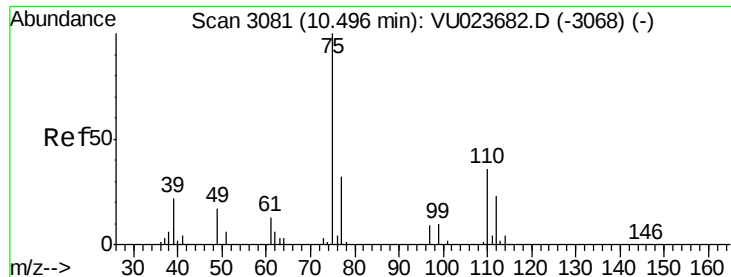

#59

1,2,3-Trichloropropane

Concen: 4.874 ug/L

RT: 11.49 min Scan# 3389

Delta R.T. 0.99 min

Lab File: VU023687.D


Acq: 07 May 2018 12:50

Tot Ion: 75 Resp: 18028

Ion Ratio Lower Upper

75 100

77 37.5 25.9 38.9

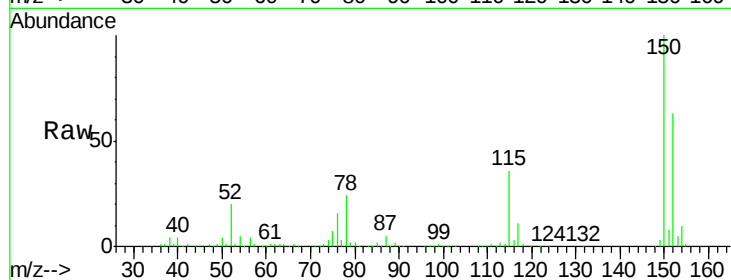

Abundance Ion 75.00 (74.70 to 75.70): VU0

Ion 77.00 (76.70 to 77.70): VU0

