


Data Path : W:\HPCHEM1\MSVOA U\DATA\VU050718\
Data File : VU023704.D
Acq On : 07 May 2018 09:53
Operator : MD/SY
Sample : BFB49
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Integration File: LSCINT.P

Method : W:\HPCHEM1\MSVOA_U\METHOD\SOMULM050118WMA.M
Title : VOC Analysis
Last Update : Tue May 08 04:32:26 2018

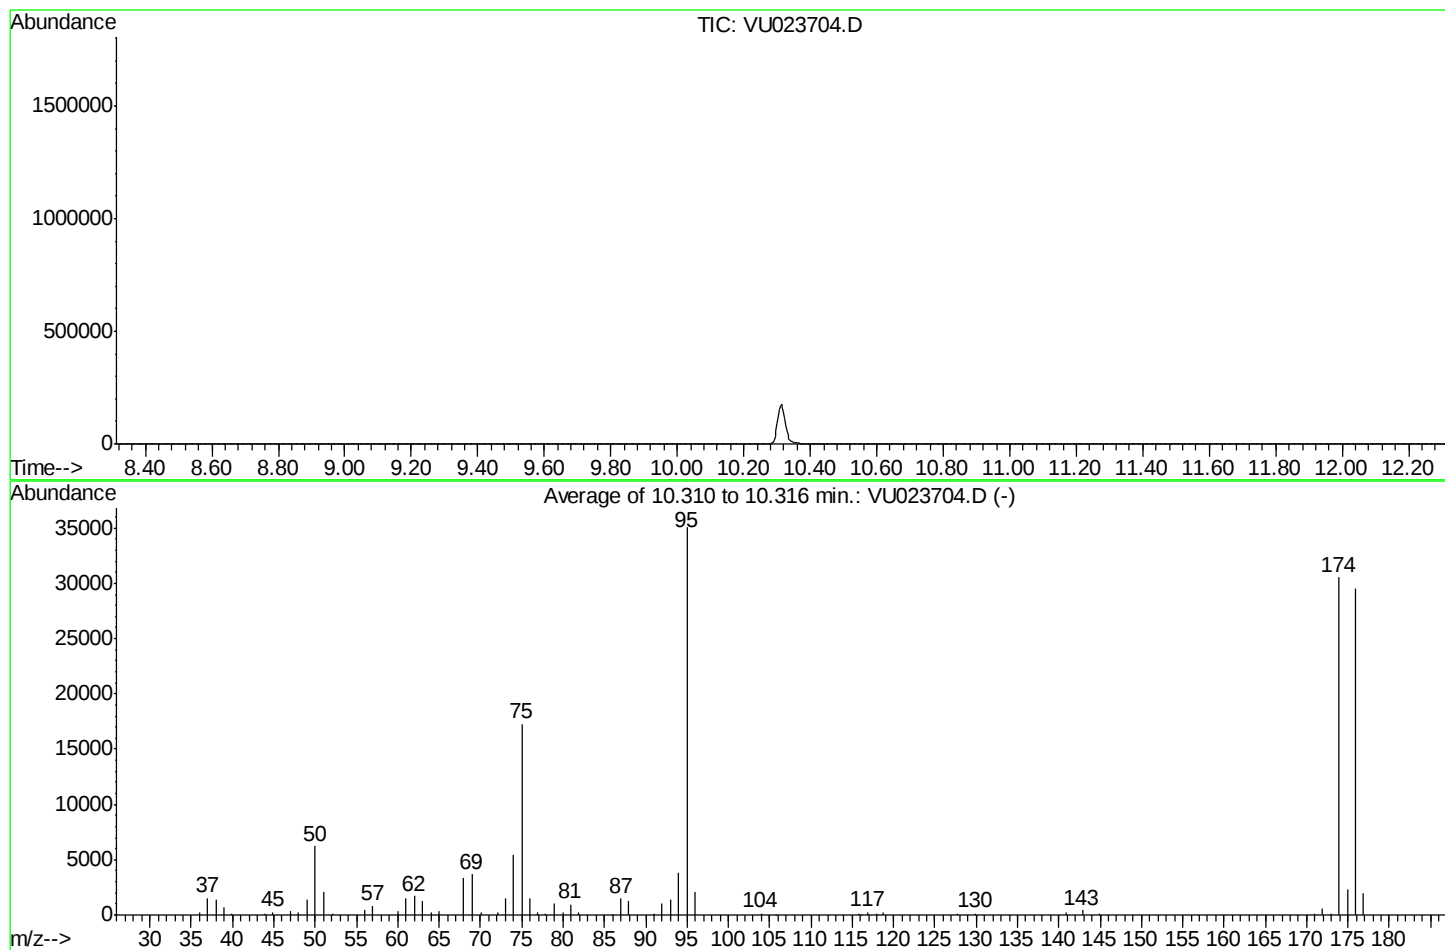

AutoFind: Scans 3023, 3024, 3025; Background Corrected with Scan 3012

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	6216	PASS
75	95	30	80	49.3	17272	PASS
95	95	100	100	100.0	35066	PASS
96	95	5	9	6.0	2111	PASS
173	174	0.00	2	0.4	110	PASS
174	95	50	120	87.0	30517	PASS
175	174	5	9	7.6	2314	PASS
176	174	95	101	96.7	29517	PASS
177	176	5	9	6.5	1921	PASS

Scan 3012 (10.275 min): VU023704.D
BFB49

m/z	Abundance
39.90	148.0
43.90	420.0

m/z	Abundance
36.00	270.0
37.00	1669.0
38.00	1429.0
39.00	644.0
40.00	230.0
44.00	568.0
44.90	316.0
47.00	429.0
47.90	221.0
49.00	1452.0
50.00	6586.0
51.00	2164.0
52.10	134.0
56.00	453.0
57.00	940.0
60.00	310.0
61.00	1627.0
62.00	1680.0
63.00	1305.0
64.10	280.0
65.00	342.0
68.00	3416.0
69.00	3760.0
70.00	214.0
72.10	188.0
73.00	1516.0
74.00	5421.0
75.00	17376.0
76.00	1537.0
76.90	247.0
77.90	136.0
78.90	1039.0
80.00	260.0
80.90	1015.0
81.90	199.0
87.00	1598.0
87.90	1305.0
92.00	1000.0
93.00	1399.0
94.00	3831.0
95.00	35696.0
96.00	2213.0
104.00	172.0
105.80	111.0
115.70	121.0
116.10	108.0
116.90	220.0
118.00	117.0
118.80	256.0
127.70	112.0
129.90	166.0
140.90	314.0
142.90	461.0
144.90	145.0
171.90	505.0
173.90	29760.0
175.00	2306.0
175.90	28992.0
176.90	2069.0

m/z	Abundance
36.00	284.0
37.00	1572.0
38.00	1399.0
39.00	709.0
39.90	254.0
43.90	595.0
44.90	309.0
47.00	393.0
47.90	218.0
49.00	1446.0
50.00	6411.0
51.00	2184.0
52.10	121.0
56.00	470.0
57.00	902.0
60.00	306.0
61.00	1565.0
62.00	1732.0
63.00	1352.0
64.00	261.0
65.00	391.0
68.00	3442.0
69.00	3800.0
70.00	210.0
72.10	197.0
73.00	1617.0
74.00	5666.0
75.00	17784.0
76.00	1592.0
77.00	279.0
77.90	129.0
78.90	1089.0
79.90	272.0
80.90	980.0
81.90	211.0
87.00	1528.0
87.90	1256.0
91.00	128.0
92.00	1103.0
93.00	1418.0
94.00	3910.0
95.00	36008.0
96.00	2163.0
104.00	154.0
115.70	153.0
116.90	256.0
118.00	112.0
118.80	244.0
127.70	109.0
129.90	171.0
140.90	282.0
142.90	431.0
144.90	147.0
170.90	100.0
171.90	544.0
173.90	31512.0
175.00	2390.0
175.90	30608.0
176.90	1972.0

m/z	Abundance
35.90	270.0
37.00	1330.0
38.00	1280.0
39.00	714.0
39.90	269.0
43.90	587.0
44.90	252.0
47.00	405.0
48.00	222.0
49.00	1376.0
50.00	5653.0
51.00	1925.0
52.00	102.0
56.00	435.0
57.00	761.0
60.00	294.0
61.00	1405.0
62.00	1656.0
63.00	1299.0
64.00	215.0
65.00	401.0
68.00	3117.0
69.00	3410.0
70.10	218.0
72.00	183.0
73.00	1514.0
74.00	5320.0
75.00	16656.0
76.00	1533.0
77.00	257.0
77.90	140.0
78.90	1041.0
79.90	263.0
80.90	884.0
81.90	203.0
85.90	114.0
87.00	1389.0
87.90	1182.0
91.00	118.0
92.00	1069.0
93.00	1359.0
94.00	3684.0
95.00	33496.0
96.00	1958.0
104.00	128.0
115.80	123.0
116.90	248.0
117.90	120.0
118.80	200.0
129.90	136.0
141.00	256.0
142.90	411.0
144.90	134.0
170.90	100.0
171.90	534.0
173.00	330.0
173.90	30280.0
175.00	2247.0
175.90	28952.0
176.90	1723.0