

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050719\
 Data File : VU031798.D
 Acq On : 07 May 2019 12:43
 Operator : JC/SP
 Sample : K2705-05DL 10X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B44DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	25	28	36	rVB3	13624	13764	0.47%	0.060%
2	1.283	55	60	68	rBV3	27378	33174	1.13%	0.144%
3	1.395	88	95	110	rBV	398736	442736	15.06%	1.927%
4	1.678	176	183	195	rVB	279928	344151	11.71%	1.498%
5	2.267	355	366	381	rBV	643403	1010288	34.36%	4.397%
6	2.829	535	541	548	rBV5	2527	4703	0.16%	0.020%
7	2.968	579	584	585	rBV	2797	2147	0.07%	0.009%
8	2.981	585	588	590	rVV3	4504	3774	0.13%	0.016%
9	2.997	590	593	603	rVV7	5114	5865	0.20%	0.026%
10	3.125	630	633	638	rVB5	1601	1177	0.04%	0.005%
11	3.170	643	647	650	rBV4	1174	918	0.03%	0.004%
12	3.199	654	656	662	rVB5	950	793	0.03%	0.003%
13	3.312	687	691	694	rVV4	1538	1341	0.05%	0.006%
14	3.498	745	749	753	rVB2	1221	869	0.03%	0.004%
15	3.521	753	756	763	rBV3	1083	1279	0.04%	0.006%
16	3.595	776	779	784	rVB3	1557	1566	0.05%	0.007%
17	3.624	784	788	790	rBV2	848	762	0.03%	0.003%
18	3.646	790	795	798	rVB3	1104	905	0.03%	0.004%
19	3.672	798	803	806	rBV2	836	1015	0.03%	0.004%
20	4.003	902	906	910	rBV2	1441	964	0.03%	0.004%
21	4.093	930	934	937	rVB2	1298	1114	0.04%	0.005%
22	4.116	937	941	942	rBV	1236	774	0.03%	0.003%
23	4.218	950	973	1017	rBV2	478870	1818242	61.85%	7.913%
24	4.550	1074	1076	1086	rVB8	1893	2215	0.08%	0.010%
25	4.643	1086	1105	1134	rBV	469053	1138405	38.72%	4.954%
26	4.804	1153	1155	1159	rVB4	1881	1055	0.04%	0.005%
27	4.842	1164	1167	1169	rBV2	1472	1108	0.04%	0.005%
28	4.871	1172	1176	1177	rBV3	1588	1068	0.04%	0.005%
29	4.984	1204	1211	1218	rBV4	2089	2972	0.10%	0.013%
30	5.054	1230	1233	1239	rVB5	1218	816	0.03%	0.004%
31	5.138	1256	1259	1261	rBV2	1029	775	0.03%	0.003%
32	5.228	1285	1287	1293	rVB4	1257	1042	0.04%	0.005%
33	5.334	1293	1320	1357	rBV2	970429	2939989	100.00%	12.795%
34	5.620	1406	1409	1414	rBV5	1636	1368	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050719\
 Data File : VU031798.D
 Acq On : 07 May 2019 12:43
 Operator : JC/SP
 Sample : K2705-05DL 10X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B44DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	5.749	1443	1449	1452	rBV5	1940	1667	0.06%	0.007%
36	5.826	1470	1473	1475	rBV4	1149	922	0.03%	0.004%
37	5.884	1477	1491	1516	rBV2	817265	1688483	57.43%	7.348%
38	6.183	1571	1584	1606	rBV2	307881	639274	21.74%	2.782%
39	6.328	1615	1629	1654	rBV	659349	1344867	45.74%	5.853%
40	6.630	1720	1723	1725	rBV3	1528	901	0.03%	0.004%
41	6.781	1766	1770	1773	rVB3	1449	1089	0.04%	0.005%
42	6.807	1776	1778	1783	rVB4	1255	963	0.03%	0.004%
43	7.045	1846	1852	1856	rVV4	1026	1474	0.05%	0.006%
44	7.090	1862	1866	1869	rBV4	818	767	0.03%	0.003%
45	7.225	1897	1908	1935	rBV	325970	625455	21.27%	2.722%
46	7.562	2000	2013	2042	rBV	1120540	2066731	70.30%	8.995%
47	7.849	2091	2102	2122	rBV	224900	411679	14.00%	1.792%
48	8.099	2178	2180	2185	rVB3	1657	1101	0.04%	0.005%
49	8.228	2218	2220	2226	rVB6	1659	1210	0.04%	0.005%
50	8.312	2235	2246	2292	rBV	861956	1754527	59.68%	7.636%
51	8.543	2315	2318	2321	rVB2	1564	853	0.03%	0.004%
52	8.803	2394	2399	2402	rVB4	1212	1134	0.04%	0.005%
53	8.842	2406	2411	2414	rVV5	1800	1505	0.05%	0.007%
54	8.871	2417	2420	2425	rVB5	1710	1325	0.05%	0.006%
55	8.897	2425	2428	2431	rBV2	1755	1346	0.05%	0.006%
56	8.938	2439	2441	2446	rVB3	1114	925	0.03%	0.004%
57	8.996	2453	2459	2464	rBV5	1097	1384	0.05%	0.006%
58	9.019	2464	2466	2471	rVB	1317	858	0.03%	0.004%
59	9.086	2471	2487	2527	rBV	1222404	2148107	73.07%	9.349%
60	9.360	2567	2572	2573	rBV3	1252	1083	0.04%	0.005%
61	9.402	2582	2585	2590	rVB4	1184	919	0.03%	0.004%
62	9.569	2631	2637	2638	rBV	1289	947	0.03%	0.004%
63	9.607	2647	2649	2653	rVB3	1266	771	0.03%	0.003%
64	9.675	2668	2670	2674	rVV2	1436	967	0.03%	0.004%
65	9.697	2674	2677	2681	rVB3	1189	870	0.03%	0.004%
66	9.742	2688	2691	2698	rVB4	2038	2265	0.08%	0.010%
67	9.781	2698	2703	2707	rBV4	1264	1350	0.05%	0.006%
68	9.819	2707	2715	2717	rBV4	1469	1381	0.05%	0.006%
69	9.874	2728	2732	2737	rVB5	1655	1488	0.05%	0.006%
70	9.938	2749	2752	2754	rBV4	965	756	0.03%	0.003%
71	9.987	2764	2767	2769	rBV	1357	1000	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050719\
 Data File : VU031798.D
 Acq On : 07 May 2019 12:43
 Operator : JC/SP
 Sample : K2705-05DL 10X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B44DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	10.128	2810	2811	2815	rVB2	1572	865	0.03%	0.004%
73	10.192	2826	2831	2834	rBV3	923	922	0.03%	0.004%
74	10.373	2884	2887	2889	rBV3	1398	946	0.03%	0.004%
75	10.427	2892	2904	2922	rBV	815246	1314520	44.71%	5.721%
76	10.604	2956	2959	2965	rVB4	1879	1429	0.05%	0.006%
77	10.659	2973	2976	2981	rBV3	1357	1121	0.04%	0.005%
78	10.713	2989	2993	2997	rVB5	918	872	0.03%	0.004%
79	10.993	3078	3080	3086	rVB5	1834	1646	0.06%	0.007%
80	11.022	3086	3089	3091	rBV	1412	983	0.03%	0.004%
81	11.180	3136	3138	3142	rBV3	1325	1246	0.04%	0.005%
82	11.218	3148	3150	3154	rVB	1137	755	0.03%	0.003%
83	11.244	3154	3158	3159	rBV2	1276	956	0.03%	0.004%
84	11.302	3173	3176	3179	rBV3	1910	1240	0.04%	0.005%
85	11.376	3196	3199	3204	rBV2	1905	1821	0.06%	0.008%
86	11.418	3209	3212	3216	rBV2	1167	942	0.03%	0.004%
87	11.482	3220	3232	3251	rBV	963425	1563708	53.19%	6.805%
88	11.855	3336	3348	3373	rBV	926986	1573730	53.53%	6.849%
89	12.678	3601	3604	3607	rBV3	1283	786	0.03%	0.003%
90	12.906	3670	3675	3678	rBV6	1715	2177	0.07%	0.009%
91	12.954	3687	3690	3694	rBV3	1033	782	0.03%	0.003%
92	12.977	3694	3697	3701	rVB3	1333	989	0.03%	0.004%
93	13.025	3709	3712	3715	rBV5	1261	1028	0.03%	0.004%
94	13.067	3722	3725	3729	rBV3	1678	1552	0.05%	0.007%
95	13.218	3768	3772	3775	rVB2	1259	1100	0.04%	0.005%
96	13.260	3782	3785	3788	rVB3	1560	912	0.03%	0.004%
97	13.395	3824	3827	3830	rBV2	1541	1051	0.04%	0.005%
98	13.527	3865	3868	3872	rBV3	1606	1501	0.05%	0.007%
99	13.813	3954	3957	3960	rBV	1676	1215	0.04%	0.005%
100	13.970	4003	4006	4008	rBV2	1505	1038	0.04%	0.005%


Sum of corrected areas: 22977311

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU050719\
Data File : VU031798.D
Acq On : 07 May 2019 12:43
Operator : JC/SP
Sample : K2705-05DL 10X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B44DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

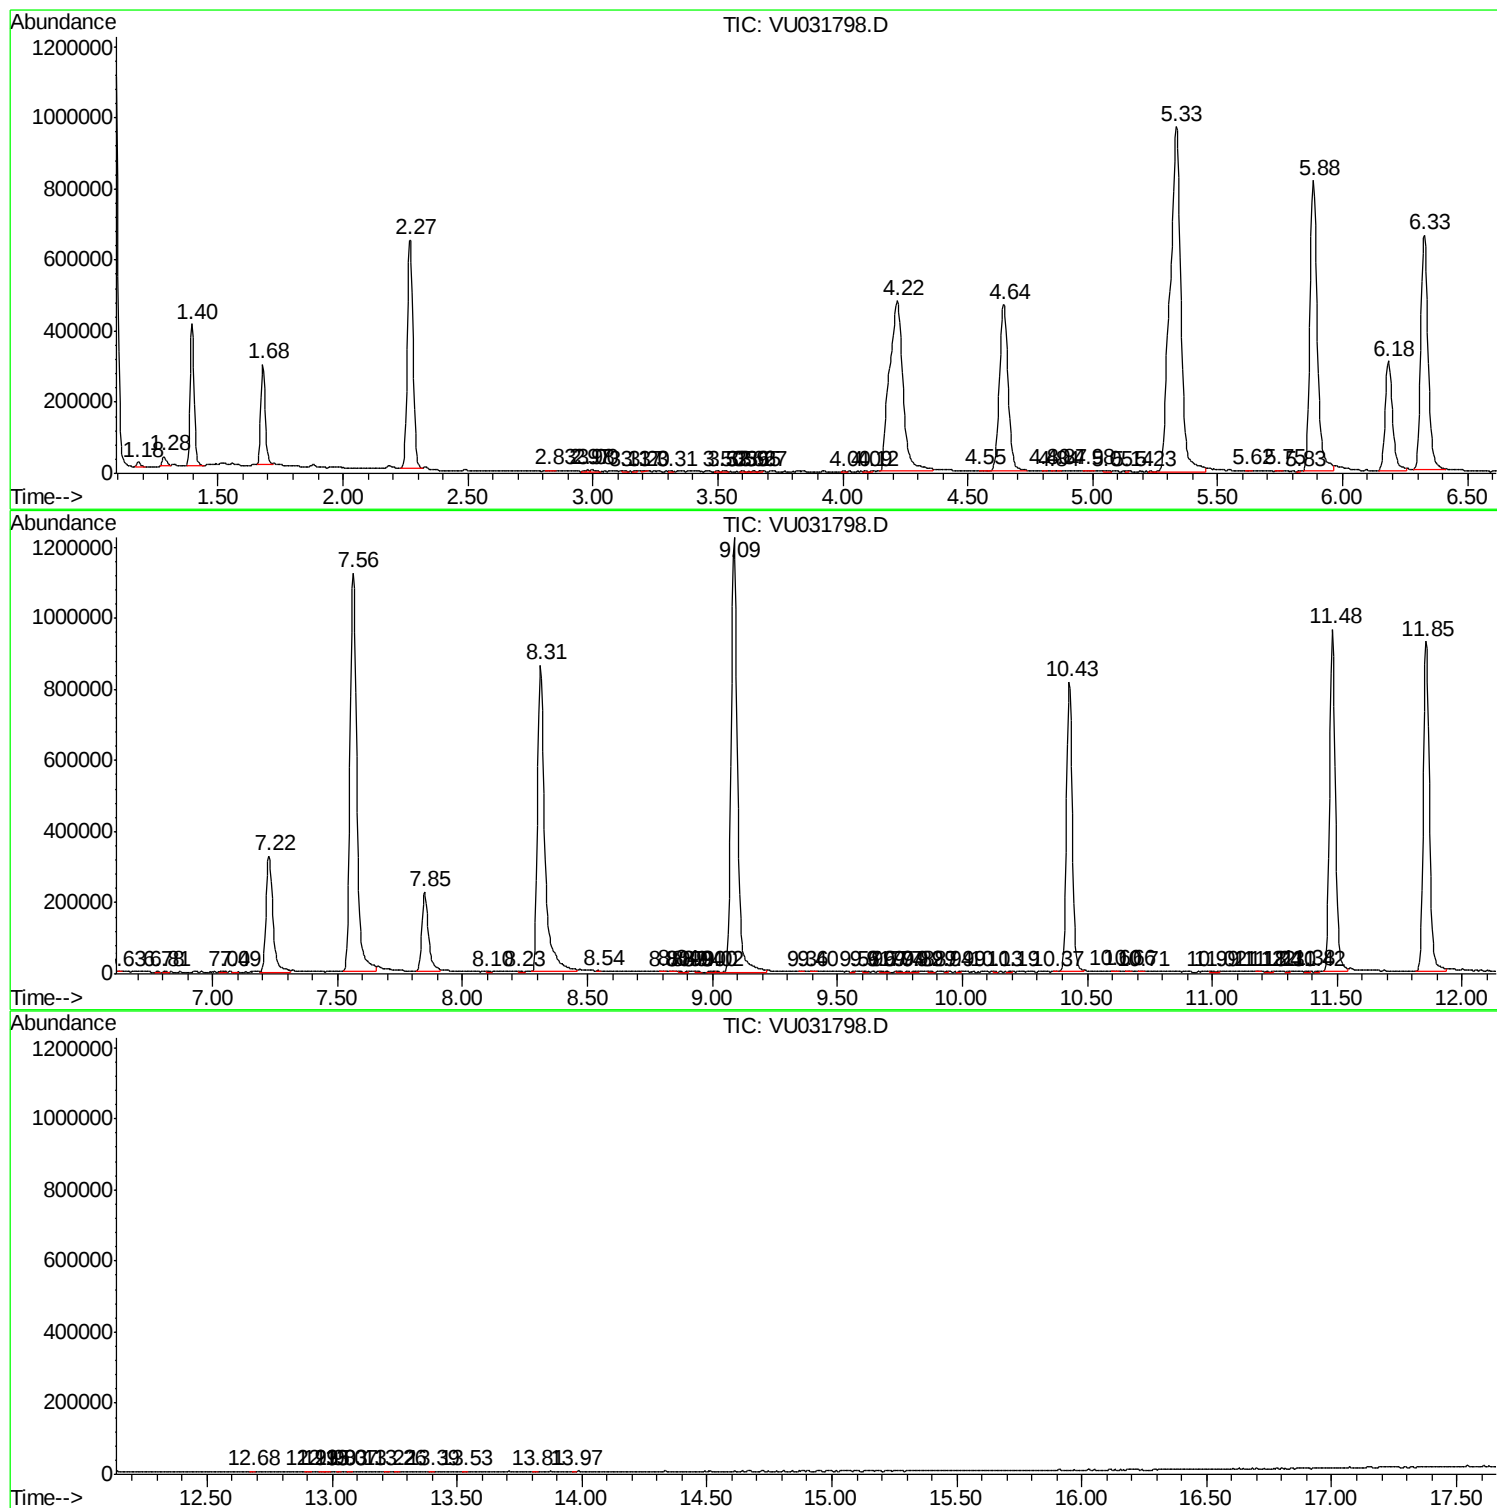

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU050719\
Data File : VU031798.D
Acq On : 07 May 2019 12:43
Operator : JC/SP
Sample : K2705-05DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B44DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_U\DATA\VU050719\
Data File : VU031798.D
Acq On : 07 May 2019 12:43
Operator : JC/SP
Sample : K2705-05DL 10X
Misc : 5.0mL/MSV0A_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSV0A_U
ClientSampleId :
C0B44DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc