

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050719\
 Data File : VU031800.D
 Acq On : 07 May 2019 13:30
 Operator : JC/SP
 Sample : K2705-07
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B46

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	24	28	37	rVB2	20228	19179	0.66%	0.093%
2	1.396	88	95	106	rVB	396036	433600	14.98%	2.103%
3	1.675	175	182	201	rVB	288140	368403	12.73%	1.786%
4	2.267	356	366	380	rVB	618812	954140	32.96%	4.627%
5	2.495	423	437	438	rBV2	35238	61895	2.14%	0.300%
6	2.740	511	513	517	rVB4	1532	919	0.03%	0.004%
7	2.797	528	531	533	rBV2	1086	650	0.02%	0.003%
8	2.833	535	542	551	rVV4	6599	13246	0.46%	0.064%
9	2.926	567	571	577	rVV4	951	1238	0.04%	0.006%
10	2.997	581	593	609	rVV3	20200	48766	1.68%	0.236%
11	3.058	609	612	615	rVB2	1047	581	0.02%	0.003%
12	3.080	617	619	623	rVB2	1236	754	0.03%	0.004%
13	3.103	623	626	628	rBV2	1438	827	0.03%	0.004%
14	3.164	638	645	646	rBV2	2023	2147	0.07%	0.010%
15	3.187	646	652	667	rVB5	6696	13270	0.46%	0.064%
16	3.273	674	679	685	rVB5	1638	2182	0.08%	0.011%
17	3.309	685	690	695	rVB4	1580	1441	0.05%	0.007%
18	3.428	725	727	730	rVB4	1005	553	0.02%	0.003%
19	3.453	730	735	742	rBV5	1848	2365	0.08%	0.011%
20	3.495	742	748	750	rBV4	1232	1305	0.05%	0.006%
21	3.579	771	774	778	rBV4	995	798	0.03%	0.004%
22	3.637	789	792	796	rVB2	1179	788	0.03%	0.004%
23	3.672	799	803	809	rVB2	1347	1298	0.04%	0.006%
24	3.701	809	812	813	rBV	1290	785	0.03%	0.004%
25	3.736	820	823	825	rVB2	1069	601	0.02%	0.003%
26	3.791	837	840	845	rBV2	855	672	0.02%	0.003%
27	3.875	862	866	872	rBV5	1235	1215	0.04%	0.006%
28	3.920	877	880	883	rVB2	1515	985	0.03%	0.005%
29	3.939	883	886	889	rBV4	785	694	0.02%	0.003%
30	3.961	889	893	898	rVB3	1169	1126	0.04%	0.005%
31	4.016	907	910	914	rBV3	1202	1172	0.04%	0.006%
32	4.129	942	945	947	rBV3	1347	904	0.03%	0.004%
33	4.183	949	962	963	rBV	273477	392992	13.58%	1.906%
34	4.556	1074	1078	1079	rBV3	1389	834	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050719\
 Data File : VU031800.D
 Acq On : 07 May 2019 13:30
 Operator : JC/SP
 Sample : K2705-07
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B46

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	4.643	1087	1105	1128	rBV	463049	1098888	37.96%	5.329%
36	4.842	1164	1167	1170	rBV3	1385	1294	0.04%	0.006%
37	4.942	1195	1198	1200	rBV4	1077	621	0.02%	0.003%
38	4.958	1200	1203	1206	rVV2	1178	853	0.03%	0.004%
39	4.987	1209	1212	1214	rBV4	1483	921	0.03%	0.004%
40	5.039	1225	1228	1230	rVB2	1080	605	0.02%	0.003%
41	5.084	1240	1242	1245	rBV2	766	574	0.02%	0.003%
42	5.145	1259	1261	1266	rVB3	1025	713	0.02%	0.003%
43	5.183	1271	1273	1277	rVB3	1193	733	0.03%	0.004%
44	5.209	1277	1281	1282	rBV2	1059	700	0.02%	0.003%
45	5.334	1297	1320	1358	rBV2	941346	2894850	100.00%	14.038%
46	5.723	1438	1441	1443	rBV3	1508	811	0.03%	0.004%
47	5.881	1477	1490	1516	rBV	805233	1668576	57.64%	8.091%
48	6.180	1574	1583	1599	rVB	15245	35116	1.21%	0.170%
49	6.260	1605	1608	1610	rBV3	1511	933	0.03%	0.005%
50	6.325	1615	1628	1653	rBV	651431	1332014	46.01%	6.459%
51	6.678	1730	1738	1741	rBV5	1985	2084	0.07%	0.010%
52	6.727	1750	1753	1756	rBV3	856	579	0.02%	0.003%
53	6.797	1770	1775	1776	rBV3	825	641	0.02%	0.003%
54	6.907	1807	1809	1814	rBV5	844	628	0.02%	0.003%
55	7.064	1852	1858	1860	rBV4	1561	1378	0.05%	0.007%
56	7.225	1896	1908	1936	rBV2	327669	622866	21.52%	3.020%
57	7.505	1991	1995	1996	rBV2	1272	827	0.03%	0.004%
58	7.563	2000	2013	2053	rBV	1085229	2024849	69.95%	9.819%
59	7.849	2091	2102	2126	rBV2	216315	401699	13.88%	1.948%
60	7.981	2141	2143	2145	rVB	1797	650	0.02%	0.003%
61	8.154	2194	2197	2198	rBV3	1548	915	0.03%	0.004%
62	8.173	2199	2203	2214	rVB5	5023	7219	0.25%	0.035%
63	8.312	2234	2246	2284	rBV2	836877	1690536	58.40%	8.198%
64	8.791	2390	2395	2397	rBV5	1157	886	0.03%	0.004%
65	8.826	2403	2406	2408	rBV4	1414	1084	0.04%	0.005%
66	8.878	2419	2422	2424	rBV2	1192	931	0.03%	0.005%
67	9.003	2457	2461	2463	rBV3	1172	916	0.03%	0.004%
68	9.087	2474	2487	2530	rBV	1181826	2090151	72.20%	10.136%
69	9.260	2539	2541	2544	rBV4	1518	774	0.03%	0.004%
70	9.276	2544	2546	2552	rVB6	1384	826	0.03%	0.004%
71	9.472	2604	2607	2610	rBV3	1253	870	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050719\
 Data File : VU031800.D
 Acq On : 07 May 2019 13:30
 Operator : JC/SP
 Sample : K2705-07
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B46

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	9.534	2623	2626	2629	rVB3	1521	1026	0.04%	0.005%
73	9.556	2630	2633	2639	rVV4	1303	1361	0.05%	0.007%
74	9.672	2666	2669	2672	rBV3	712	641	0.02%	0.003%
75	9.826	2714	2717	2719	rBV2	1382	644	0.02%	0.003%
76	9.958	2755	2758	2760	rBV	1233	874	0.03%	0.004%
77	10.070	2790	2793	2797	rBV4	1217	1185	0.04%	0.006%
78	10.234	2841	2844	2847	rVB2	2260	1409	0.05%	0.007%
79	10.270	2851	2855	2857	rBV	895	647	0.02%	0.003%
80	10.286	2857	2860	2866	rBV3	1403	1786	0.06%	0.009%
81	10.328	2870	2873	2875	rBV	1286	842	0.03%	0.004%
82	10.427	2891	2904	2926	rBV	800315	1286078	44.43%	6.236%
83	10.611	2955	2961	2965	rBV4	3100	3767	0.13%	0.018%
84	10.691	2984	2986	2988	rBV2	985	558	0.02%	0.003%
85	10.730	2993	2998	3002	rBV4	2154	2349	0.08%	0.011%
86	11.013	3083	3086	3088	rBV2	982	586	0.02%	0.003%
87	11.058	3097	3100	3103	rBV2	895	733	0.03%	0.004%
88	11.132	3120	3123	3125	rBV2	948	613	0.02%	0.003%
89	11.218	3146	3150	3152	rBV2	874	664	0.02%	0.003%
90	11.296	3170	3174	3177	rVB3	1865	1231	0.04%	0.006%
91	11.482	3219	3232	3267	rBV	939455	1549243	53.52%	7.513%
92	11.855	3336	3348	3373	rBV	900726	1531860	52.92%	7.428%
93	12.704	3608	3612	3614	rBV3	2650	1982	0.07%	0.010%
94	12.739	3620	3623	3625	rBV2	1297	710	0.02%	0.003%
95	12.926	3679	3681	3682	rBV2	1199	557	0.02%	0.003%
96	13.408	3828	3831	3834	rBV5	1973	1780	0.06%	0.009%
97	13.993	4011	4013	4021	rVB3	1949	2478	0.09%	0.012%
98	14.048	4026	4030	4034	rBV6	1834	2158	0.07%	0.010%
99	14.099	4044	4046	4048	rBV	1430	671	0.02%	0.003%
100	14.254	4091	4094	4097	rBV3	2345	1756	0.06%	0.009%


Sum of corrected areas: 20622025

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU050719\
Data File : VU031800.D
Acq On : 07 May 2019 13:30
Operator : JC/SP
Sample : K2705-07
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B46

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

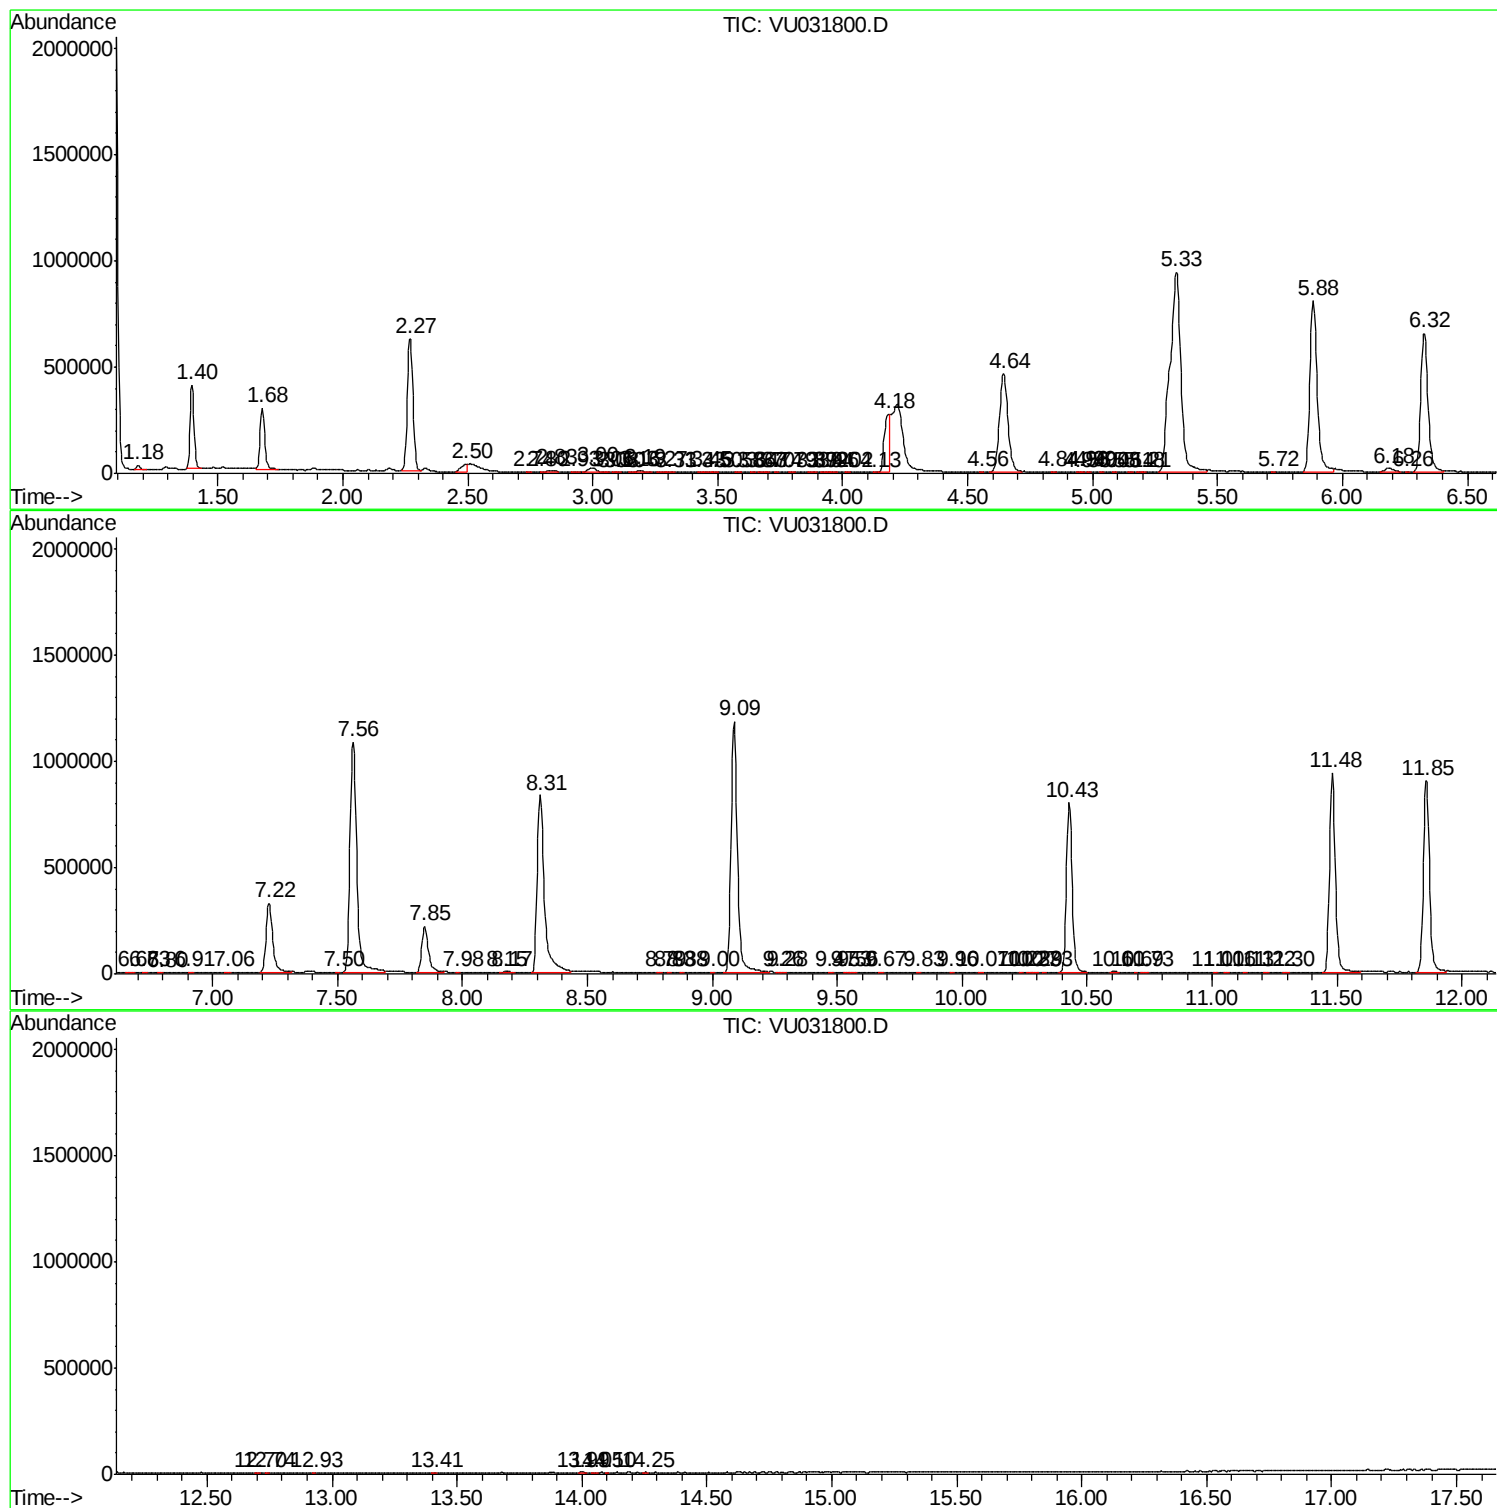

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU050719\
Data File : VU031800.D
Acq On : 07 May 2019 13:30
Operator : JC/SP
Sample : K2705-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B46

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU050719\
Data File : VU031800.D
Acq On : 07 May 2019 13:30
Operator : JC/SP
Sample : K2705-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B46

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc