

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050719\
 Data File : VU031803.D
 Acq On : 07 May 2019 14:40
 Operator : JC/SP
 Sample : K2694-14
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFHK3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.396	88	95	109	rBV	366824	400751	14.05%	1.906%
2	1.679	175	183	203	rVB	279807	366853	12.86%	1.745%
3	2.270	356	367	380	rVB	624290	952465	33.39%	4.529%
4	2.473	422	430	434	rBV5	2185	3445	0.12%	0.016%
5	2.547	451	453	456	rBV3	1194	715	0.03%	0.003%
6	2.720	505	507	511	rBV3	1065	721	0.03%	0.003%
7	2.775	521	524	525	rBV2	1401	801	0.03%	0.004%
8	2.826	534	540	541	rBV2	2086	2049	0.07%	0.010%
9	3.080	616	619	625	rVB5	1037	942	0.03%	0.004%
10	3.161	640	644	648	rVB3	1571	1311	0.05%	0.006%
11	3.190	648	653	656	rBV	1923	1543	0.05%	0.007%
12	3.232	661	666	668	rBV2	1278	1145	0.04%	0.005%
13	3.489	743	746	748	rBV	1292	794	0.03%	0.004%
14	3.630	784	790	792	rBV2	932	955	0.03%	0.005%
15	3.675	800	804	807	rVB3	1331	1146	0.04%	0.005%
16	3.701	807	812	816	rBV4	1068	1046	0.04%	0.005%
17	3.746	823	826	830	rVV2	1465	1056	0.04%	0.005%
18	3.807	842	845	849	rVV2	1623	1152	0.04%	0.005%
19	3.865	858	863	868	rVB4	1415	1684	0.06%	0.008%
20	3.897	868	873	878	rBV3	1550	1990	0.07%	0.009%
21	3.987	896	901	906	rVB6	1361	1477	0.05%	0.007%
22	4.103	931	937	941	rBV3	1554	1718	0.06%	0.008%
23	4.135	943	947	950	rBV2	1250	894	0.03%	0.004%
24	4.183	950	962	990	rBV2	268339	806703	28.28%	3.836%
25	4.534	1068	1071	1074	rVB3	2175	1357	0.05%	0.006%
26	4.553	1074	1077	1082	rBV5	1777	1496	0.05%	0.007%
27	4.643	1089	1105	1136	rBV	478253	1130187	39.62%	5.375%
28	4.981	1206	1210	1212	rBV4	1652	1462	0.05%	0.007%
29	5.045	1228	1230	1234	rVB2	1515	1115	0.04%	0.005%
30	5.074	1234	1239	1242	rBV4	1769	1803	0.06%	0.009%
31	5.145	1255	1261	1266	rVV4	1265	1394	0.05%	0.007%
32	5.212	1278	1282	1284	rBV4	1748	1273	0.04%	0.006%
33	5.257	1293	1296	1298	rBV2	1999	1376	0.05%	0.007%
34	5.334	1298	1320	1344	rBV2	943512	2852628	100.00%	13.566%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\U050719\
 Data File : VU031803.D
 Acq On : 07 May 2019 14:40
 Operator : JC/SP
 Sample : K2694-14
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFHK3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	5.604	1401	1404	1409	rBV5	1873	1839	0.06%	0.009%
36	5.768	1449	1455	1458	rBV6	1501	1545	0.05%	0.007%
37	5.884	1477	1491	1513	rBV	811393	1656039	58.05%	7.875%
38	6.177	1575	1582	1583	rBV5	7502	8013	0.28%	0.038%
39	6.328	1615	1629	1654	rBV	659202	1341990	47.04%	6.382%
40	6.559	1698	1701	1702	rBV3	1538	820	0.03%	0.004%
41	6.682	1735	1739	1743	rBV3	1383	1470	0.05%	0.007%
42	6.768	1762	1766	1770	rBV5	1547	1435	0.05%	0.007%
43	6.981	1828	1832	1836	rBV4	1539	1278	0.04%	0.006%
44	7.077	1857	1862	1865	rBV3	1394	1209	0.04%	0.006%
45	7.109	1868	1872	1876	rVB4	1029	864	0.03%	0.004%
46	7.225	1896	1908	1930	rBV2	322348	615614	21.58%	2.928%
47	7.563	1999	2013	2038	rBV	1098169	2016734	70.70%	9.591%
48	7.849	2091	2102	2126	rBV2	221760	407892	14.30%	1.940%
49	8.112	2181	2184	2187	rVB4	1196	729	0.03%	0.003%
50	8.135	2188	2191	2195	rBV4	860	773	0.03%	0.004%
51	8.241	2222	2224	2228	rVB4	1364	807	0.03%	0.004%
52	8.312	2234	2246	2280	rBV	878412	1762924	61.80%	8.384%
53	8.469	2288	2295	2318	rVB3	49179	101218	3.55%	0.481%
54	8.678	2358	2360	2363	rVB3	1688	965	0.03%	0.005%
55	8.714	2369	2371	2375	rBV4	1368	1118	0.04%	0.005%
56	8.736	2375	2378	2381	rVB3	1937	1293	0.05%	0.006%
57	8.868	2414	2419	2427	rBV7	1498	2919	0.10%	0.014%
58	8.987	2451	2456	2463	rBV5	2356	3560	0.12%	0.017%
59	9.029	2466	2469	2471	rBV2	2418	1649	0.06%	0.008%
60	9.087	2474	2487	2533	rVV	1204934	2101998	73.69%	9.996%
61	9.270	2542	2544	2549	rBV4	1428	1334	0.05%	0.006%
62	9.453	2596	2601	2604	rVB6	1232	1283	0.04%	0.006%
63	9.524	2620	2623	2625	rBV2	1672	1125	0.04%	0.005%
64	9.617	2648	2652	2655	rBV3	1016	966	0.03%	0.005%
65	9.652	2660	2663	2666	rBV2	948	720	0.03%	0.003%
66	9.691	2671	2675	2678	rBV2	2519	1928	0.07%	0.009%
67	9.781	2700	2703	2708	rBV3	1470	1210	0.04%	0.006%
68	9.810	2708	2712	2716	rBV4	2024	1553	0.05%	0.007%
69	10.045	2778	2785	2786	rBV7	3548	3599	0.13%	0.017%
70	10.090	2796	2799	2803	rVB3	1654	1127	0.04%	0.005%
71	10.183	2824	2828	2830	rBV2	1152	920	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050719\
 Data File : VU031803.D
 Acq On : 07 May 2019 14:40
 Operator : JC/SP
 Sample : K2694-14
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFHK3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	10.353	2878	2881	2887	rVB2	1308	1227	0.04%	0.006%
73	10.427	2892	2904	2927	rBV	796314	1294523	45.38%	6.156%
74	10.598	2951	2957	2961	rBV7	3503	4886	0.17%	0.023%
75	10.710	2989	2992	2995	rBV2	1381	898	0.03%	0.004%
76	10.878	3041	3044	3047	rVB2	1187	721	0.03%	0.003%
77	10.968	3067	3072	3074	rBV3	1880	1770	0.06%	0.008%
78	11.061	3097	3101	3104	rBV2	1496	1020	0.04%	0.005%
79	11.087	3106	3109	3115	rBV4	1541	1371	0.05%	0.007%
80	11.119	3116	3119	3121	rBV3	1325	848	0.03%	0.004%
81	11.157	3127	3131	3135	rBV5	1205	1024	0.04%	0.005%
82	11.196	3140	3143	3145	rBV3	1129	833	0.03%	0.004%
83	11.347	3187	3190	3192	rVV4	1392	999	0.04%	0.005%
84	11.382	3196	3201	3208	rBV6	2198	3278	0.11%	0.016%
85	11.482	3220	3232	3256	rBV	956966	1553920	54.47%	7.390%
86	11.810	3332	3334	3335	rBV2	1800	828	0.03%	0.004%
87	11.855	3337	3348	3372	rVV	919546	1544591	54.15%	7.345%
88	12.170	3444	3446	3448	rBV3	1766	961	0.03%	0.005%
89	12.238	3465	3467	3470	rBV3	1586	1018	0.04%	0.005%
90	12.627	3585	3588	3590	rBV	1400	927	0.03%	0.004%
91	12.656	3594	3597	3599	rBV2	1333	905	0.03%	0.004%
92	12.688	3604	3607	3610	rBV2	1278	1162	0.04%	0.006%
93	13.173	3755	3758	3761	rBV	1984	1367	0.05%	0.007%
94	13.273	3786	3789	3790	rBV2	1374	814	0.03%	0.004%
95	13.389	3822	3825	3828	rBV3	1472	1279	0.04%	0.006%
96	13.562	3876	3879	3881	rBV3	1413	905	0.03%	0.004%
97	13.746	3933	3936	3940	rBV2	1497	1304	0.05%	0.006%
98	14.302	4106	4109	4115	rVB4	2234	2147	0.08%	0.010%
99	15.180	4379	4382	4384	rBV3	2005	1556	0.05%	0.007%
100	15.784	4568	4570	4572	rBV2	1866	1084	0.04%	0.005%


Sum of corrected areas: 21028073

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU050719\
Data File : VU031803.D
Acq On : 07 May 2019 14:40
Operator : JC/SP
Sample : K2694-14
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFHK3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

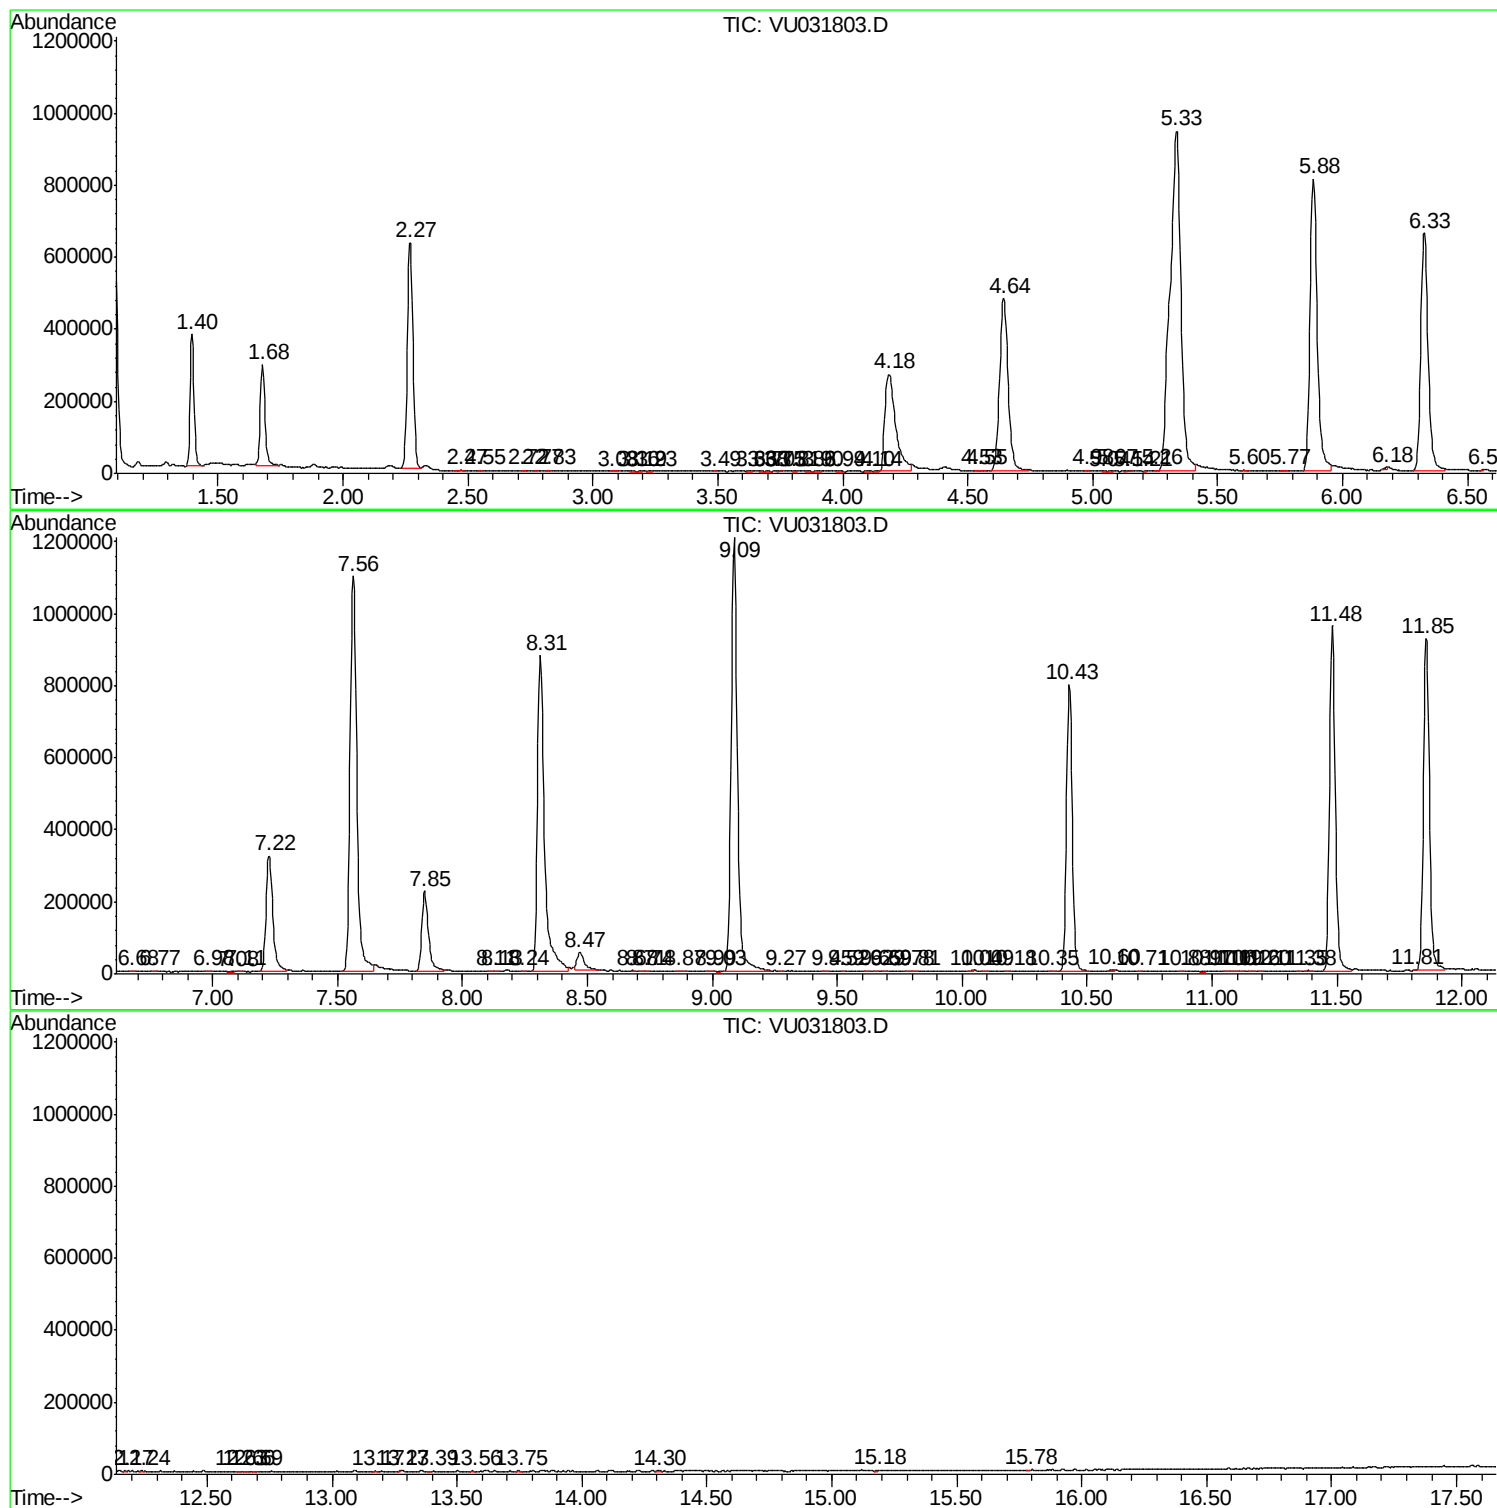

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU050719\
Data File : VU031803.D
Acq On : 07 May 2019 14:40
Operator : JC/SP
Sample : K2694-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFHK3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU050719\
Data File : VU031803.D
Acq On : 07 May 2019 14:40
Operator : JC/SP
Sample : K2694-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFHK3

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc