


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050719\
Data File : VU031792.D
Acq On : 07 May 2019 10:09
Operator : JC/SP
Sample : BFB39
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB39

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Title : VOC Analysis
Last Update : Wed May 08 06:47:54 2019

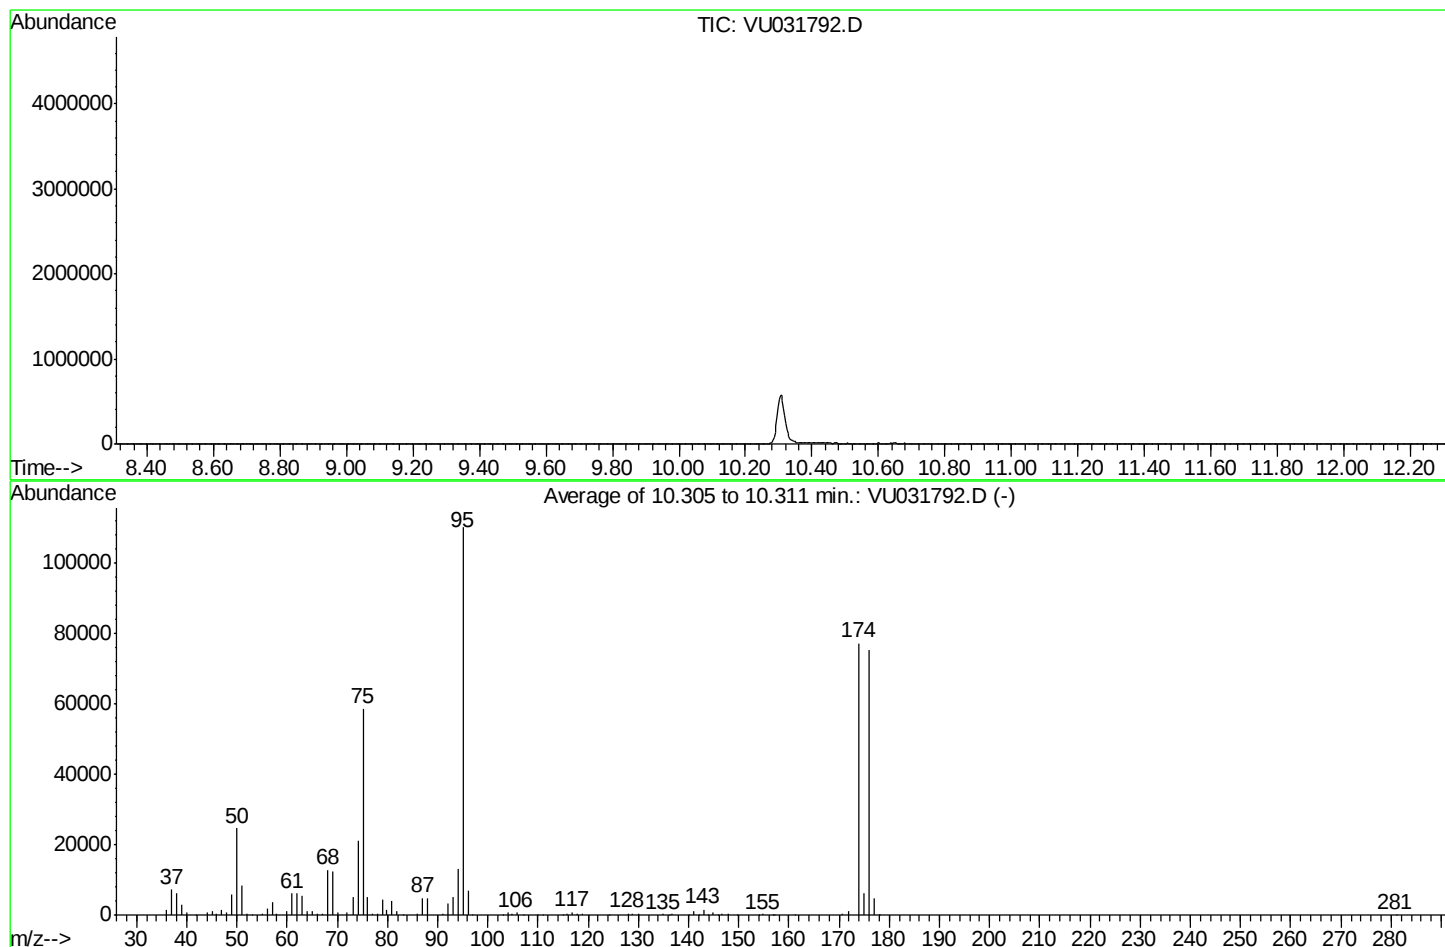

AutoFind: Scans 2866, 2867, 2868; Background Corrected with Scan 2854

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.4	24696	PASS
75	95	30	80	53.3	58680	PASS
95	95	100	100	100.0	110186	PASS
96	95	5	9	6.3	6984	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	70.0	77154	PASS
175	174	5	9	8.0	6200	PASS
176	174	95	101	97.8	75472	PASS
177	176	5	9	6.4	4812	PASS

Scan 2854 (10.266 min): VU031792.D
BFB39

m/z	Abundance
40.00	4224.0
44.00	1730.0

Instrument :
MSVOA_U
ClientSampleId :
BFB39

m/z	Abundance
36.00	1254.0
37.00	7336.0
38.00	6284.0
39.00	3341.0
40.00	4967.0
44.00	2347.0
45.10	1303.0
45.90	189.0
47.00	1832.0
48.10	1104.0
49.00	6346.0
50.00	25776.0
51.00	8820.0
52.00	408.0
53.00	103.0
55.10	470.0
56.00	1889.0
57.00	3663.0
57.90	199.0
60.00	1111.0
61.00	6434.0
62.10	6500.0
63.10	5887.0
64.10	1191.0
65.00	1402.0
66.00	243.0
67.10	408.0
68.10	13644.0
69.00	13639.0
70.00	1002.0
72.00	808.0
73.10	5492.0
74.10	21816.0
75.10	61728.0
76.10	5752.0
77.10	602.0
77.80	216.0
78.90	4696.0
79.90	1406.0
81.00	4539.0
81.90	1260.0
86.00	253.0
87.00	4808.0
88.00	4762.0
91.00	497.0
92.10	3526.0
93.00	5677.0
94.10	13808.0
95.10	113624.0
96.00	7247.0
96.90	140.0
103.00	170.0
103.90	551.0
104.90	282.0
105.80	809.0
115.90	472.0
116.90	942.0
117.80	496.0
118.90	511.0
124.30	100.0
128.00	510.0
128.90	202.0
130.00	238.0
135.00	297.0
136.80	238.0
140.00	110.0
141.00	1256.0
143.00	1652.0
143.80	113.0
144.90	832.0
145.80	204.0
146.80	217.0
148.00	267.0
149.70	152.0
154.10	183.0
154.90	235.0
156.90	119.0
161.00	138.0
170.70	344.0
172.00	1270.0
174.00	80800.0
175.00	6522.0
176.00	77680.0
177.00	5142.0
177.90	125.0
281.00	120.0

Instrument :
MSVOA_U
ClientSampleId :
BFB39

m/z	Abundance
36.00	1348.0
37.00	7431.0
38.00	6555.0
39.00	3082.0
40.00	4972.0
41.70	114.0
44.10	2288.0
45.10	1276.0
45.90	241.0
47.00	1682.0
48.00	948.0
49.00	6043.0
50.00	25192.0
51.00	8506.0
52.00	327.0
53.00	190.0
55.00	448.0
56.10	1748.0
57.00	3571.0
57.90	195.0
60.00	1147.0
61.00	6265.0
62.00	6204.0
63.10	5541.0
64.10	1128.0
65.00	1104.0
66.00	308.0
67.10	388.0
68.10	13303.0
69.00	12751.0
70.00	925.0
72.00	762.0
73.00	5267.0
74.10	21632.0
75.10	60584.0
76.00	5568.0
77.10	554.0
77.90	318.0
78.90	4465.0
79.90	1451.0
81.00	4206.0
81.90	1100.0
83.00	131.0
86.10	279.0
87.00	4986.0
88.00	4910.0
91.00	461.0
92.10	3235.0
93.00	5168.0
94.10	13579.0
95.10	113648.0
96.00	7236.0
96.90	132.0
103.00	137.0
104.00	609.0
104.90	339.0
105.80	762.0
109.80	123.0
111.00	134.0
115.00	106.0
115.80	469.0
116.90	979.0
117.70	559.0
118.90	535.0
127.90	503.0
128.80	208.0
130.00	261.0
135.00	322.0
136.80	212.0
140.00	211.0
141.00	1231.0
142.00	152.0
143.00	1651.0
143.80	114.0
144.90	733.0
145.80	116.0
146.80	192.0
148.00	246.0
154.10	180.0
154.90	220.0
156.90	131.0
161.10	185.0
170.70	430.0
172.00	1316.0
174.00	79360.0
175.00	6557.0
176.00	78096.0
177.00	4872.0
281.00	149.0

Instrument :
MSVOA_U
ClientSampleId :
BFB39

m/z	Abundance
36.00	1308.0
37.00	6720.0
38.10	5993.0
39.00	2612.0
40.00	4924.0
41.70	101.0
44.00	2300.0
45.10	1128.0
45.80	237.0
47.00	1299.0
47.90	703.0
49.00	5117.0
50.10	23120.0
51.00	7451.0
52.00	224.0
53.10	216.0
55.00	384.0
56.10	1451.0
57.10	3219.0
57.90	211.0
60.00	1151.0
61.00	5619.0
62.00	5754.0
63.10	4730.0
64.10	951.0
65.00	871.0
66.00	228.0
67.00	400.0
68.10	11711.0
69.10	11209.0
70.00	768.0
72.00	643.0
73.00	4952.0
74.10	19920.0
75.10	53728.0
76.00	4538.0
77.10	472.0
78.00	399.0
79.00	3984.0
79.90	1377.0
80.90	3493.0
81.90	1092.0
83.10	182.0
86.10	233.0
87.00	4411.0
88.00	4323.0
91.00	367.0
92.00	3003.0
93.00	4397.0
94.10	12078.0
95.10	103288.0
96.10	6471.0
103.90	577.0
104.90	278.0
105.80	542.0
107.00	140.0
109.80	105.0
111.00	158.0
115.00	114.0
115.80	441.0
116.90	821.0
117.80	549.0
119.00	624.0
127.90	452.0
128.80	224.0
130.00	313.0
135.00	278.0
136.10	127.0
136.80	170.0
140.00	247.0
141.00	1162.0
142.00	192.0
143.00	1471.0
144.90	580.0
146.70	207.0
148.00	256.0
154.00	108.0
154.90	218.0
157.10	124.0
161.10	142.0
170.70	370.0
172.00	1218.0
174.00	71304.0
175.00	5523.0
176.00	70640.0
177.00	4424.0
178.10	116.0
281.00	126.0

Instrument :
MSVOA_U
ClientSampleId :
BFB39