


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050720\
 Data File : VU038027.D
 Acq On : 07 May 2020 08:53
 Operator : JC/MD
 Sample : BFB19
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB19

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR050720WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu May 07 10:21:16 2020

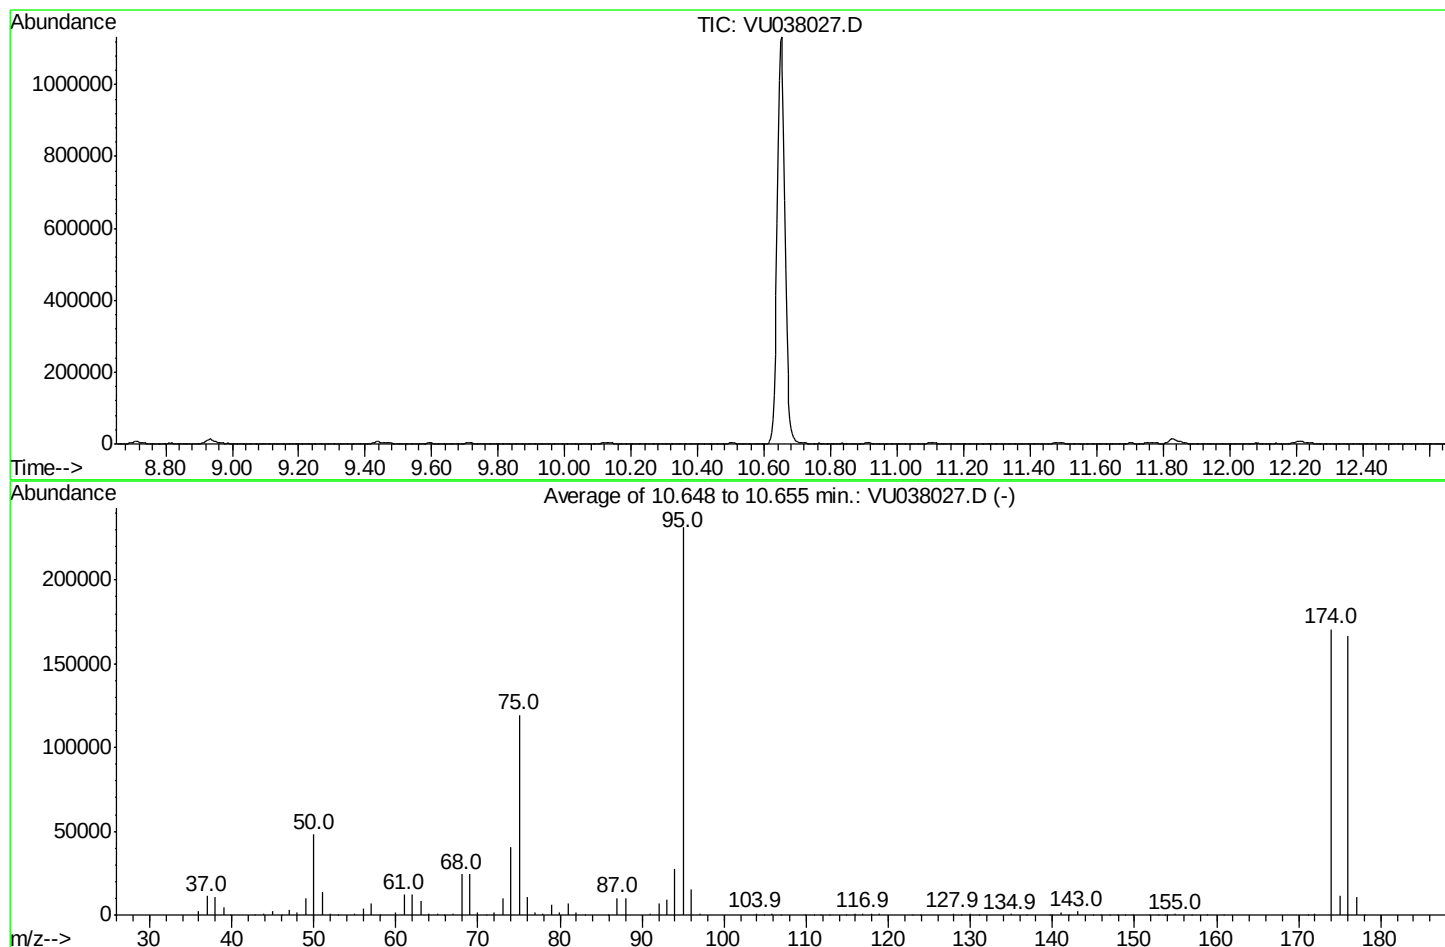

AutoFind: Scans 2895, 2896, 2897; Background Corrected with Scan 2880

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	48037	PASS
75	95	30	80	51.6	119554	PASS
95	95	100	100	100.0	231488	PASS
96	95	5	9	6.7	15433	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	73.7	170517	PASS
175	174	5	9	6.8	11566	PASS
176	174	95	101	97.6	166378	PASS
177	176	5	9	6.3	10530	PASS

m/z	Abundance
36.00	2101.0
37.00	11667.0
38.00	10843.0
39.00	4458.0
39.90	449.0
42.90	173.0
44.00	2401.0
45.00	2278.0
46.20	263.0
47.00	3115.0
47.90	1485.0
49.00	10794.0
50.00	49896.0
51.00	14244.0
52.00	655.0
52.90	102.0
55.00	593.0
56.00	3648.0
57.00	7166.0
58.00	329.0
60.00	1974.0
61.00	12356.0
62.00	12689.0
63.00	8269.0
64.00	957.0
65.10	511.0
66.00	146.0
67.00	751.0
68.00	25048.0
69.00	25224.0
70.00	1933.0
72.00	1291.0
73.00	10431.0
74.00	41392.0
75.00	122600.0
76.00	11335.0
77.00	1388.0
77.90	1253.0
78.90	6639.0
79.90	2053.0
80.90	6996.0
81.90	1362.0
85.80	308.0
87.00	10522.0
88.00	10395.0
91.00	883.0
92.00	6542.0
93.00	10095.0
94.00	27728.0
95.00	237888.0
96.00	15982.0
97.00	494.0
103.90	985.0
104.80	318.0
105.80	959.0
106.90	219.0
109.90	145.0
111.00	100.0
111.70	100.0
112.80	200.0
114.90	251.0
115.90	895.0
116.90	1199.0
117.90	763.0
118.90	908.0
123.90	168.0
127.90	862.0
128.80	306.0
130.00	772.0
131.00	197.0
134.90	441.0
136.90	321.0
139.90	141.0
141.00	1793.0
142.00	280.0
143.00	2207.0
144.90	233.0
145.90	308.0
147.90	331.0
148.80	140.0
149.80	154.0
152.90	155.0
154.00	130.0
155.00	557.0
156.90	350.0
158.90	109.0
160.80	190.0
171.10	189.0
172.00	1126.0
174.00	171392.0
175.00	11704.0
176.00	165504.0

Instrument :
MSVOA_U
ClientSampleId :
BFB19

177.0010657.0

178.00333.0

Instrument :
MSVOA_U
ClientSampleId :
BFB19

m/z	Abundance
36.00	1997.0
37.00	11460.0
38.00	10746.0
39.00	4384.0
39.90	579.0
42.90	143.0
44.00	2205.0
45.00	2408.0
46.10	215.0
47.00	3133.0
47.90	1550.0
49.00	10353.0
50.00	49208.0
51.00	14315.0
52.00	635.0
55.00	604.0
56.00	3702.0
57.00	7249.0
58.00	304.0
59.90	1851.0
61.00	12482.0
62.00	12312.0
63.00	8263.0
64.00	948.0
65.00	476.0
65.90	118.0
67.00	770.0
68.00	25072.0
69.00	25304.0
70.00	1861.0
71.10	112.0
72.00	1383.0
73.00	10296.0
74.00	41488.0
75.00	123368.0
76.00	10805.0
76.90	1364.0
77.90	1099.0
78.90	6631.0
79.90	1967.0
80.90	6857.0
82.00	1339.0
85.80	389.0
87.00	10356.0
88.00	10024.0
91.00	827.0
92.00	6799.0
93.00	9928.0
94.00	28048.0
95.00	238656.0
96.00	15989.0
97.00	491.0
103.90	929.0
104.80	344.0
105.80	860.0
106.90	247.0
109.90	153.0
111.00	124.0
112.90	204.0
114.90	185.0
115.90	853.0
116.90	1103.0
117.90	851.0
118.90	987.0
123.90	156.0
127.90	812.0
128.90	421.0
129.90	796.0
131.00	198.0
134.90	425.0
136.80	332.0
140.00	112.0
141.00	1934.0
142.00	332.0
143.00	2299.0
144.90	261.0
145.90	381.0
146.90	136.0
148.00	362.0
148.80	133.0
149.90	114.0
151.80	103.0
152.90	139.0
153.90	124.0
155.00	603.0
157.00	349.0
160.90	166.0
171.10	195.0
172.00	1102.0
174.00	175872.0
175.00	11845.0
176.00	171968.0

Instrument :
MSVOA_U
ClientSampleId :
BFB19

177.0010863.0

178.00316.0

Instrument :
MSVOA_U
ClientSampleId :
BFB19

m/z	Abundance
35.90	1865.0
37.00	10347.0
38.00	9690.0
39.00	3904.0
39.90	654.0
42.80	112.0
43.90	2072.0
45.00	2280.0
46.00	131.0
47.00	2896.0
47.90	1334.0
49.00	9531.0
50.00	45008.0
51.00	13428.0
52.00	554.0
55.00	589.0
56.00	3490.0
57.00	6608.0
58.00	294.0
59.90	1763.0
61.00	11295.0
62.00	10782.0
63.00	7672.0
64.10	980.0
65.00	468.0
67.00	711.0
68.00	22960.0
69.00	23288.0
69.90	1692.0
71.00	162.0
72.00	1219.0
73.00	9418.0
74.00	38152.0
75.00	112696.0
76.00	9283.0
76.90	1377.0
78.00	868.0
78.90	5916.0
80.00	1745.0
81.00	6024.0
82.00	1269.0
83.10	104.0
85.80	367.0
87.00	9261.0
88.00	8944.0
91.00	744.0
92.00	6367.0
93.00	8708.0
94.00	25976.0
95.00	217920.0
96.00	14330.0
97.00	463.0
103.90	784.0
104.80	322.0
105.80	721.0
106.90	221.0
109.90	116.0
111.00	174.0
112.90	166.0
114.90	156.0
115.90	744.0
116.90	1026.0
117.90	799.0
118.90	1049.0
122.90	111.0
124.00	142.0
127.90	684.0
128.90	416.0
129.90	745.0
131.00	193.0
135.00	375.0
136.80	311.0
139.60	111.0
140.10	100.0
141.00	1822.0
142.00	287.0
143.00	2026.0
144.90	274.0
145.90	353.0
146.90	150.0
148.00	366.0
148.80	112.0
151.80	107.0
152.90	111.0
153.70	101.0
155.00	534.0
157.00	280.0
160.80	137.0
171.10	140.0
172.00	855.0
174.00	164288.0
175.00	11150.0

Instrument :
MSVOA_U
ClientSampleId :
BFB19

176.00161664.0

177.0010071.0

178.00273.0

Instrument :
MSVOA_U

ClientSampleId :
BFB19

Scan 2880 (10.600 min): VU038027.D
BFB19

m/z	Abundance
40.00	274.0
43.90	1336.0

Instrument :
MSVOA_U
ClientSampleId :
BFB19