

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050721\
 Data File : VU043605.D
 Acq On : 07 May 2021 12:29
 Operator : SY/MD
 Sample : M2333-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BP-VPB-RW8-TB-20210503

Quant Time: May 08 01:07:09 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U050621W.M
 Quant Title : SW846 8260
 QLast Update : Thu May 06 07:26:23 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.382	168	120650	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.256	114	218005	50.00	ug/l	0.00
63) Chlorobenzene-d5	9.423	117	210372	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.819	152	95242	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.710	65	123268	50.47	ug/l	0.00
Spiked Amount 50.000			Recovery	=	100.94%	
35) Dibromofluoromethane	5.298	113	85264	49.04	ug/l	0.00
Spiked Amount 50.000			Recovery	=	98.08%	
50) Toluene-d8	7.906	98	299066	48.51	ug/l	0.00
Spiked Amount 50.000			Recovery	=	97.02%	
62) 4-Bromofluorobenzene	10.639	95	105504	44.99	ug/l	0.00
Spiked Amount 50.000			Recovery	=	89.98%	
Target Compounds					Qvalue	
3) Chloromethane	1.527	50	675	0.62	ug/l	99
5) Bromomethane	1.854	94	348	0.32	ug/l	85
10) Methyl Iodide	2.735	142	654	0.37	ug/l #	74
11) Tert butyl alcohol	3.192	59	2565	3.91	ug/l #	73
13) Acrolein	2.485	56	21	6.11	ug/l #	14
16) Acetone	2.636	43	1074	0.79	ug/l #	79
17) Carbon Disulfide	2.797	76	1088	0.25	ug/l #	77
20) Methylene Chloride	3.051	84	754	0.40	ug/l	88
23) Vinyl Acetate	3.967	43	113	9.97	ug/l #	78
31) Cyclohexane	5.378	56	3538	1.21	ug/l #	19
36) 1,1-Dichloropropene	5.382	75	11548	4.67	ug/l #	49
38) Carbon Tetrachloride	5.382	117	13287	5.30	ug/l #	17
51) 4-Methyl-2-Pentanone	7.796	43	1493	19.46	ug/l #	80
53) t-1,3-Dichloropropene	8.218	75	76	2.27	ug/l #	1
56) Ethyl methacrylate	8.340	69	163	4.26	ug/l #	24
59) 2-Hexanone	8.687	43	1765	21.11	ug/l	91
67) Ethyl Benzene	9.578	91	353	1.49	ug/l #	45
68) m/p-Xylenes	9.703	106	189	2.39	ug/l #	42
70) Styrene	10.115	104	214	2.73	ug/l #	61
74) N-amyl acetate	10.327	43	712	2.65	ug/l #	62
76) 1,2,3-Trichloropropane	10.639	75	60931	20.12	ug/l #	42
80) 1,3,5-Trimethylbenzene	11.095	105	310	0.78	ug/l #	52
81) trans-1,4-Dichloro-2-b...	10.639	75	60931	65.52	ug/l #	3
84) 1,2,4-Trimethylbenzene	11.475	105	506	1.19	ug/l #	63
85) sec-Butylbenzene	11.645	105	521	1.40	ug/l #	59
86) p-Isopropyltoluene	11.799	119	501	1.54	ug/l	86
89) n-Butylbenzene	12.217	91	956	2.67	ug/l #	73
93) 1,2,4-Trichlorobenzene	13.854	180	911	0.41	ug/l	91
95) Naphthalene	14.095	128	5918	2.23	ug/l	96
96) 1,2,3-Trichlorobenzene	14.339	180	1233	0.55	ug/l	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050721\
Data File : VU043605.D
Acq On : 07 May 2021 12:29
Operator : SY/MD
Sample : M2333-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BP-VPB-RW8-TB-20210503

Quant Time: May 08 01:07:09 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U050621W.M
Quant Title : SW846 8260
QLast Update : Thu May 06 07:26:23 2021
Response via : Initial Calibration




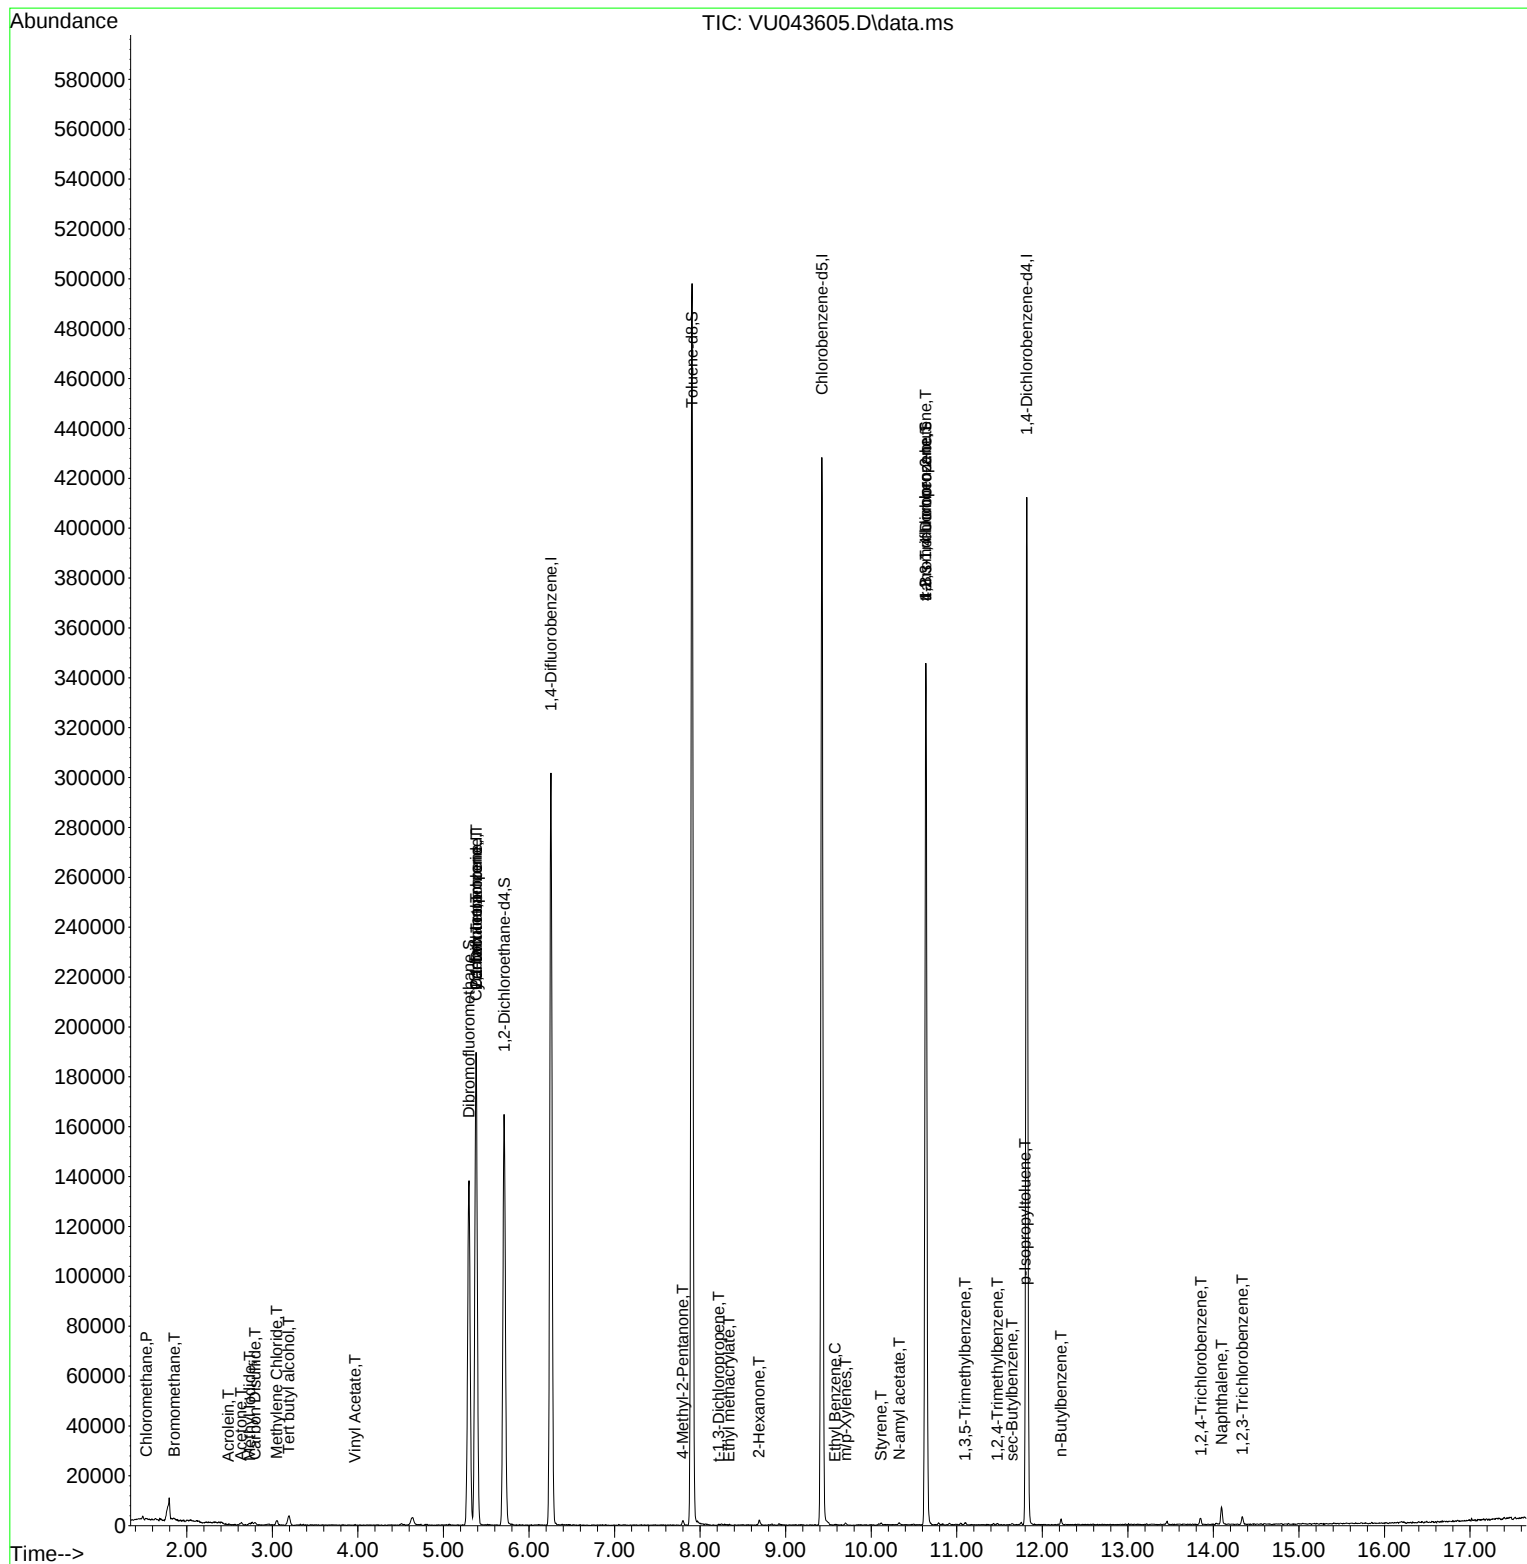




#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 5.382 min Scan# 1257
Delta R.T. -0.000 min
Lab File: VU043605.D
Acq: 07 May 2021 12:29




Instrument :
MSVOA_U
ClientSampleId :
BP-VPB-RW8-TB-20210503


Tgt Ion:168 Resp: 120650
Ion Ratio Lower Upper
168 100
99 63.3 49.0 73.6

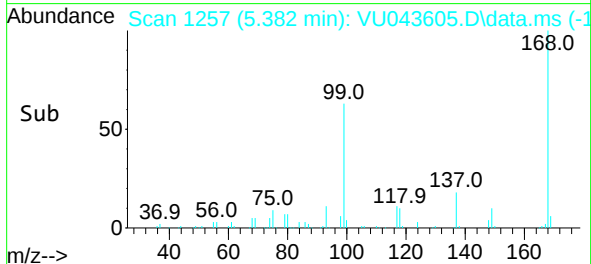

#3
Chloromethane
Concen: 0.62 ug/l
RT: 1.527 min Scan# 58
Delta R.T. 0.006 min
Lab File: VU043605.D
Acq: 07 May 2021 12:29

Tgt Ion: 50 Resp: 675
Ion Ratio Lower Upper
50 100
52 32.0 25.9 38.9


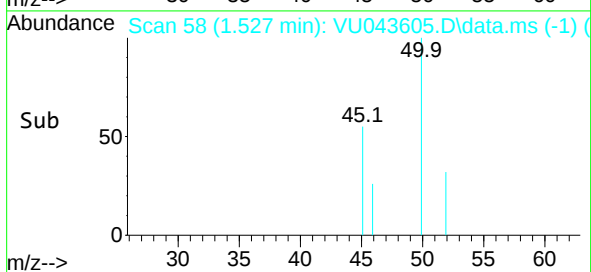






#5
Bromomethane
Concen: 0.32 ug/l
RT: 1.854 min Scan# 160
Delta R.T. 0.016 min
Lab File: VU043605.D
Acq: 07 May 2021 12:29




Instrument :
MSVOA_U
ClientSampleId :
BP-VPB-RW8-TB-20210503


Tgt Ion: 94 Resp: 348
Ion Ratio Lower Upper
94 100
96 77.1 73.3 109.9

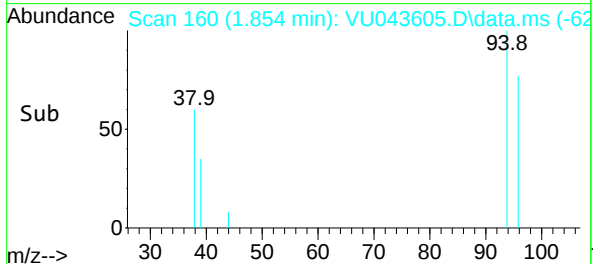

#10
Methyl Iodide
Concen: 0.37 ug/l
RT: 2.735 min Scan# 434
Delta R.T. 0.010 min
Lab File: VU043605.D
Acq: 07 May 2021 12:29

Tgt Ion: 142 Resp: 654
Ion Ratio Lower Upper
142 100
127 33.0 38.9 58.3#
141 0.0 11.8 17.6#

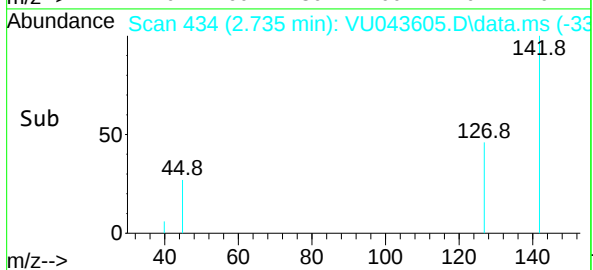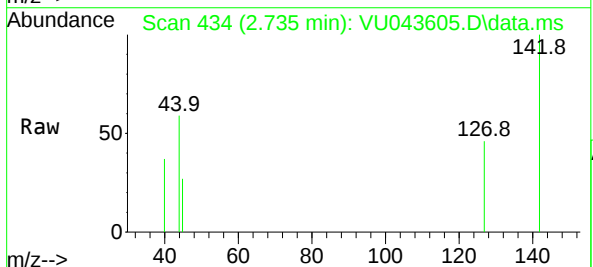







#11

Tert butyl alcohol
Concen: 3.91 ug/l
RT: 3.192 min Scan# 576
Delta R.T. -0.003 min
Lab File: VU043605.D
Acq: 07 May 2021 12:29

Instrument :
MSVOA_U
ClientSampleId :
BP-VPB-RW8-TB-20210503




Tgt Ion: 59 Resp: 2565
Ion Ratio Lower Upper
59 100
57 0.0 8.0 12.0#

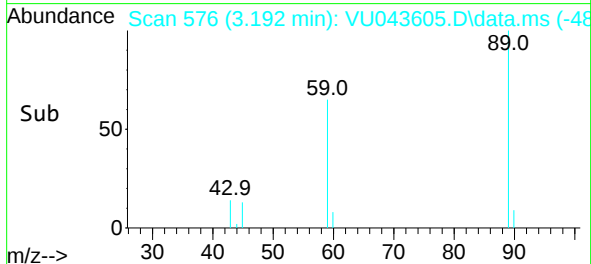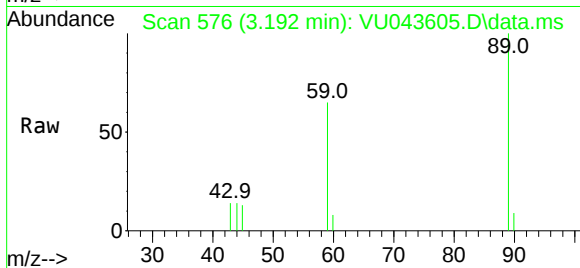


#13

Acrolein
Concen: 6.11 ug/l
RT: 2.485 min Scan# 356
Delta R.T. -0.003 min
Lab File: VU043605.D
Acq: 07 May 2021 12:29

Tgt Ion: 56 Resp: 21
Ion Ratio Lower Upper
56 100
55 0.0 56.9 85.3#


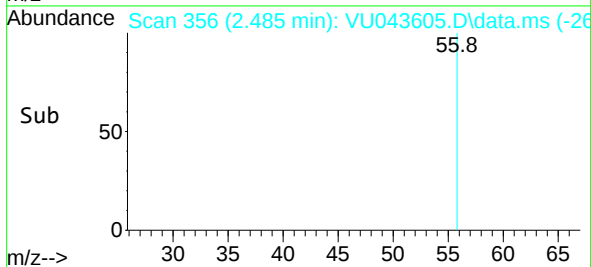

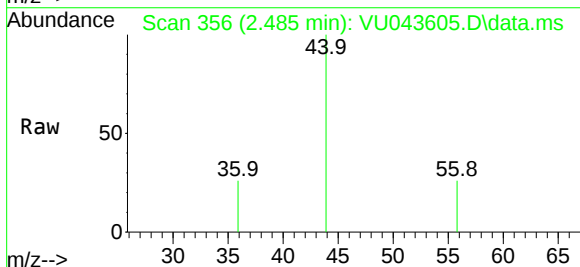




#16
Acetone
Concen: 0.79 ug/l
RT: 2.636 min Scan# 403
Delta R.T. 0.006 min
Lab File: VU043605.D
Acq: 07 May 2021 12:29




Instrument :
MSVOA_U
ClientSampleId :
BP-VPB-RW8-TB-20210503


Tgt Ion: 43 Resp: 1074
Ion Ratio Lower Upper
43 100
58 37.9 21.7 32.5#

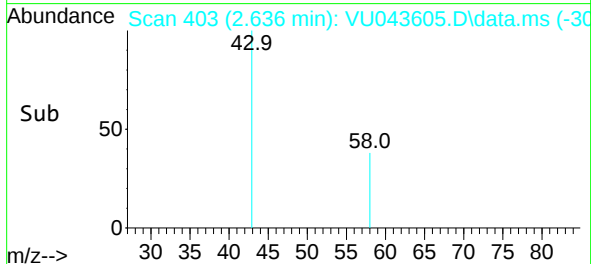

#17
Carbon Disulfide
Concen: 0.25 ug/l
RT: 2.797 min Scan# 453
Delta R.T. -0.000 min
Lab File: VU043605.D
Acq: 07 May 2021 12:29

Tgt Ion: 76 Resp: 1088
Ion Ratio Lower Upper
76 100
78 17.1 7.0 10.6#

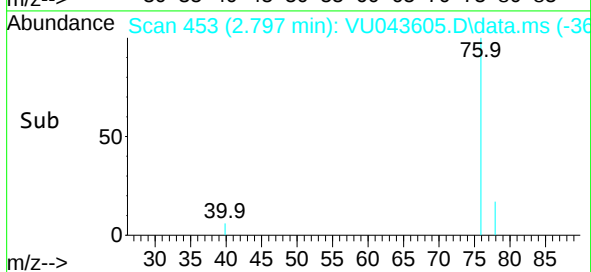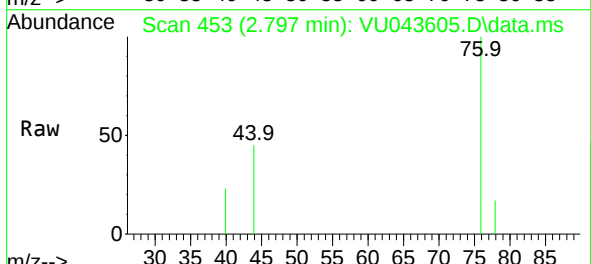



#20

Methylene Chloride

Concen: 0.40 ug/l

RT: 3.051 min Scan# 532

Delta R.T. -0.000 min

Lab File: VU043605.D


Acq: 07 May 2021 12:29

Instrument :

MSVOA_U

ClientSampleId :

BP-VPB-RW8-TB-20210503



Tgt Ion: 84 Resp: 754




Ion Ratio Lower Upper

84 100

49 133.0 119.0 178.4

51 52.3 36.8 55.2

86 71.5 49.8 74.6

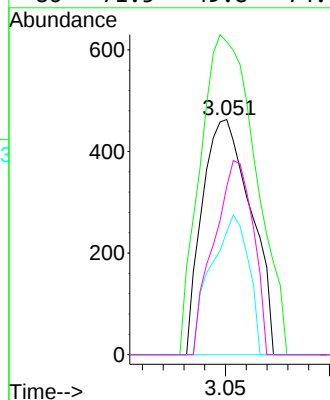

#23

Vinyl Acetate

Concen: 9.97 ug/l

RT: 3.967 min Scan# 817

Delta R.T. 0.003 min

Lab File: VU043605.D




Acq: 07 May 2021 12:29


Tgt Ion: 43 Resp: 113

Ion Ratio Lower Upper

43 100

86 0.0 6.2 9.2#


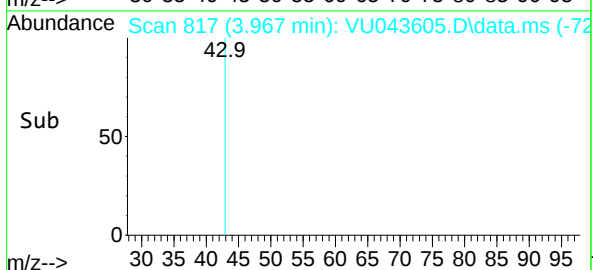
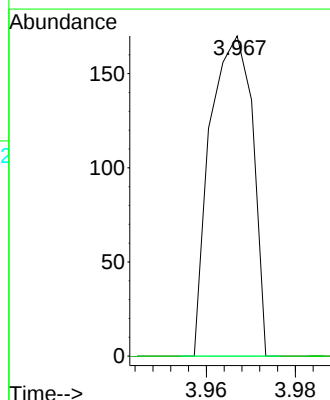





#31
Cyclohexane
Concen: 1.21 ug/l
RT: 5.378 min Scan# 1256
Delta R.T. -0.016 min
Lab File: VU043605.D
Acq: 07 May 2021 12:29




Instrument :
MSVOA_U
ClientSampleId :
BP-VPB-RW8-TB-20210503


Tgt Ion: 56 Resp: 3538
Ion Ratio Lower Upper
56 100
69 142.1 23.9 35.9#
84 96.2 57.7 86.5#

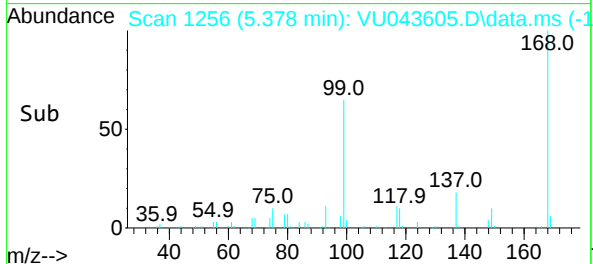

#33
1,2-Dichloroethane-d4
Concen: 50.47 ug/l
RT: 5.710 min Scan# 1359
Delta R.T. -0.000 min
Lab File: VU043605.D
Acq: 07 May 2021 12:29

Tgt Ion: 65 Resp: 123268
Ion Ratio Lower Upper
65 100
67 52.4 0.0 104.6


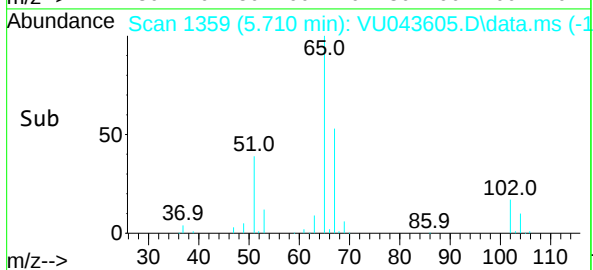

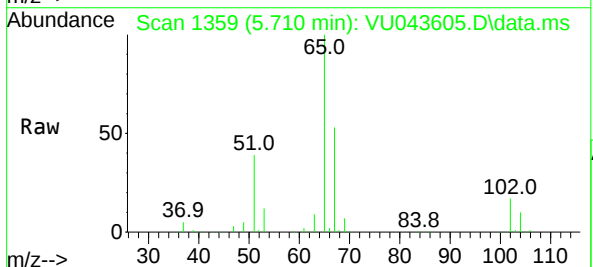




#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 6.256 min Scan# 1529
Delta R.T. -0.000 min
Lab File: VU043605.D
Acq: 07 May 2021 12:29




Instrument :
MSVOA_U
ClientSampleId :
BP-VPB-RW8-TB-20210503


Tgt Ion:	114	Resp:	218005
Ion Ratio	Lower	Upper	
114	100		
63	25.0	0.0	50.2
88	16.6	0.0	33.8

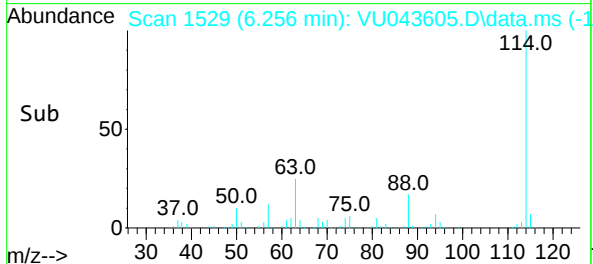

#35
Dibromofluoromethane
Concen: 49.04 ug/l
RT: 5.298 min Scan# 1231
Delta R.T. -0.000 min
Lab File: VU043605.D
Acq: 07 May 2021 12:29

Tgt Ion:	113	Resp:	85264
Ion Ratio	Lower	Upper	
113	100		
111	102.0	82.3	123.5
192	18.9	15.8	23.6

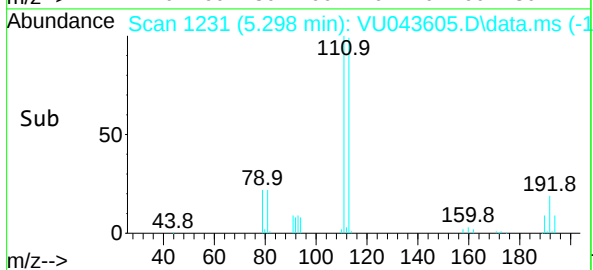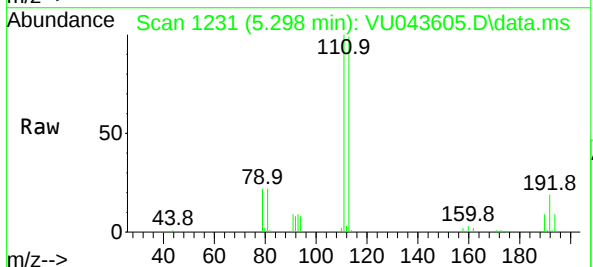







#36

1,1-Dichloropropene
Concen: 4.67 ug/l
RT: 5.382 min Scan# 1257
Delta R.T. -0.151 min
Lab File: VU043605.D
Acq: 07 May 2021 12:29

Instrument :
MSVOA_U
ClientSampleId :
BP-VPB-RW8-TB-20210503




Tgt Ion: 75 Resp: 11548
Ion Ratio Lower Upper
75 100
110 6.5 16.2 48.5#
77 0.0 24.4 36.6#

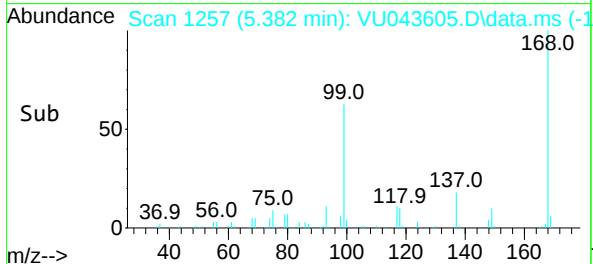


#38

Carbon Tetrachloride
Concen: 5.30 ug/l
RT: 5.382 min Scan# 1257
Delta R.T. -0.151 min
Lab File: VU043605.D
Acq: 07 May 2021 12:29

Tgt Ion: 117 Resp: 13287
Ion Ratio Lower Upper
117 100
119 5.7 75.4 113.0#
121 0.0 25.2 37.8#


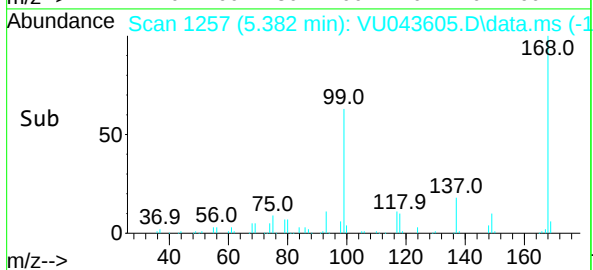

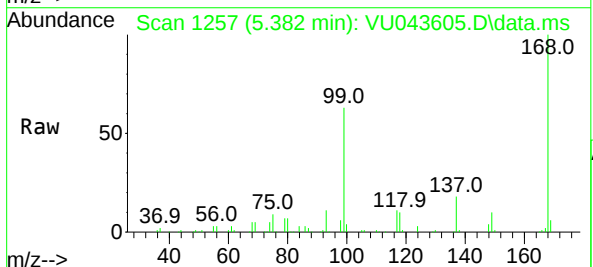




#50
Toluene-d8
Concen: 48.51 ug/l
RT: 7.906 min Scan# 2042
Delta R.T. -0.000 min
Lab File: VU043605.D
Acq: 07 May 2021 12:29




Instrument :
MSVOA_U
ClientSampleId :
BP-VPB-RW8-TB-20210503


Tgt Ion: 98 Resp: 299066
Ion Ratio Lower Upper
98 100
100 62.9 50.5 75.7

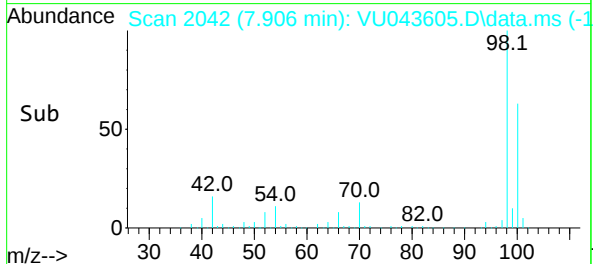

#51
4-Methyl-2-Pentanone
Concen: 19.46 ug/l
RT: 7.796 min Scan# 2008
Delta R.T. -0.004 min
Lab File: VU043605.D
Acq: 07 May 2021 12:29

Tgt Ion: 43 Resp: 1493
Ion Ratio Lower Upper
43 100
58 22.6 27.2 40.8#


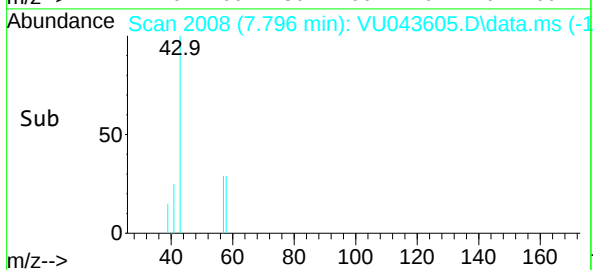

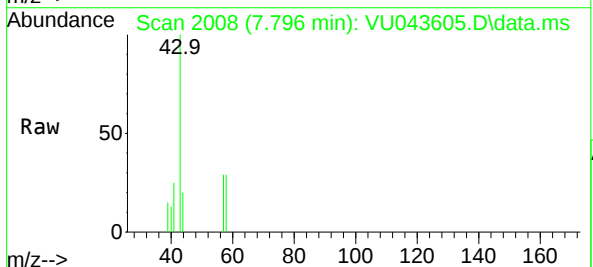




#53
t-1,3-Dichloropropene
Concen: 2.27 ug/l
RT: 8.218 min Scan# 2139
Delta R.T. -0.000 min
Lab File: VU043605.D
Acq: 07 May 2021 12:29




Instrument :
MSVOA_U
ClientSampleId :
BP-VPB-RW8-TB-20210503


Tgt Ion: 75 Resp: 76
Ion Ratio Lower Upper
75 100
77 144.1 25.5 38.3#

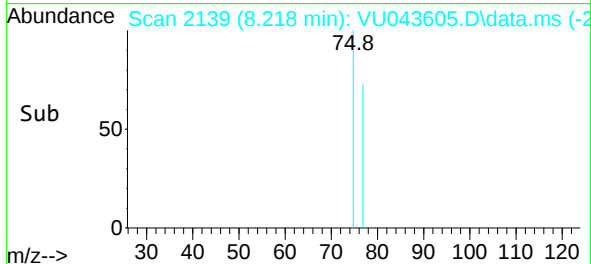

#56
Ethyl methacrylate
Concen: 4.26 ug/l
RT: 8.340 min Scan# 2177
Delta R.T. -0.000 min
Lab File: VU043605.D
Acq: 07 May 2021 12:29

Tgt Ion: 69 Resp: 163
Ion Ratio Lower Upper
69 100
41 11.7 66.7 100.1#
39 0.0 37.8 56.8#


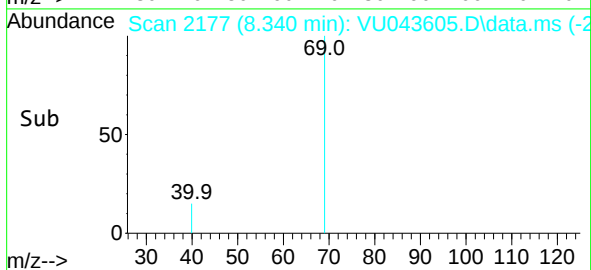

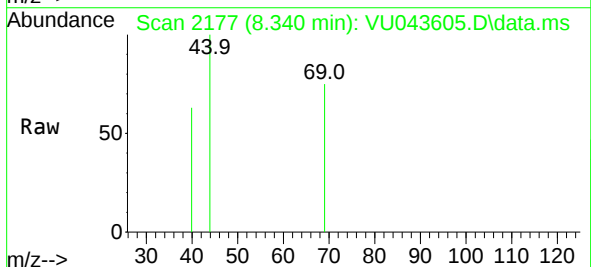




#59
2-Hexanone
Concen: 21.11 ug/l
RT: 8.687 min Scan# 2285
Delta R.T. -0.003 min
Lab File: VU043605.D
Acq: 07 May 2021 12:29




Instrument :
MSVOA_U
ClientSampleId :
BP-VPB-RW8-TB-20210503


Tgt Ion: 43 Resp: 1765
Ion Ratio Lower Upper
43 100
58 40.5 23.4 70.2



#62
4-Bromofluorobenzene
Concen: 44.99 ug/l
RT: 10.639 min Scan# 2892
Delta R.T. -0.000 min
Lab File: VU043605.D
Acq: 07 May 2021 12:29

Tgt Ion: 95 Resp: 105504
Ion Ratio Lower Upper
95 100
174 78.3 0.0 158.8
176 75.6 0.0 155.6

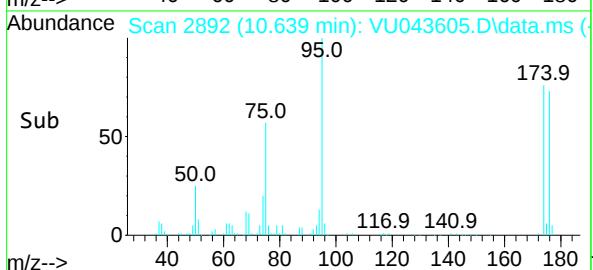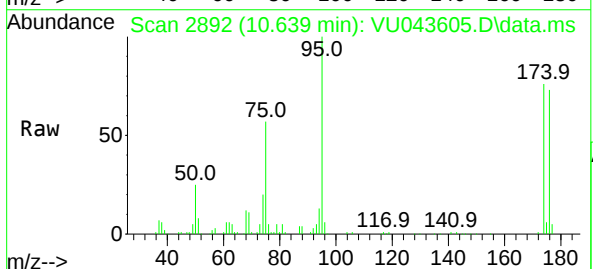



#63

Chlorobenzene-d5

Concen: 50.00 ug/l

RT: 9.423 min Scan# 2514

Delta R.T. 0.000 min

Lab File: VU043605.D

Acq: 07 May 2021 12:29

Tgt Ion:117 Resp: 210372

Ion Ratio Lower Upper

117 100

82 60.9 47.5 71.3





119 32.3 24.7 37.1

Instrument :

MSVOA_U

ClientSampleId :

BP-VPB-RW8-TB-20210503

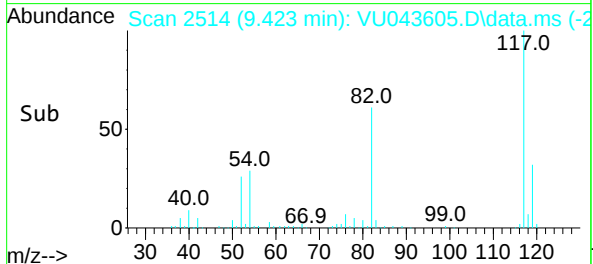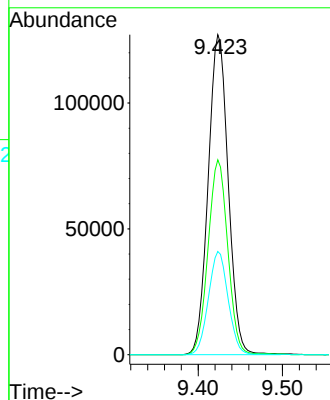

#67

Ethyl Benzene

Concen: 1.49 ug/l

RT: 9.578 min Scan# 2562

Delta R.T. -0.000 min

Lab File: VU043605.D




Acq: 07 May 2021 12:29


Tgt Ion: 91 Resp: 353

Ion Ratio Lower Upper

91 100

106 0.0 24.0 36.0#


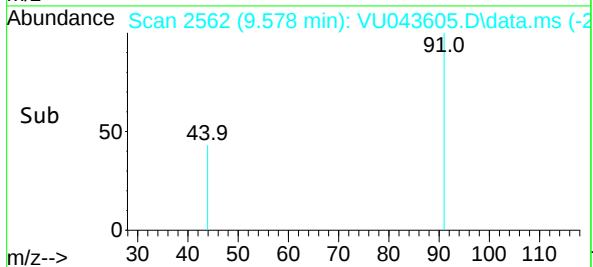
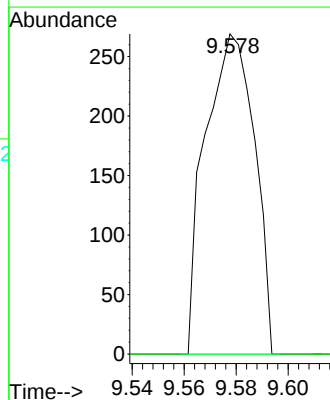
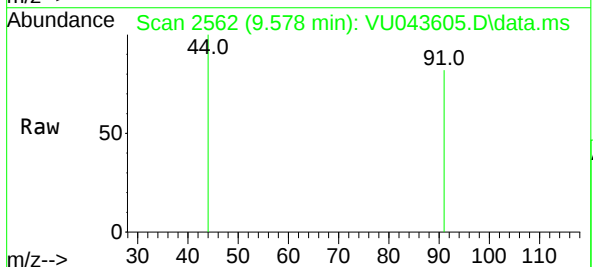




#68
m/p-Xylenes
Concen: 2.39 ug/l
RT: 9.703 min Scan# 2601
Delta R.T. 0.003 min
Lab File: VU043605.D
Acq: 07 May 2021 12:29




Instrument :
MSVOA_U
ClientSampleId :
BP-VPB-RW8-TB-20210503


Tgt Ion:106 Resp: 189
Ion Ratio Lower Upper
106 100
91 306.9 171.7 257.5#

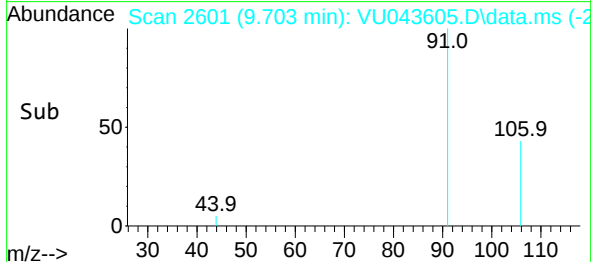

#70
Styrene
Concen: 2.73 ug/l
RT: 10.115 min Scan# 2729
Delta R.T. -0.006 min
Lab File: VU043605.D
Acq: 07 May 2021 12:29

Tgt Ion:104 Resp: 214
Ion Ratio Lower Upper
104 100
78 56.1 44.6 67.0
103 0.0 45.1 67.7#


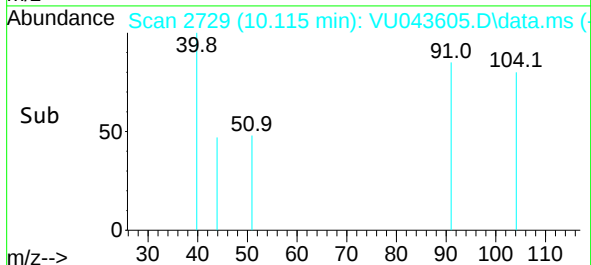
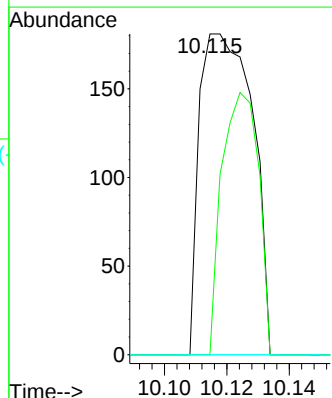
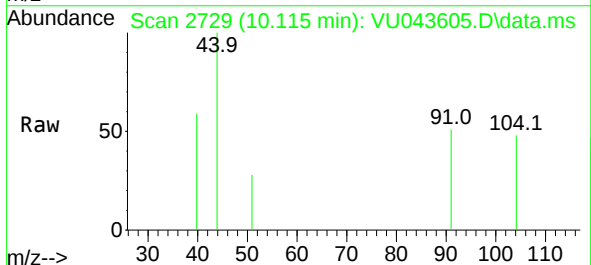


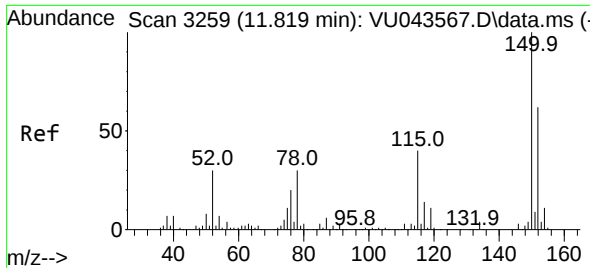

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 11.819 min Scan# 3259
Delta R.T. -0.000 min
Lab File: VU043605.D
Acq: 07 May 2021 12:29




Instrument :
MSVOA_U
ClientSampleId :
BP-VPB-RW8-TB-20210503


Tgt Ion:152 Resp: 95242
Ion Ratio Lower Upper
152 100
115 60.7 46.1 138.3
150 157.0 0.0 361.0

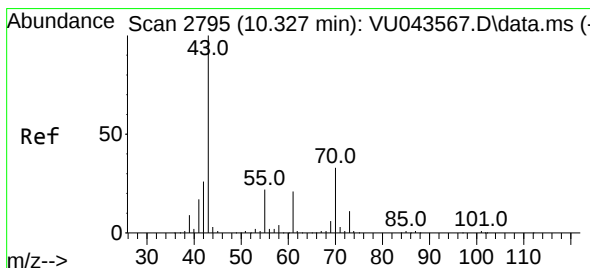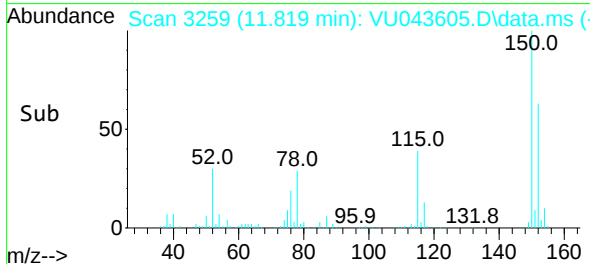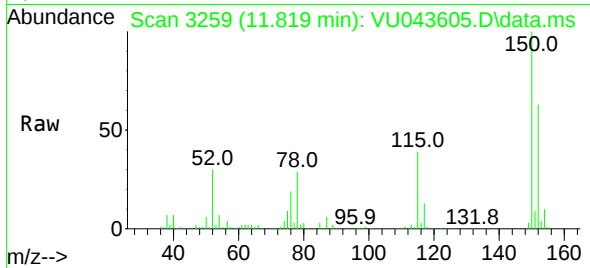

#74
N-ethyl acetate
Concen: 2.65 ug/l
RT: 10.327 min Scan# 2795
Delta R.T. -0.000 min
Lab File: VU043605.D
Acq: 07 May 2021 12:29

Tgt Ion: 43 Resp: 712
Ion Ratio Lower Upper
43 100
70 17.4 26.4 39.6#
55 0.0 18.0 27.0#
61 0.0 16.6 25.0#


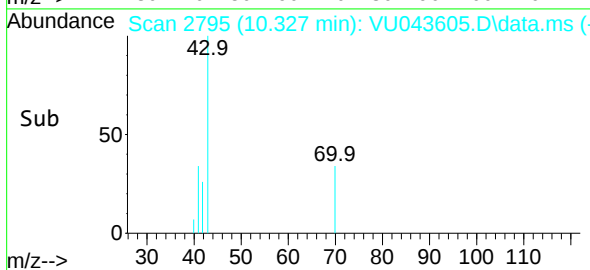

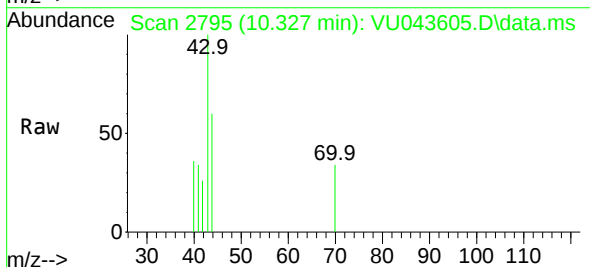




#76
1,2,3-Trichloropropane
Concen: 20.12 ug/l
RT: 10.639 min Scan# 2892
Delta R.T. -0.193 min
Lab File: VU043605.D
Acq: 07 May 2021 12:29




Instrument :
MSVOA_U
ClientSampleId :
BP-VPB-RW8-TB-20210503


Tgt Ion: 75 Resp: 60931
Ion Ratio Lower Upper
75 100
77 1.0 17.1 51.3#

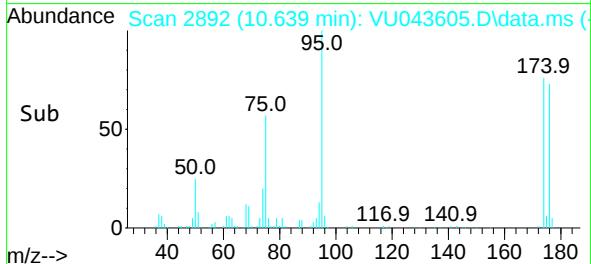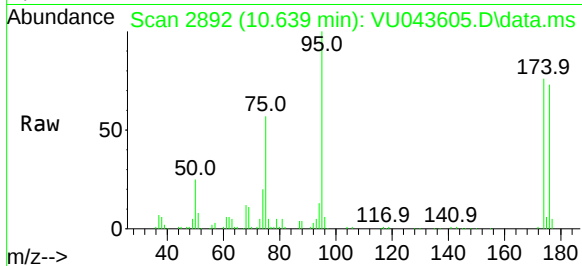

#80
1,3,5-Trimethylbenzene
Concen: 0.78 ug/l
RT: 11.095 min Scan# 3034
Delta R.T. 0.000 min
Lab File: VU043605.D
Acq: 07 May 2021 12:29

Tgt Ion: 105 Resp: 310
Ion Ratio Lower Upper
105 100
120 13.9 22.9 68.7#


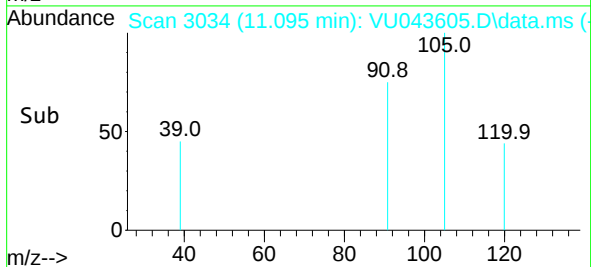

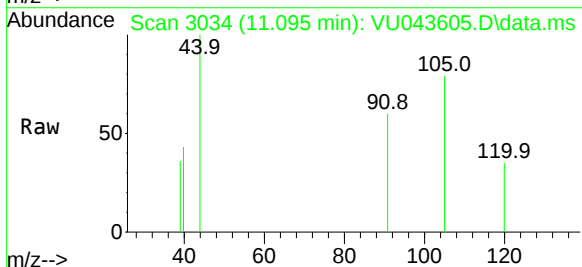




#81
trans-1,4-Dichloro-2-butene
Concen: 65.52 ug/l
RT: 10.639 min Scan# 2892
Delta R.T. 0.087 min
Lab File: VU043605.D
Acq: 07 May 2021 12:29




Instrument :
MSVOA_U
ClientSampleId :
BP-VPB-RW8-TB-20210503


Tgt Ion: 75 Resp: 60931
Ion Ratio Lower Upper
75 100
53 0.0 95.8 143.8#
89 0.0 36.1 54.1#

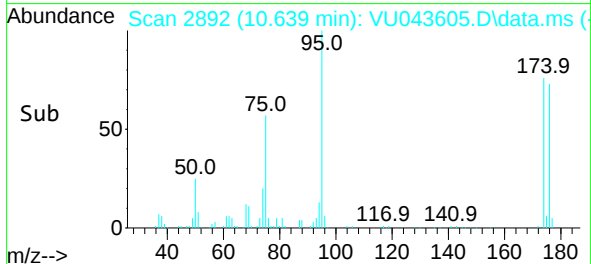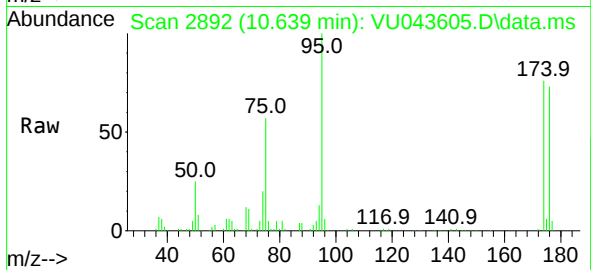

#84
1,2,4-Trimethylbenzene
Concen: 1.19 ug/l
RT: 11.475 min Scan# 3152
Delta R.T. -0.000 min
Lab File: VU043605.D
Acq: 07 May 2021 12:29

Tgt Ion: 105 Resp: 506
Ion Ratio Lower Upper
105 100
120 19.2 21.4 64.2#




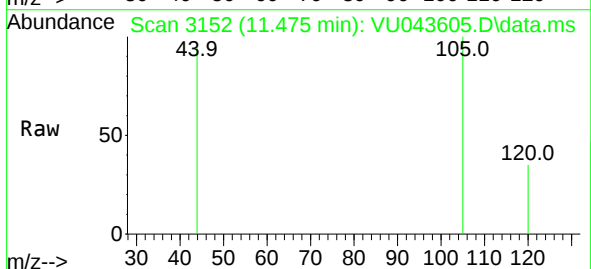


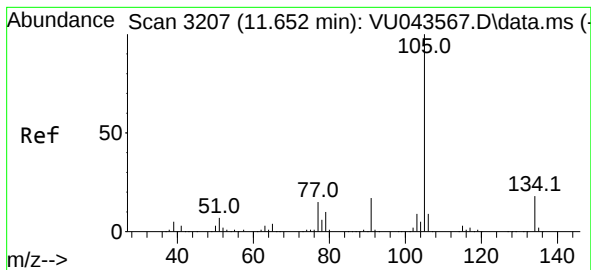

#85
 sec-Butylbenzene
 Concen: 1.40 ug/l
 RT: 11.645 min Scan# 3205
 Delta R.T. -0.007 min
 Lab File: VU043605.D
 Acq: 07 May 2021 12:29




Instrument :
 MSVOA_U
 ClientSampleId :
 BP-VPB-RW8-TB-20210503


Tgt Ion:105 Resp: 521
 Ion Ratio Lower Upper
 105 100
 134 0.0 9.2 27.6#

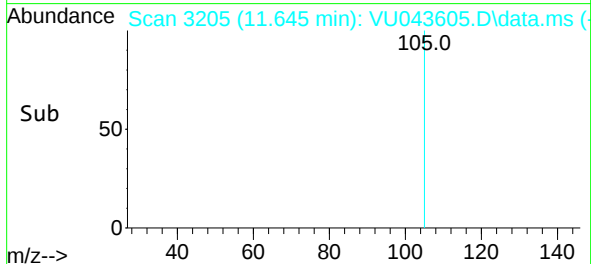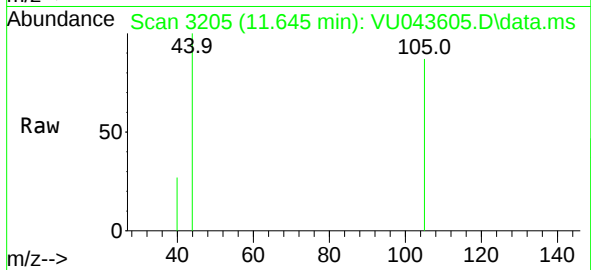

#86
 p-Isopropyltoluene
 Concen: 1.54 ug/l
 RT: 11.799 min Scan# 3253
 Delta R.T. 0.000 min
 Lab File: VU043605.D
 Acq: 07 May 2021 12:29

Tgt Ion:119 Resp: 501
 Ion Ratio Lower Upper
 119 100
 134 23.8 12.7 38.0
 91 13.8 13.3 39.9

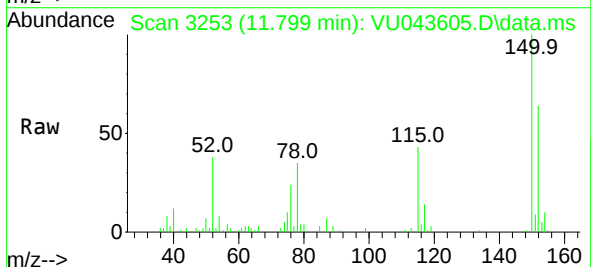



#89

n-Butylbenzene

Concen: 2.67 ug/l

RT: 12.217 min Scan# 3383





Delta R.T. 0.003 min

Lab File: VU043605.D

Acq: 07 May 2021 12:29

Tgt Ion:	91	Resp:	956
Ion	Ratio	Lower	Upper
91	100		
92	35.3	25.4	76.2
134	4.2	11.3	33.9#

Instrument :
MSVOA_U
ClientSampleId :
BP-VPB-RW8-TB-20210503

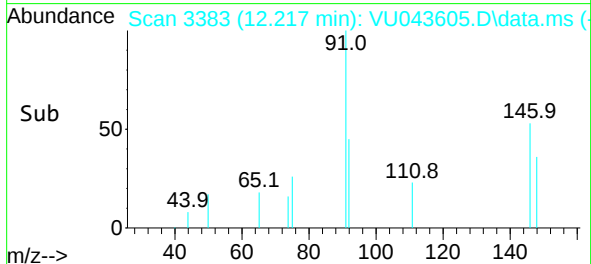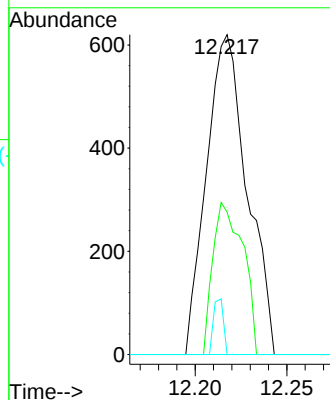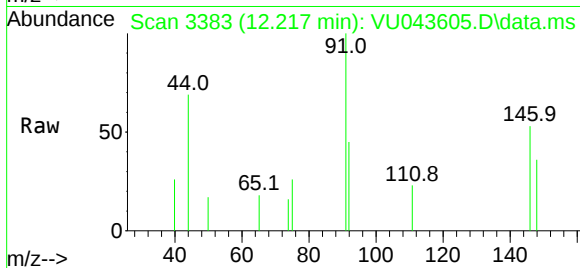

#93

1,2,4-Trichlorobenzene

Concen: 0.41 ug/l




RT: 13.854 min Scan# 3892


Delta R.T. 0.006 min

Lab File: VU043605.D

Acq: 07 May 2021 12:29


Tgt Ion:	180	Resp:	911
Ion	Ratio	Lower	Upper
180	100		
182	105.2	47.2	141.6
145	30.2	14.9	44.9

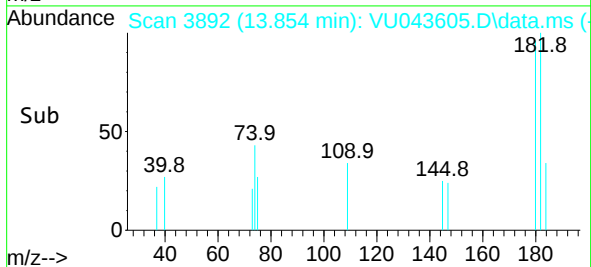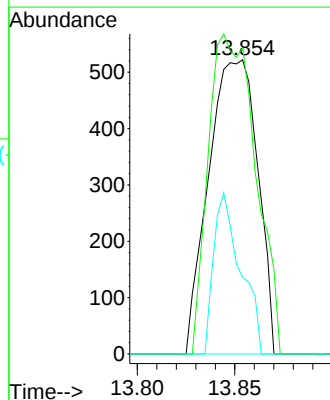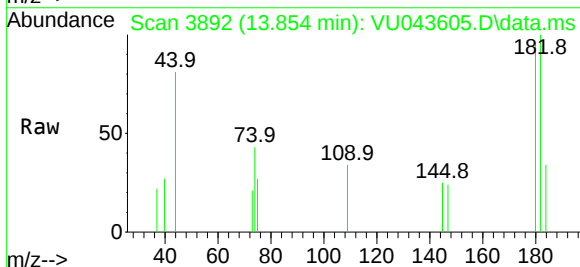






#95
Naphthalene
Concen: 2.23 ug/l
RT: 14.095 min Scan# 3967
Delta R.T. 0.000 min
Lab File: VU043605.D
Acq: 07 May 2021 12:29


Instrument :
MSVOA_U
ClientSampleId :
BP-VPB-RW8-TB-20210503

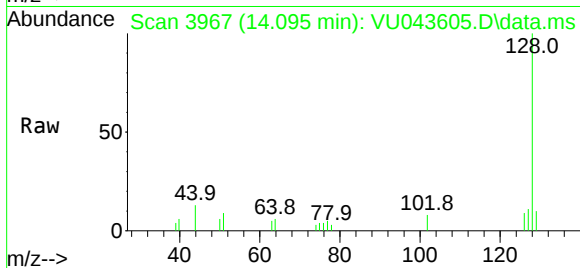

Tgt Ion:128 Resp: 5918
Ion Ratio Lower Upper
128 100
127 10.7 10.7 16.1
129 10.4 8.6 12.8



#96
1,2,3-Trichlorobenzene
Concen: 0.55 ug/l
RT: 14.339 min Scan# 4043
Delta R.T. 0.003 min
Lab File: VU043605.D
Acq: 07 May 2021 12:29

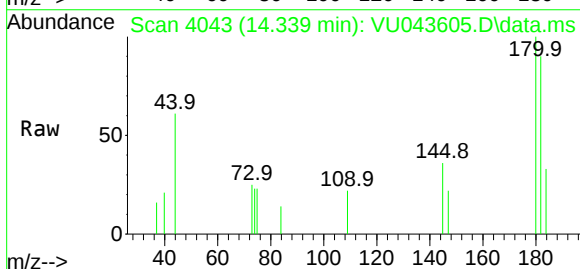

Tgt Ion:180 Resp: 1233
Ion Ratio Lower Upper
180 100
182 92.3 48.2 144.6
145 32.8 16.2 48.6

