


Data Path : W:\HPCHEM1\MSVOA U\DATA\VU050818\
Data File : VU023725.D
Acq On : 08 May 2018 09:38
Operator : MD/SY
Sample : BFB50
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Integration File: LSCINT.P

Method : W:\HPCHEM1\MSVOA_U\METHOD\SOMULM050818WMA.M
Title : VOC Analysis
Last Update : Thu May 10 16:04:14 2018

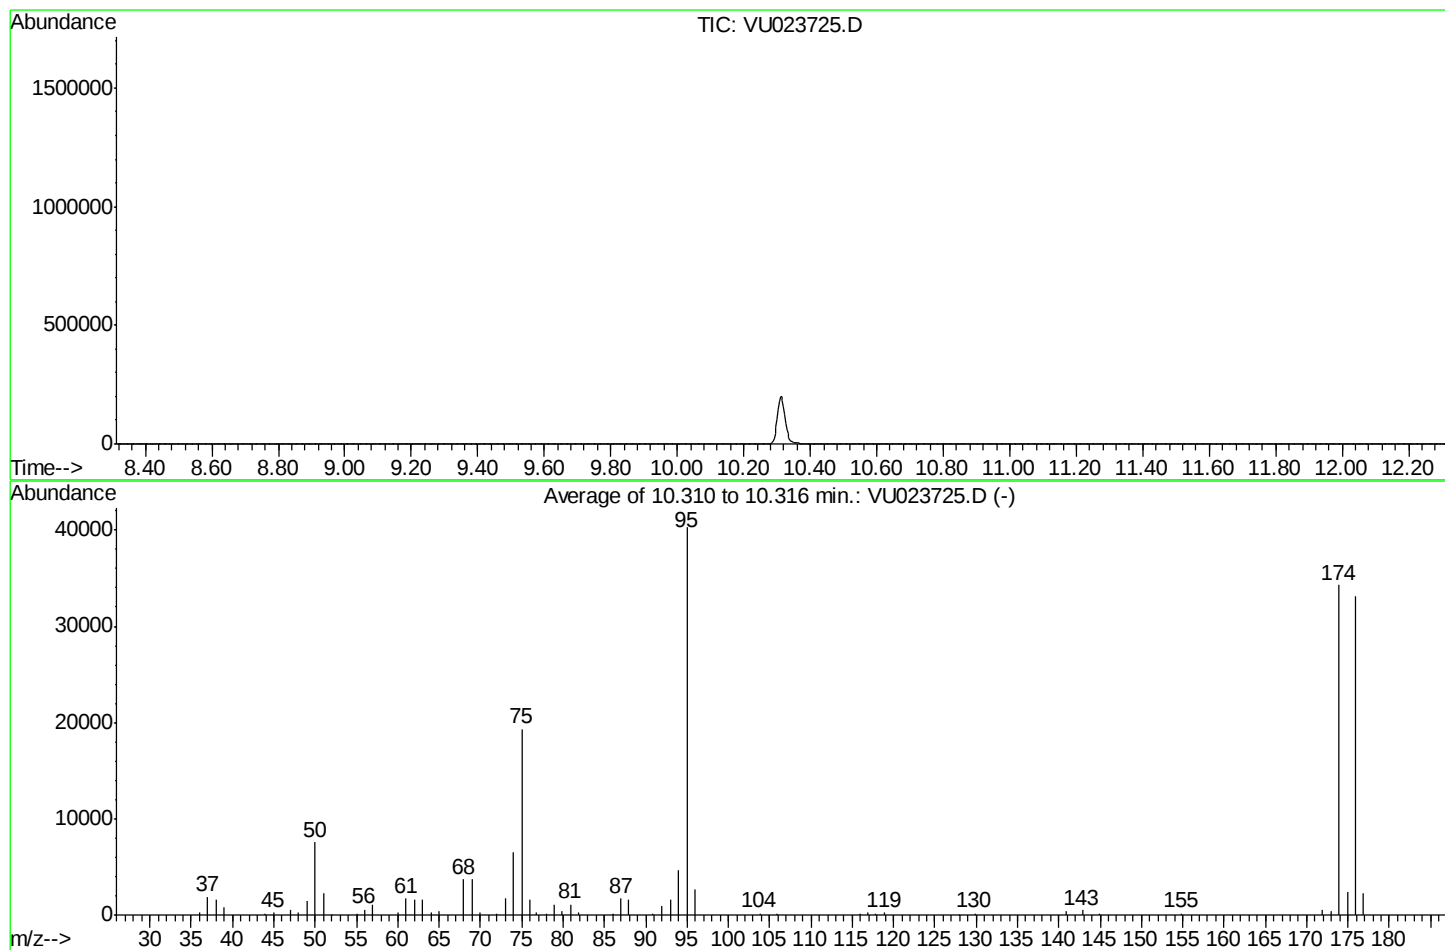

AutoFind: Scans 3023, 3024, 3025; Background Corrected with Scan 3011

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	7574	PASS
75	95	30	80	48.0	19333	PASS
95	95	100	100	100.0	40290	PASS
96	95	5	9	6.6	2639	PASS
173	174	0.00	2	1.3	432	PASS
174	95	50	120	85.1	34296	PASS
175	174	5	9	7.0	2416	PASS
176	174	95	101	96.5	33096	PASS
177	176	5	9	6.9	2296	PASS

Scan 3011 (10.271 min): VU023725.D
BFB50

m/z	Abundance
39.90	214.0
44.00	525.0

m/z	Abundance
36.00	267.0
37.00	2051.0
38.00	1705.0
39.00	782.0
39.90	212.0
44.00	698.0
45.00	290.0
47.00	537.0
47.90	321.0
49.00	1466.0
50.00	7831.0
51.00	2428.0
52.00	107.0
55.00	104.0
56.00	620.0
57.00	1006.0
60.00	368.0
61.00	1785.0
62.10	1674.0
63.00	1786.0
64.00	280.0
65.10	387.0
68.00	3966.0
69.00	3787.0
70.00	276.0
71.90	205.0
73.00	1806.0
74.00	6574.0
75.00	19928.0
76.00	1641.0
76.80	247.0
78.00	225.0
78.90	1135.0
79.90	395.0
80.90	1165.0
81.80	280.0
87.00	1801.0
87.90	1553.0
90.90	137.0
92.00	983.0
93.00	1691.0
94.00	4601.0
95.00	41008.0
96.00	2862.0
103.80	123.0
105.90	113.0
115.90	111.0
117.00	231.0
117.90	120.0
118.90	237.0
127.80	108.0
129.90	159.0
140.90	406.0
142.90	547.0
144.80	156.0
154.90	138.0
171.80	477.0
173.00	472.0
173.90	34200.0
174.90	2472.0
175.90	32944.0
176.90	2338.0

m/z	Abundance
35.90	277.0
37.00	1982.0
38.00	1605.0
39.00	770.0
39.90	195.0
43.90	745.0
45.00	267.0
47.10	506.0
47.90	310.0
49.00	1430.0
50.00	7872.0
51.00	2336.0
52.00	105.0
55.10	120.0
56.00	586.0
57.00	1031.0
60.00	343.0
61.00	1735.0
62.10	1666.0
63.00	1680.0
64.00	264.0
65.00	400.0
68.00	3794.0
69.00	3816.0
70.00	318.0
71.90	195.0
73.00	1776.0
74.00	6682.0
75.00	19960.0
76.00	1586.0
76.80	280.0
78.00	211.0
78.90	1177.0
79.90	404.0
80.90	1174.0
81.90	273.0
86.10	126.0
87.00	1764.0
87.90	1657.0
90.90	111.0
92.00	889.0
93.00	1700.0
94.00	4832.0
95.00	41616.0
96.00	2705.0
103.80	163.0
105.90	122.0
115.90	124.0
116.90	244.0
117.90	120.0
118.90	242.0
127.80	107.0
129.90	135.0
140.90	444.0
142.90	531.0
144.90	142.0
154.90	146.0
171.80	532.0
173.00	460.0
173.90	35312.0
174.90	2496.0
175.90	34224.0
176.90	2370.0

m/z	Abundance
35.90	262.0
37.00	1763.0
38.00	1464.0
39.00	723.0
39.90	190.0
43.90	743.0
45.00	241.0
47.10	465.0
47.90	248.0
49.00	1350.0
50.00	7020.0
51.00	2038.0
55.10	129.0
56.00	523.0
57.00	974.0
60.00	302.0
61.00	1582.0
62.10	1587.0
63.00	1449.0
64.00	226.0
65.00	355.0
68.00	3364.0
69.00	3447.0
70.00	331.0
72.00	174.0
73.00	1604.0
74.00	6198.0
75.00	18112.0
76.00	1411.0
76.80	238.0
77.90	145.0
78.90	1080.0
79.90	360.0
80.90	1041.0
81.90	253.0
86.10	159.0
87.00	1580.0
87.90	1585.0
92.00	821.0
93.00	1571.0
94.00	4534.0
95.00	38248.0
96.00	2351.0
103.80	169.0
105.80	132.0
116.00	119.0
116.90	221.0
117.80	107.0
118.90	248.0
129.80	112.0
140.90	402.0
142.90	472.0
144.90	125.0
154.80	123.0
171.80	512.0
173.00	365.0
173.90	33376.0
174.90	2281.0
175.90	32120.0
176.90	2180.0