

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050819\
 Data File : VU031821.D
 Acq On : 08 May 2019 13:51
 Operator : JC/SP
 Sample : K2661-03
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B23

Quant Time: May 09 05:43:56 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR050819WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu May 09 05:32:34 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	351240	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	356506	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	140602	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	109642	4.58	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	91.60%
7) Chloroethane-d5	1.68	69	94407	4.78	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	95.60%
11) 1,1-Dichloroethene-d2	2.27	63	169207	3.28	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	65.60%
20) 2-Butanone-d5	4.20	46	468226	50.10	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	100.20%
24) Chloroform-d	4.64	84	241620	4.92	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.40%
26) 1,2-Dichloroethane-d4	5.31	65	144749	4.86	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.20%
32) Benzene-d6	5.33	84	448901	4.92	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.40%
36) 1,2-Dichloropropane-d6	6.32	67	161430	4.82	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.40%
41) Toluene-d8	7.56	98	354660	4.54	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.80%
43) trans-1,3-Dichloropropene-	7.85	79	55846	4.75	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	95.00%
46) 2-Hexanone-d5	8.31	63	286307	48.14	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.28%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	124432	4.76	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.20%
64) 1,2-Dichlorobenzene-d4	11.86	152	122297	5.26	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.20%


Target Compounds					Ovalue
13) Acetone	2.34	43	22872	3.583 ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050819\
Data File : VU031821.D
Acq On : 08 May 2019 13:51
Operator : JC/SP
Sample : K2661-03
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B23

Quant Time: May 09 05:43:56 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR050819WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu May 09 05:32:34 2019
Response via : Initial Calibration

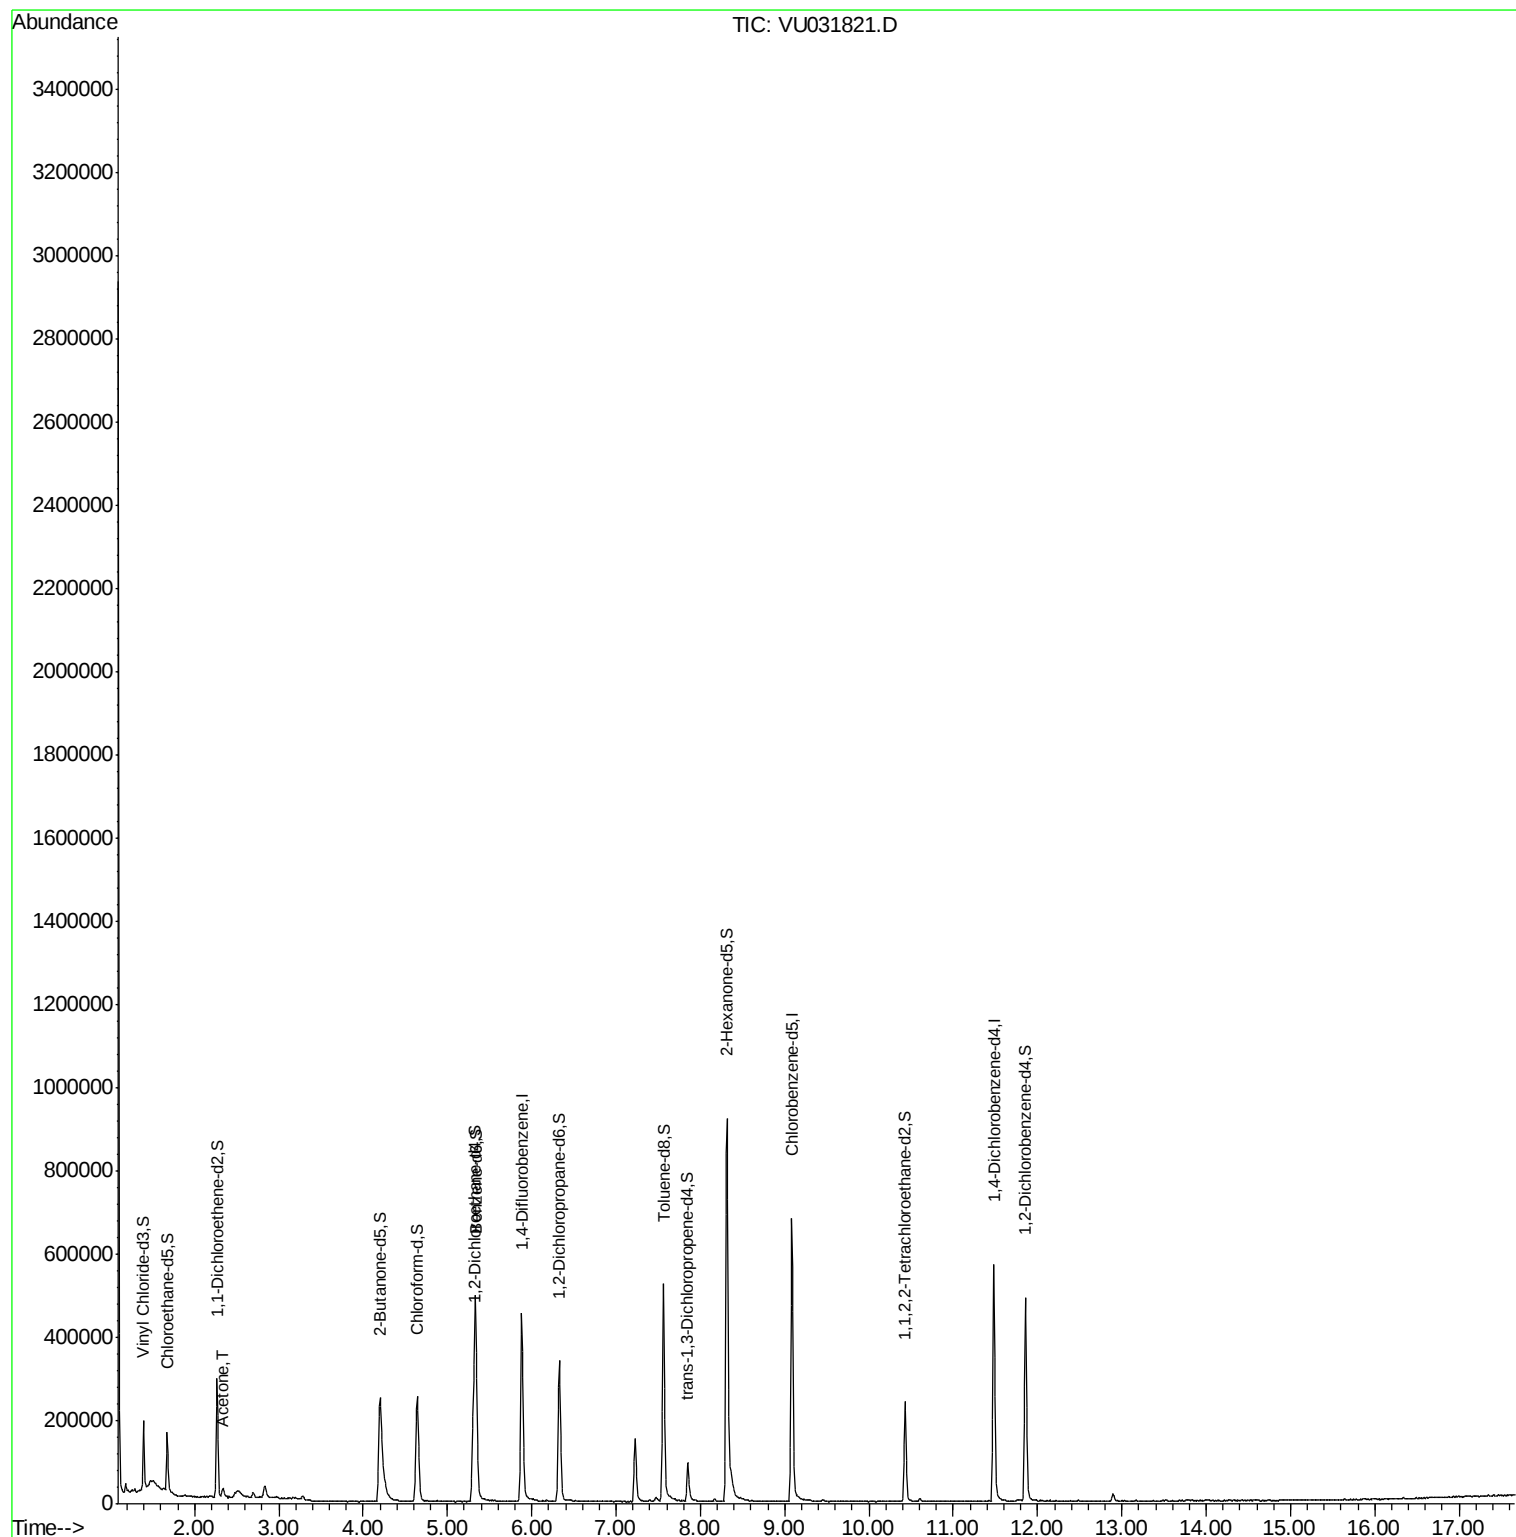

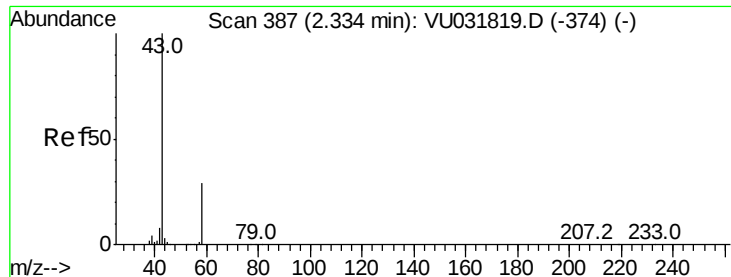

#13

Acetone

Concen: 3.583 ug/L

RT: 2.34 min Scan# 388

Delta R.T. 0.00 min

Lab File: VU031821.D

Acq: 08 May 2019 13:51

Instrument :

MSVOA_U

ClientSampleId :

C0B23

Tot Ion: 43 Resp: 22872

Ion Ratio Lower Upper

43 100

58 26.6 0.0 53.6

