

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050819\
 Data File : VU031822.D
 Acq On : 08 May 2019 14:16
 Operator : JC/SP
 Sample : K2661-04
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B24

Quant Time: May 09 05:57:21 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR050819WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu May 09 05:32:34 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	329321	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	336168	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	129804	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	110456	4.92	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	98.40%
7) Chloroethane-d5	1.68	69	90817	4.91	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	98.20%
11) 1,1-Dichloroethene-d2	2.27	63	161733	3.35	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.00%
20) 2-Butanone-d5	4.20	46	468760	53.49	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	106.98%
24) Chloroform-d	4.64	84	242342	5.27	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	105.40%
26) 1,2-Dichloroethane-d4	5.31	65	141362	5.06	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.20%
32) Benzene-d6	5.33	84	445905	5.18	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.60%
36) 1,2-Dichloropropane-d6	6.33	67	162019	5.13	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.60%
41) Toluene-d8	7.56	98	337501	4.58	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.60%
43) trans-1,3-Dichloropropene-	7.85	79	53561	4.83	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	96.60%
46) 2-Hexanone-d5	8.31	63	287761	51.31	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	102.62%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	126240	5.13	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	102.60%
64) 1,2-Dichlorobenzene-d4	11.86	152	117125	5.46	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	109.20%


Target Compounds					Ovalue
13) Acetone	2.34	43	24296	4.059 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050819\
Data File : VU031822.D
Acq On : 08 May 2019 14:16
Operator : JC/SP
Sample : K2661-04
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B24

Quant Time: May 09 05:57:21 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR050819WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu May 09 05:32:34 2019
Response via : Initial Calibration

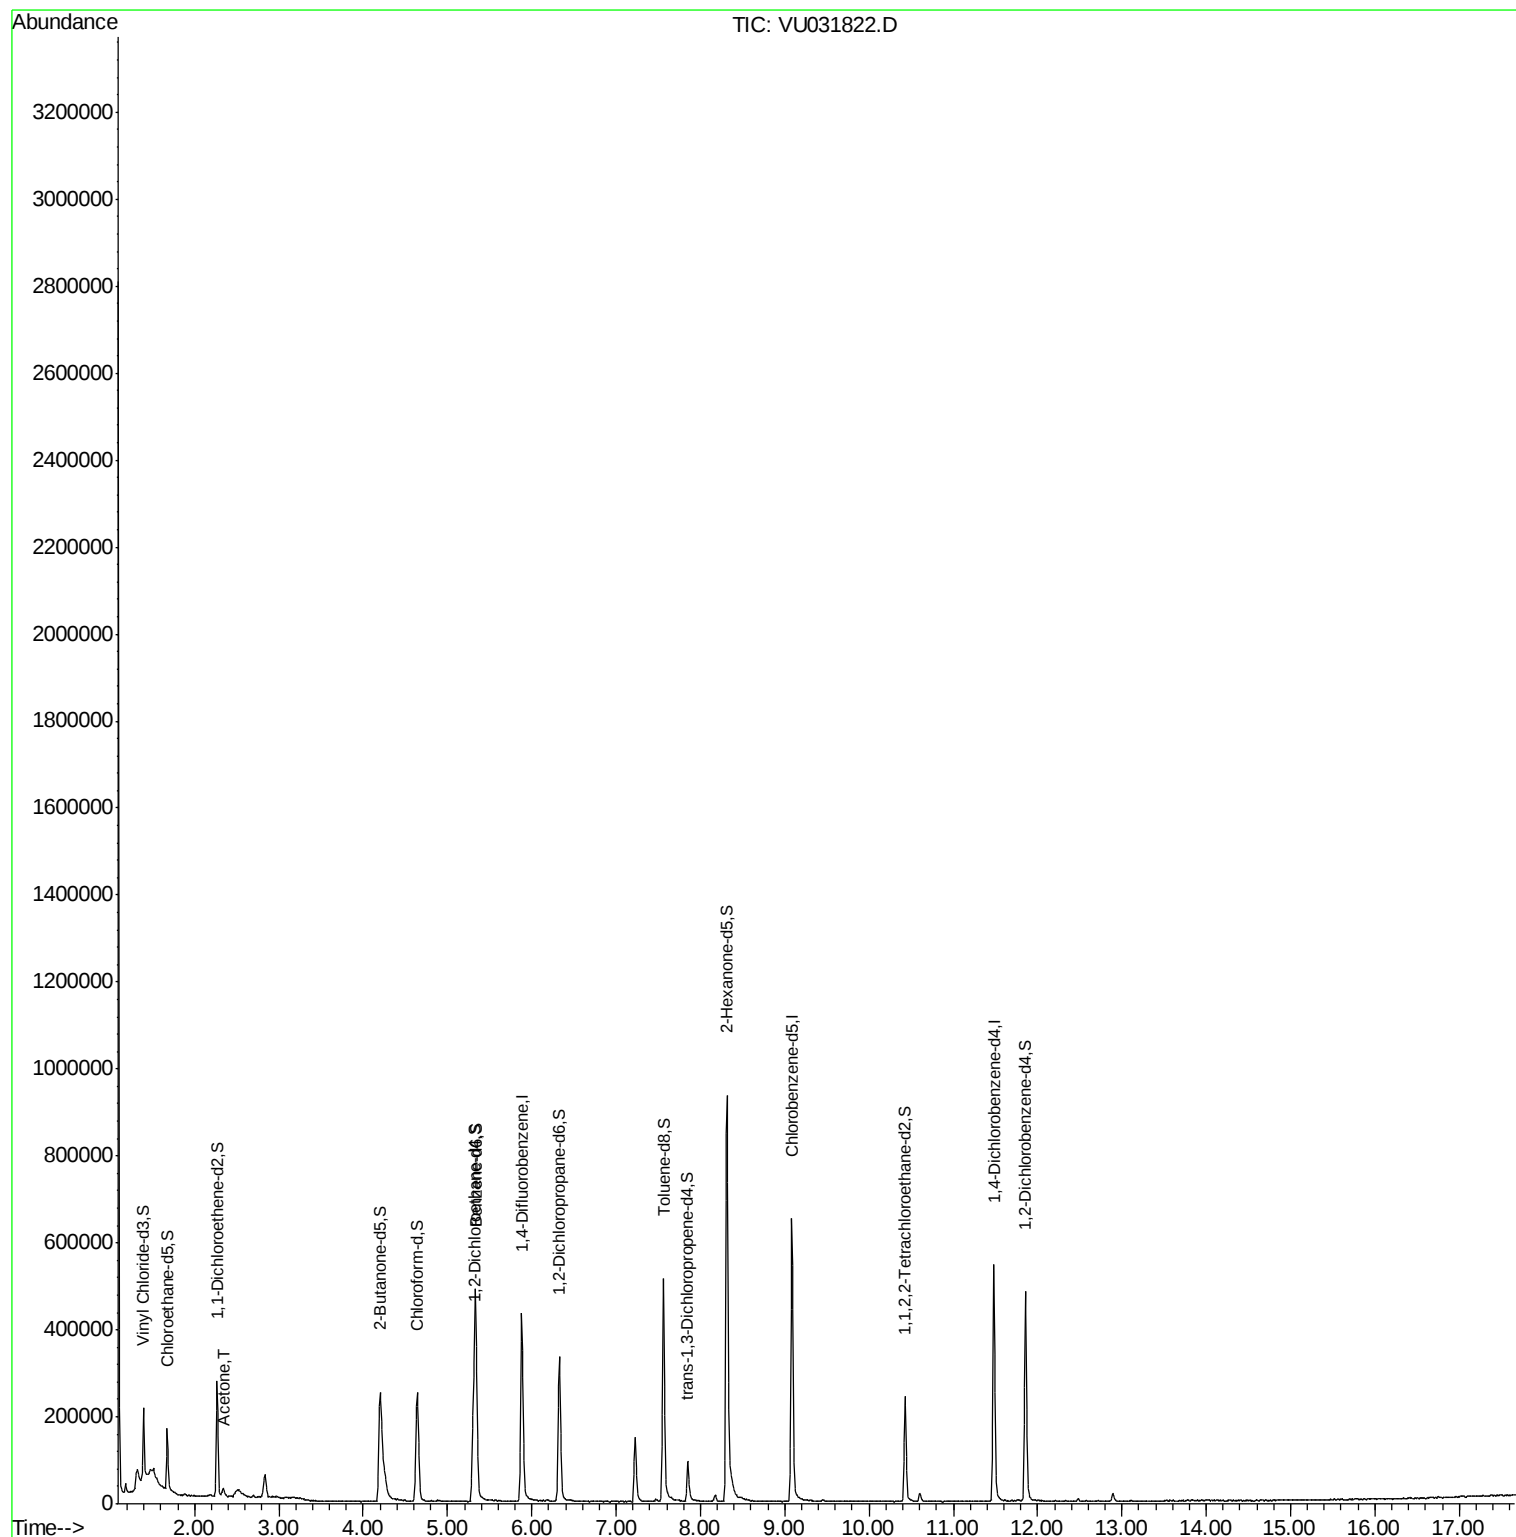

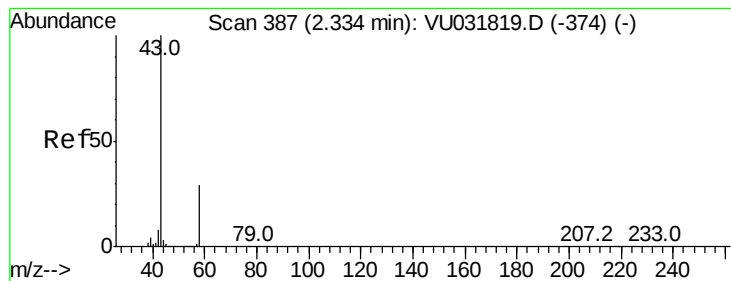

#13
 Acetone
 Concen: 4.059 ug/L
 RT: 2.34 min Scan# 389
 Delta R.T. 0.01 min
 Lab File: VU031822.D
 Acq: 08 May 2019 14:16

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B24

Tot Ion: 43 Resp: 24296
 Ion Ratio Lower Upper
 43 100
 58 24.4 0.0 53.6

