

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050819\
 Data File : VU031827.D
 Acq On : 08 May 2019 17:17
 Operator : JC/SP
 Sample : K2695-08
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XH2

Quant Time: May 09 06:29:52 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR050819WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu May 09 05:32:34 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	448235	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	442719	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	176775	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	148212	4.85	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	97.00%
7) Chloroethane-d5	1.68	69	126859	5.03	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	100.60%
11) 1,1-Dichloroethene-d2	2.27	63	216673	3.29	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	65.80%
20) 2-Butanone-d5	4.20	46	539677	45.25	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	90.50%
24) Chloroform-d	4.64	84	283185	4.52	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.40%
26) 1,2-Dichloroethane-d4	5.31	65	162051	4.26	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.20%
32) Benzene-d6	5.33	84	561000	4.95	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.00%
36) 1,2-Dichloropropane-d6	6.33	67	199602	4.80	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.00%
41) Toluene-d8	7.56	98	442386	4.56	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.20%
43) trans-1,3-Dichloropropene-	7.85	79	60944	4.17	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.40%
46) 2-Hexanone-d5	8.31	63	355038	48.07	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.14%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	151064	4.66	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.20%
64) 1,2-Dichlorobenzene-d4	11.86	152	159398	5.45	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	109.00%


Target Compounds					Ovalue
13) Acetone	2.34	43	46921	5.760 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050819\
Data File : VU031827.D
Acq On : 08 May 2019 17:17
Operator : JC/SP
Sample : K2695-08
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XH2

Quant Time: May 09 06:29:52 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR050819WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu May 09 05:32:34 2019
Response via : Initial Calibration

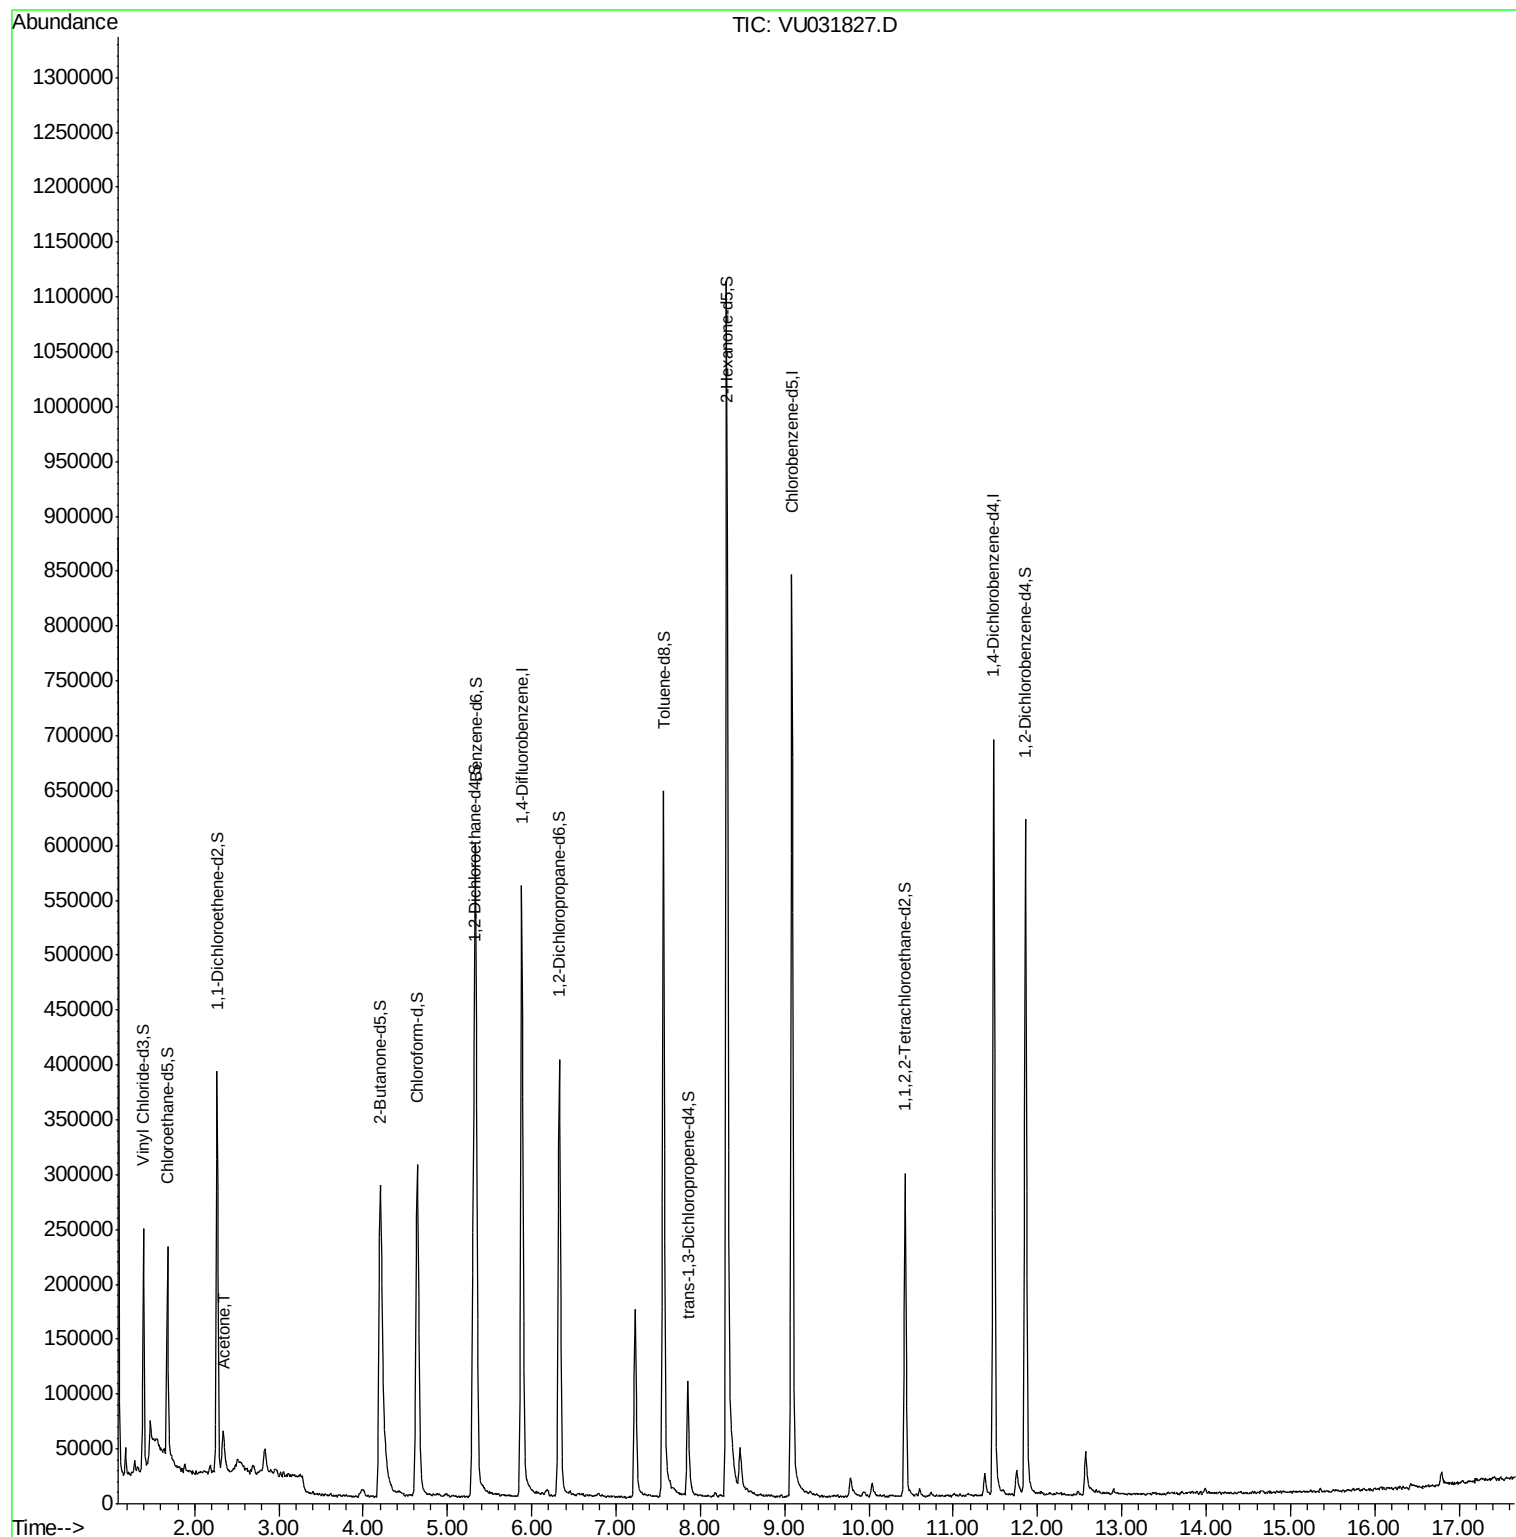

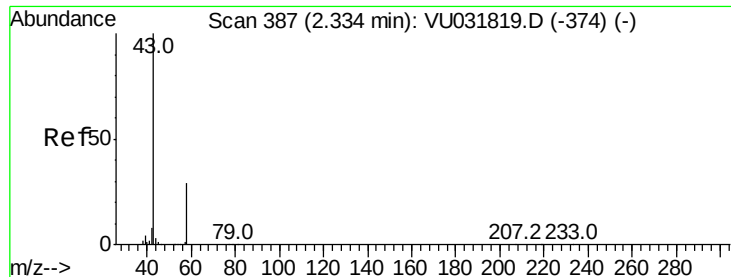

#13

Acetone

Concen: 5.760 ug/L

RT: 2.34 min Scan# 389

Delta R.T. 0.01 min

Lab File: VU031827.D

Acq: 08 May 2019 17:17

Instrument :
MSVOA_U
ClientSampleId :
C0XH2

Tot Ion: 43 Resp: 46921

Ion Ratio Lower Upper

43 100

58 29.9 0.0 53.6

