

Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU050819\
 Data File : VU031865.D
 Acq On : 09 May 2019 10:27
 Operator : JC/SP
 Sample : K2695-12
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XH6

Quant Time: May 20 03:00:03 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR050819WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri May 10 03:36:08 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	412069	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	418367	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	161935	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	123897	4.41	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	88.20%
7) Chloroethane-d5	1.68	69	112346	4.85	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	97.00%
11) 1,1-Dichloroethene-d2	2.27	63	191030	3.16	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	63.20%
20) 2-Butanone-d5	4.19	46	502737	45.85	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	91.70%
24) Chloroform-d	4.64	84	266352	4.62	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.40%
26) 1,2-Dichloroethane-d4	5.31	65	152528	4.36	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.20%
32) Benzene-d6	5.33	84	507223	4.74	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.80%
36) 1,2-Dichloropropane-d6	6.32	67	181607	4.62	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	92.40%
41) Toluene-d8	7.56	98	374808	4.09	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.80%
43) trans-1,3-Dichloropropene-	7.85	79	59696	4.32	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.40%
46) 2-Hexanone-d5	8.31	63	325433	46.62	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	93.24%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	141307	4.61	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.20%
64) 1,2-Dichlorobenzene-d4	11.86	152	144739	5.41	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	108.20%


Target Compounds					Ovalue
13) Acetone	2.32	43	43034	5.746 ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU050819\
Data File : VU031865.D
Acq On : 09 May 2019 10:27
Operator : JC/SP
Sample : K2695-12
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XH6

Quant Time: May 20 03:00:03 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR050819WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri May 10 03:36:08 2019
Response via : Initial Calibration

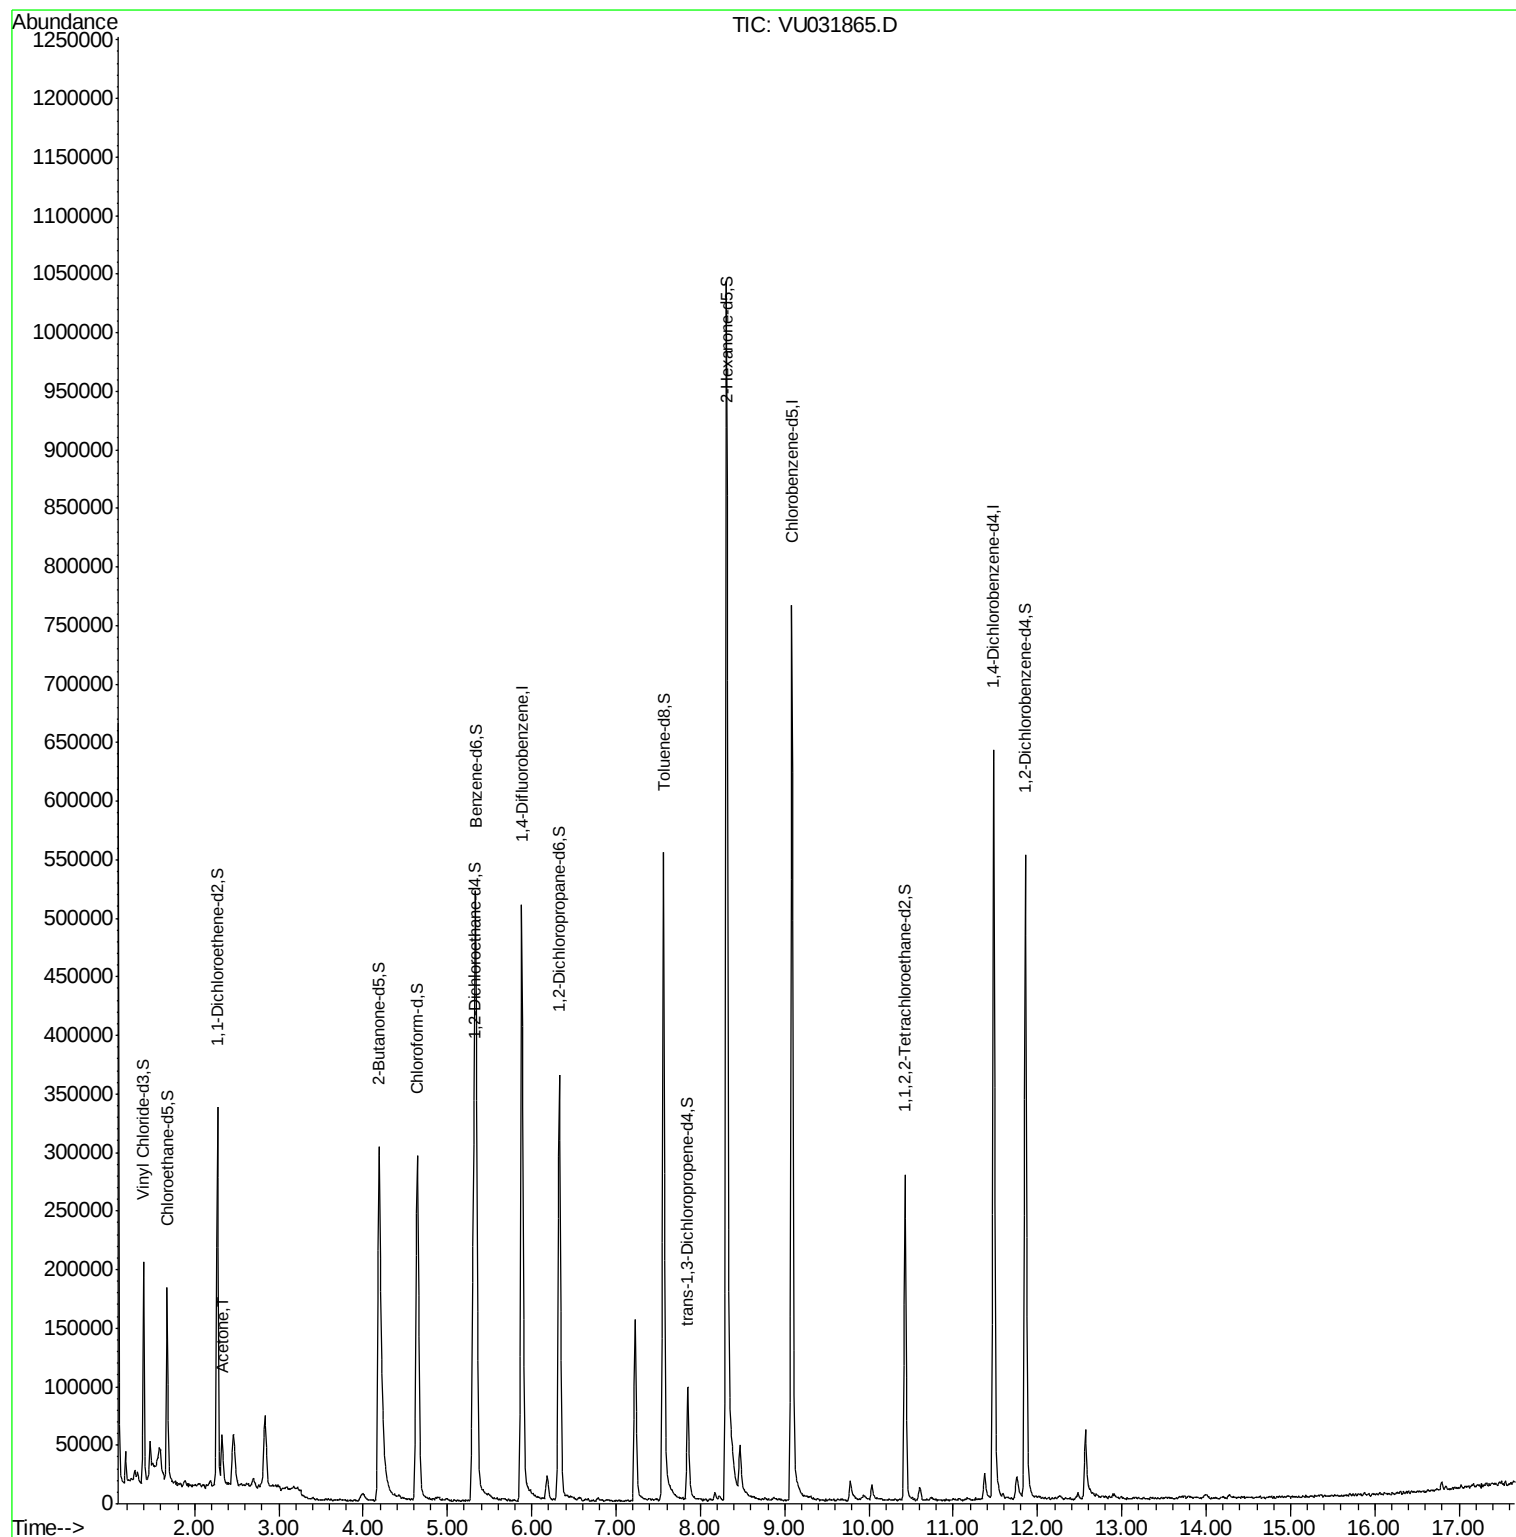

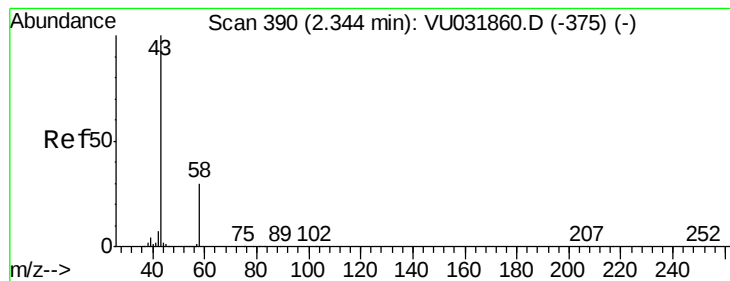

#13

Acetone

Concen: 5.746 ug/L

RT: 2.32 min Scan# 383

Delta R.T. -0.02 min

Lab File: VU031865.D

Acq: 09 May 2019 10:27

Instrument :

MSVOA_U

ClientSampleId :

C0XH6

Tot Ion: 43 Resp: 43034

Ion Ratio Lower Upper

43 100

58 30.8 0.0 53.6

