

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050819\
 Data File : VU031866.D
 Acq On : 09 May 2019 10:51
 Operator : JC/SP
 Sample : K2695-08
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XH2

Quant Time: May 10 04:18:58 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR050819WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri May 10 03:36:08 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	417258	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	426182	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	163520	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	126684	4.46	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	89.20%
7) Chloroethane-d5	1.68	69	116767	4.98	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	99.60%
11) 1,1-Dichloroethene-d2	2.27	63	191809	3.13	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	62.60%
20) 2-Butanone-d5	4.20	46	540373	48.67	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	97.34%
24) Chloroform-d	4.64	84	274326	4.70	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.00%
26) 1,2-Dichloroethane-d4	5.31	65	156086	4.41	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.20%
32) Benzene-d6	5.33	84	511203	4.69	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.80%
36) 1,2-Dichloropropane-d6	6.33	67	186464	4.66	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.20%
41) Toluene-d8	7.56	98	393080	4.21	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.20%
43) trans-1,3-Dichloropropene-	7.85	79	58496	4.16	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.20%
46) 2-Hexanone-d5	8.31	63	348741	49.05	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	98.10%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	147961	4.74	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	94.80%
64) 1,2-Dichlorobenzene-d4	11.86	152	149606	5.53	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	110.60%


Target Compounds					Ovalue
13) Acetone	2.35	43	45822	6.043 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050819\
Data File : VU031866.D
Acq On : 09 May 2019 10:51
Operator : JC/SP
Sample : K2695-08
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XH2

Quant Time: May 10 04:18:58 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR050819WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri May 10 03:36:08 2019
Response via : Initial Calibration

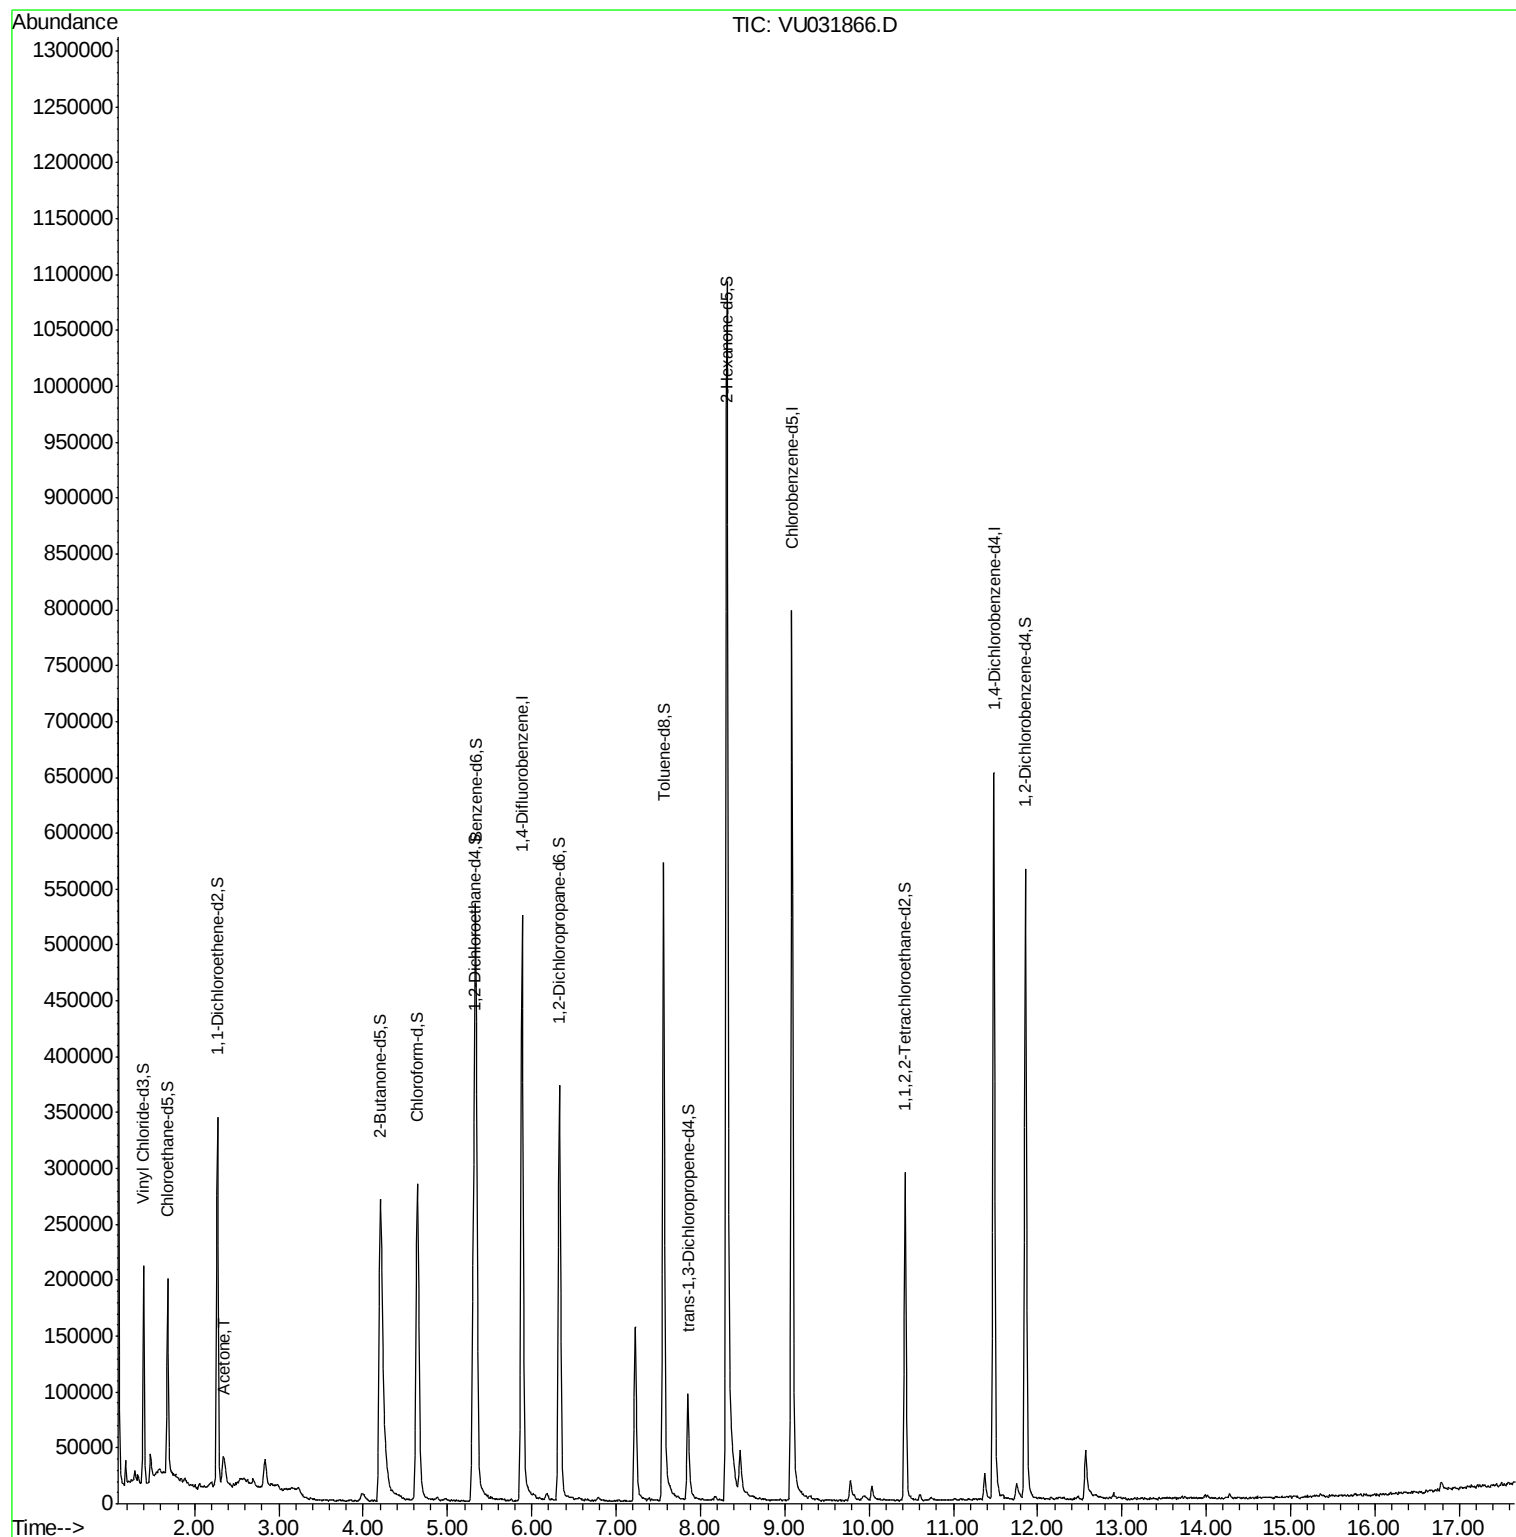

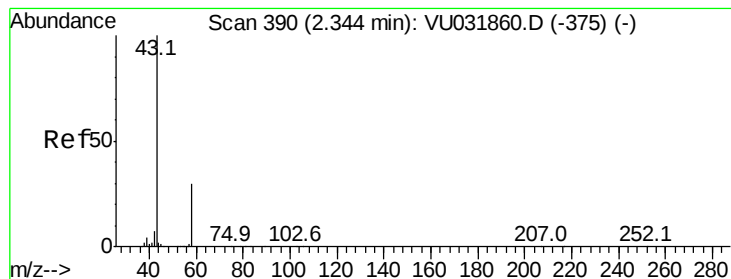

#13

Acetone

Concen: 6.043 ug/L

RT: 2.35 min Scan# 391

Delta R.T. 0.00 min

Lab File: VU031866.D

Acq: 09 May 2019 10:51

Instrument :
MSVOA_U
ClientSampleId :
C0XH2

Tot Ion: 43 Resp: 45822

Ion Ratio Lower Upper

43 100

58 27.7 0.0 53.6

