

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050819\
 Data File : VU031873.D
 Acq On : 09 May 2019 13:45
 Operator : JC/SP
 Sample : K2706-03DL 100X
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0JP3DL

Quant Time: May 10 04:55:34 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR050819WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri May 10 03:36:08 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	412485	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	422722	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	154975	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	121182	4.31	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	86.20%
7) Chloroethane-d5	1.68	69	108907	4.70	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	94.00%
11) 1,1-Dichloroethene-d2	2.27	63	181627	3.00	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	60.00%
20) 2-Butanone-d5	4.21	46	500711	45.62	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	91.24%
24) Chloroform-d	4.64	84	257143	4.46	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.20%
26) 1,2-Dichloroethane-d4	5.31	65	147061	4.20	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.00%
32) Benzene-d6	5.33	84	483848	4.47	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.40%
36) 1,2-Dichloropropane-d6	6.33	67	174958	4.40	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	88.00%
41) Toluene-d8	7.56	98	361687	3.91	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	78.20%
43) trans-1,3-Dichloropropene-	7.85	79	55284	3.96	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	79.20%
46) 2-Hexanone-d5	8.31	63	319417	45.29	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	90.58%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	139771	4.51	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	90.20%
64) 1,2-Dichlorobenzene-d4	11.86	152	131033	5.11	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.20%


Target Compounds					Ovalue
13) Acetone	2.34	43	383476	51.154 ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU050819\
Data File : VU031873.D
Acq On : 09 May 2019 13:45
Operator : JC/SP
Sample : K2706-03DL 100X
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0JP3DL

Quant Time: May 10 04:55:34 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR050819WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri May 10 03:36:08 2019
Response via : Initial Calibration

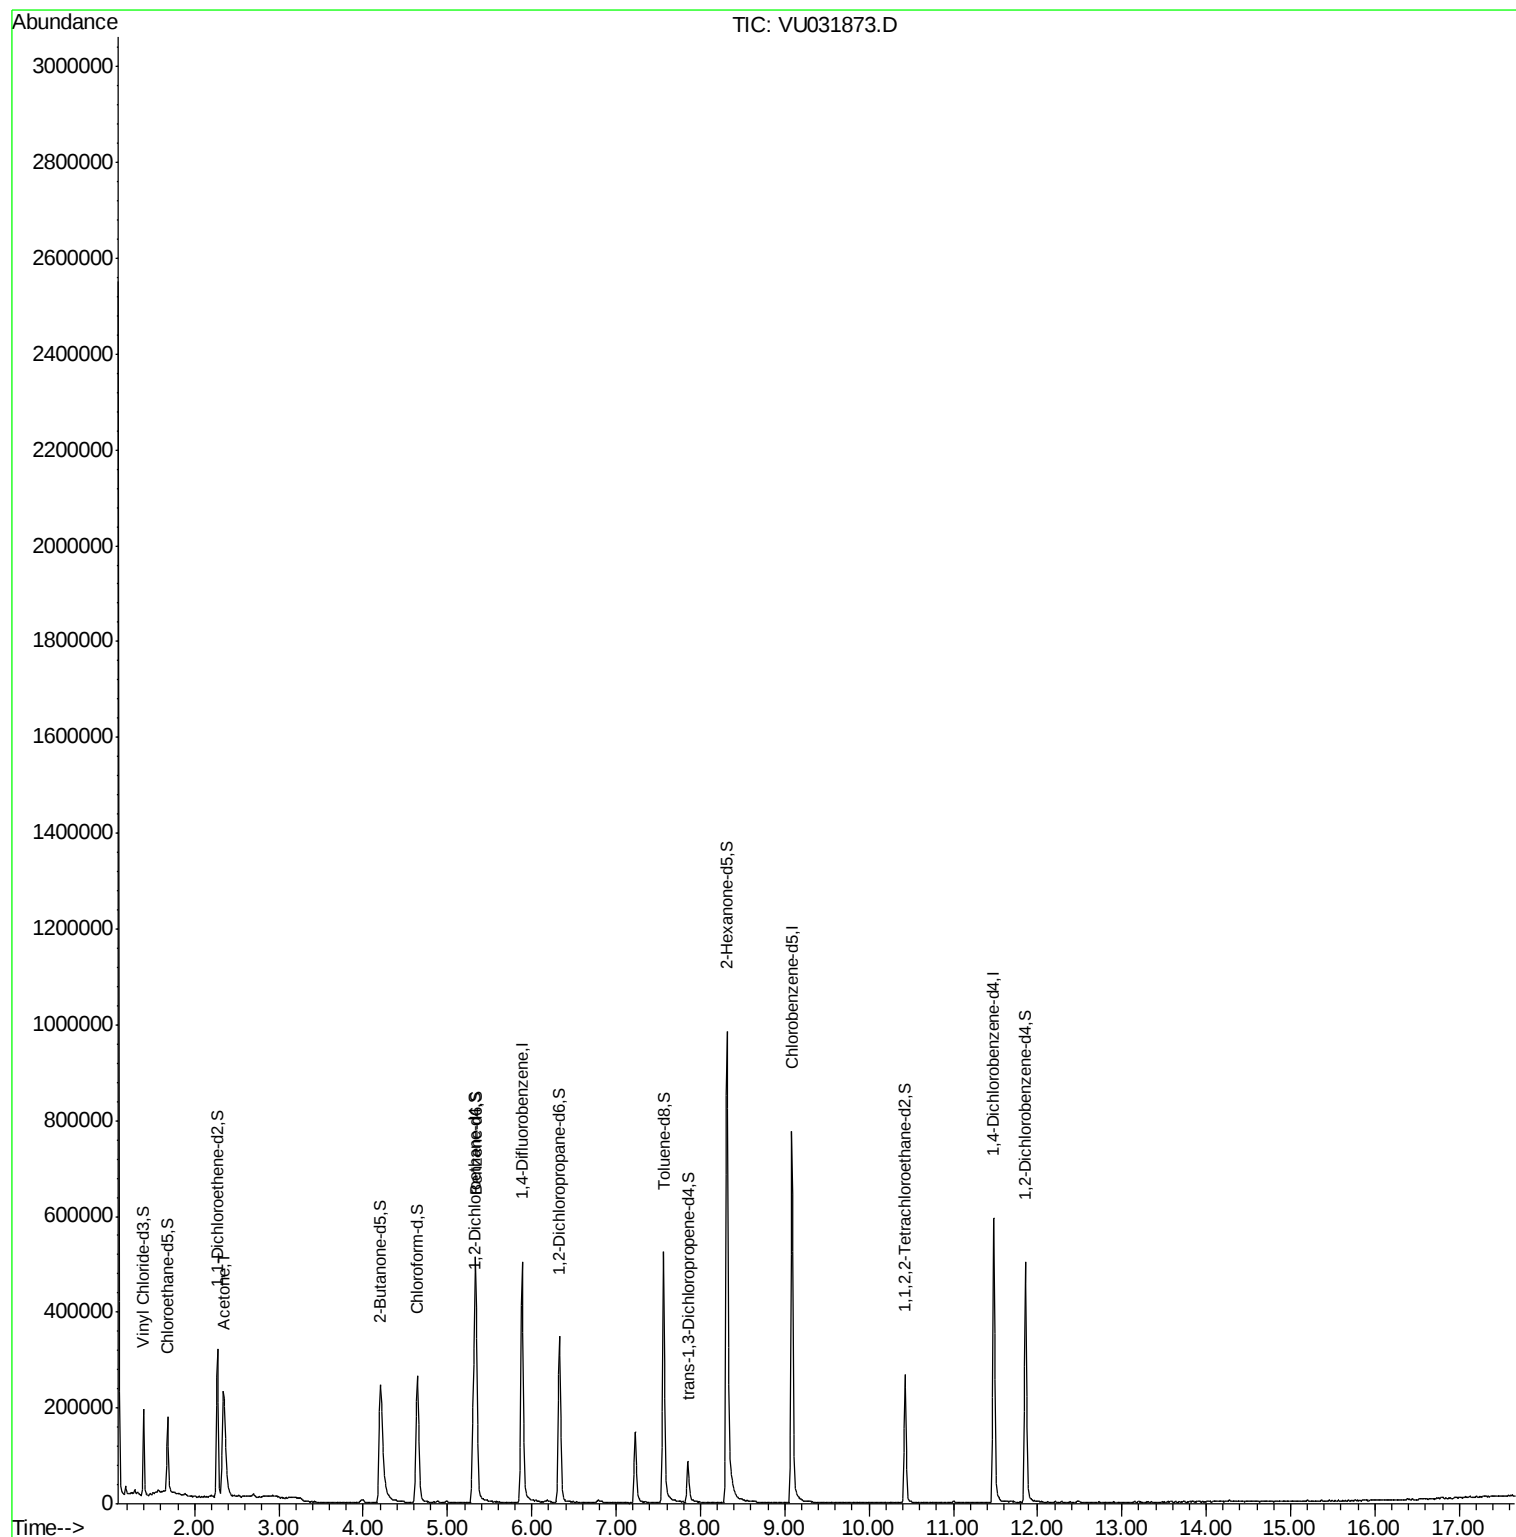

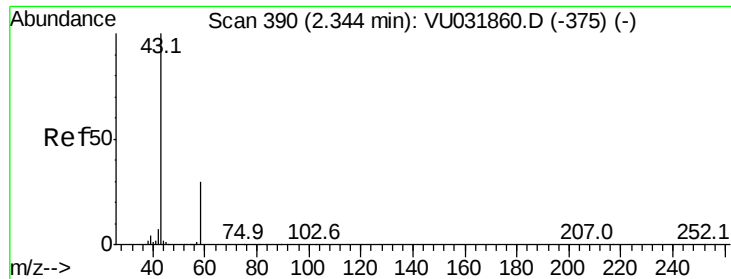

#13

Acetone

Concen: 51.154 ug/L

RT: 2.34 min Scan# 390

Delta R.T. -0.00 min

Lab File: VU031873.D

Acq: 09 May 2019 13:45

Instrument :

MSVOA_U

ClientSampleId :

C0JP3DL

Tot Ion: 43 Resp: 383476

Ion Ratio Lower Upper

43 100

58 31.5 0.0 53.6

