

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050819\
 Data File : VU031866.D
 Acq On : 09 May 2019 10:51
 Operator : JC/SP
 Sample : K2695-08
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XH2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.1

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR050819WMA.M

Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	23	28	34	rBV2	22609	23106	1.07%	0.165%
2	1.395	86	95	106	rBV	194381	222167	10.26%	1.585%
3	1.479	115	121	127	rBV	24359	30342	1.40%	0.216%
4	1.682	177	184	199	rVB	173213	208133	9.61%	1.485%
5	2.270	357	367	381	rBV	329038	486934	22.49%	3.473%
6	2.344	381	390	408	rVB3	23814	62165	2.87%	0.443%
7	2.836	532	543	554	rBV	24798	56715	2.62%	0.405%
8	4.206	955	969	1009	rBV	269922	933512	43.12%	6.659%
9	4.643	1087	1105	1135	rBV2	282215	718528	33.19%	5.125%
10	5.334	1298	1320	1354	rBV2	534910	1548500	71.53%	11.046%
11	5.884	1476	1491	1512	rBV	524773	1064875	49.19%	7.596%
12	6.328	1614	1629	1654	rBV	370647	763794	35.28%	5.448%
13	7.225	1893	1908	1925	rBV	156009	300310	13.87%	2.142%
14	7.562	2000	2013	2031	rBV	570765	1040617	48.07%	7.423%
15	7.852	2090	2103	2130	rBV	94683	189579	8.76%	1.352%
16	8.315	2233	2247	2286	rBV	1091069	2164676	100.00%	15.441%
17	8.472	2287	2296	2313	rVB5	38794	81979	3.79%	0.585%
18	9.086	2474	2487	2512	rBV	794994	1370102	63.29%	9.773%
19	9.778	2693	2702	2712	rBV2	18217	33231	1.54%	0.237%
20	10.035	2774	2782	2797	rBV7	12712	23278	1.08%	0.166%
21	10.427	2893	2904	2920	rBV	292934	474828	21.94%	3.387%
22	11.372	3188	3198	3212	rBV6	23310	42418	1.96%	0.303%
23	11.482	3220	3232	3254	rBV	649232	1079384	49.86%	7.700%
24	11.752	3303	3316	3327	rBV7	14355	34496	1.59%	0.246%
25	11.855	3335	3348	3371	rBV	562049	960862	44.39%	6.854%
26	12.569	3561	3570	3598	rBV6	44345	104324	4.82%	0.744%


Sum of corrected areas: 14018855

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU050819\
Data File : VU031866.D
Acq On : 09 May 2019 10:51
Operator : JC/SP
Sample : K2695-08
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :
C0XH2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR050819WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

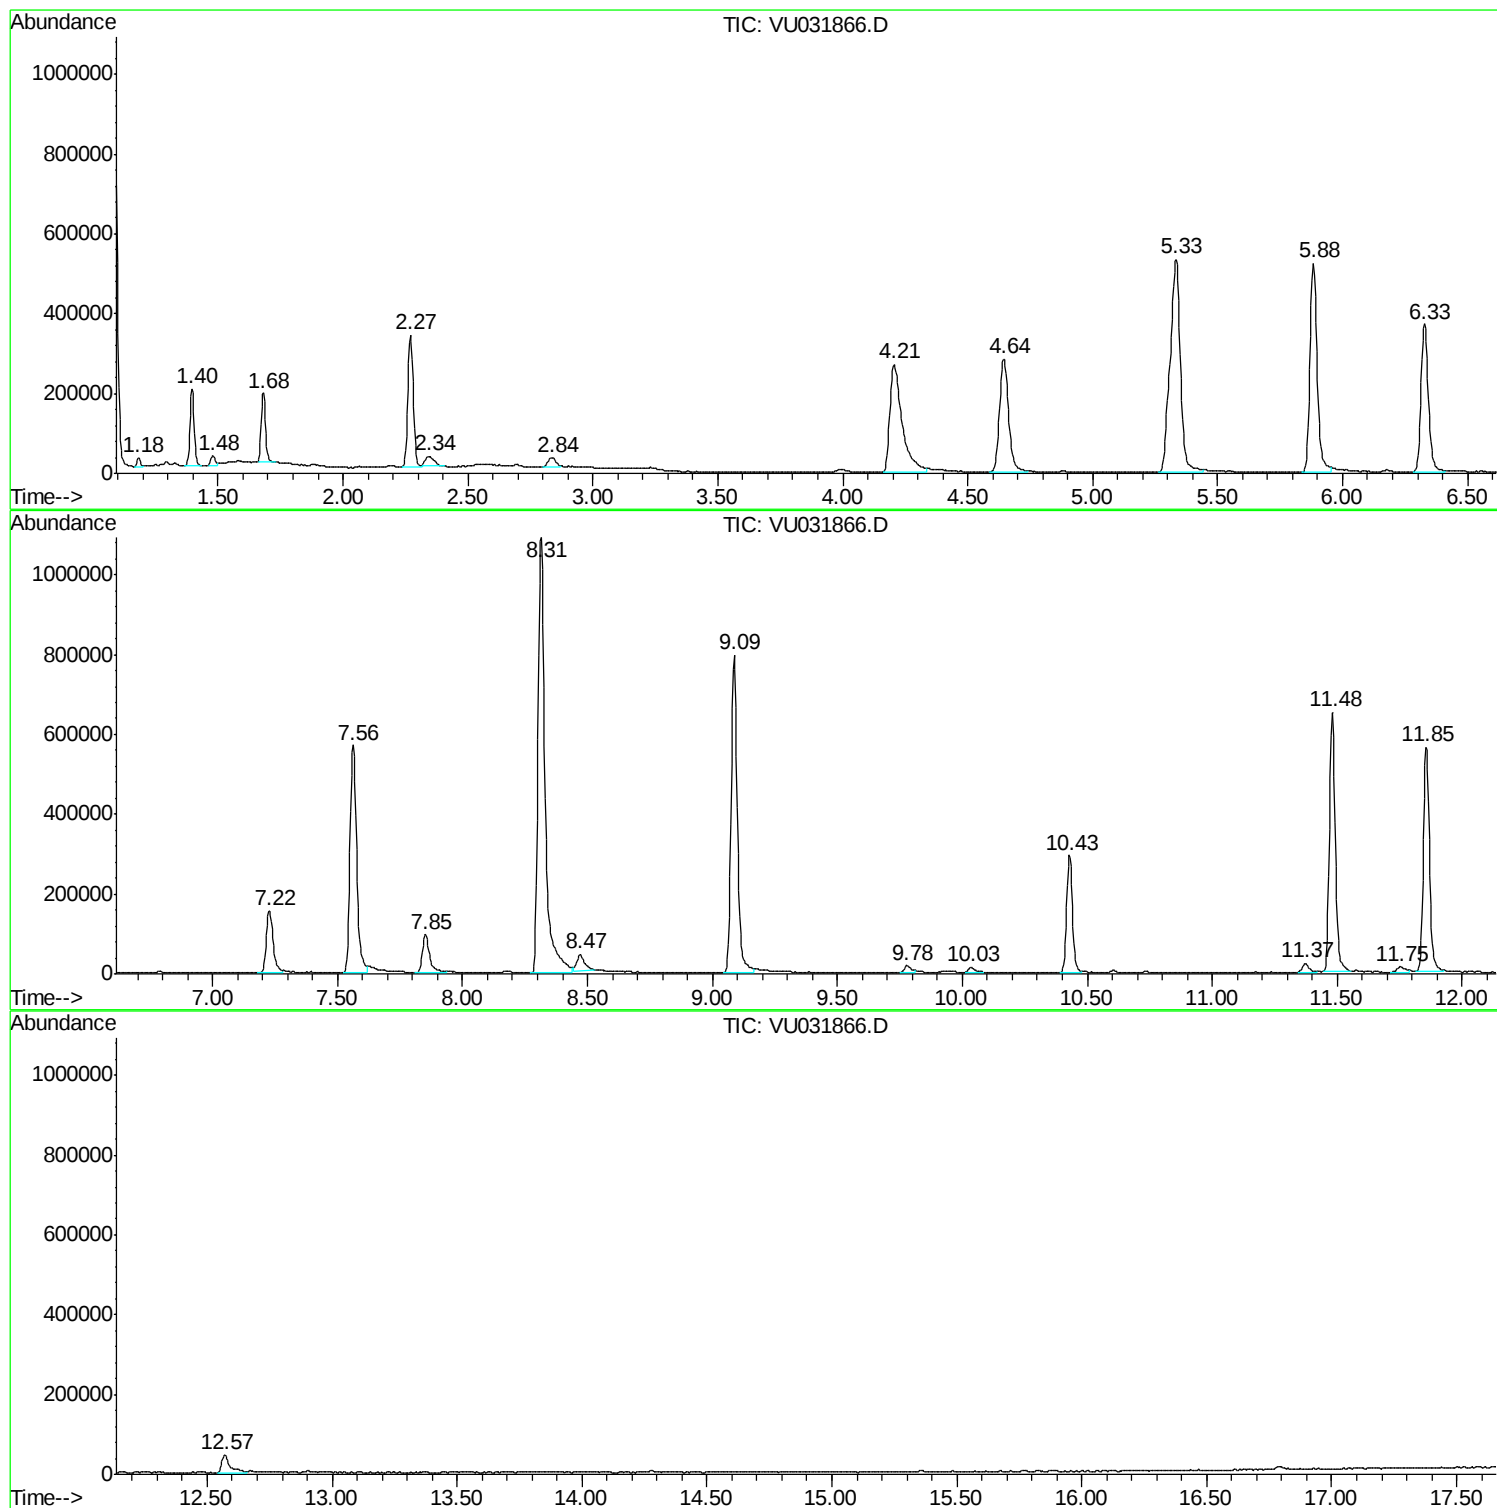

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050819\
Data File : VU031866.D
Acq On : 09 May 2019 10:51
Operator : JC/SP
Sample : K2695-08
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XH2










Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR050819WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.22	1.41 ug/L	300310	1,4-Difluorobenzene	5.88

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Borane, diethyl-1-propynyl-	108	C7H13B	022405-32-9	38
2		Thiophosgene	114	CCl2S	000463-71-8	37
3		Methane, oxybis[chloro-	114	C2H4Cl2O	000542-88-1	25
4		Methane, oxybis[chloro-	114	C2H4Cl2O	000542-88-1	25
5		3-Thiatricyclo[3.1.1.0(2,4)]heptane	112	C6H8S	1000221-37-0	9

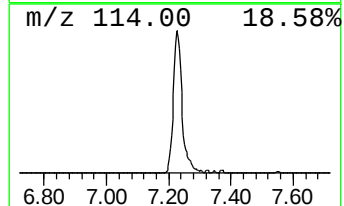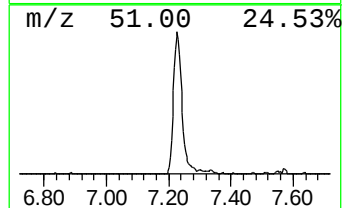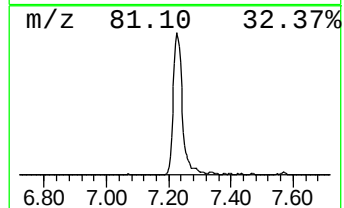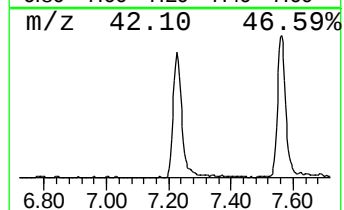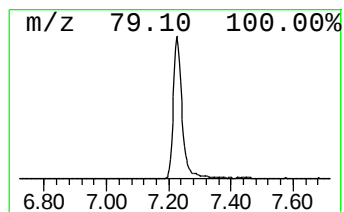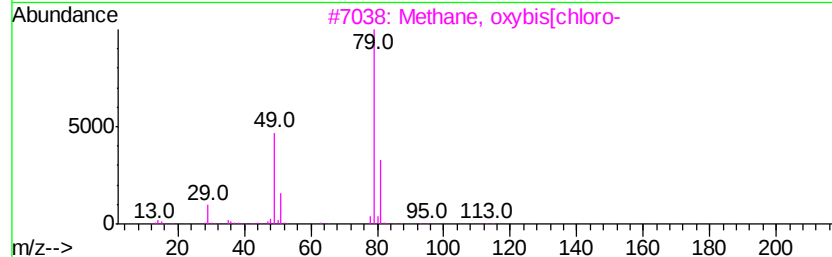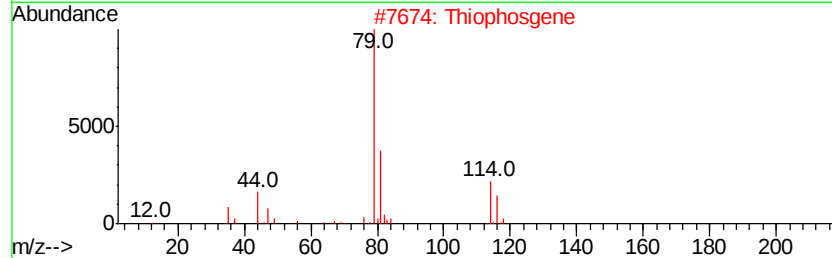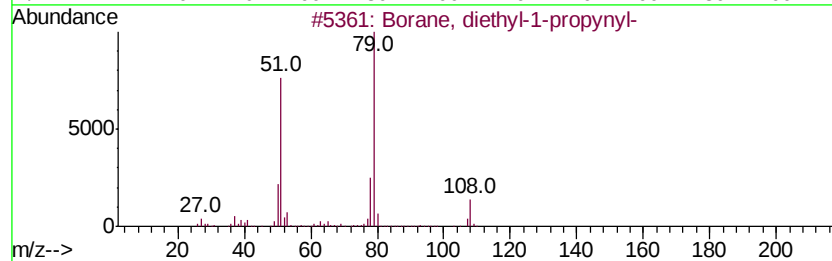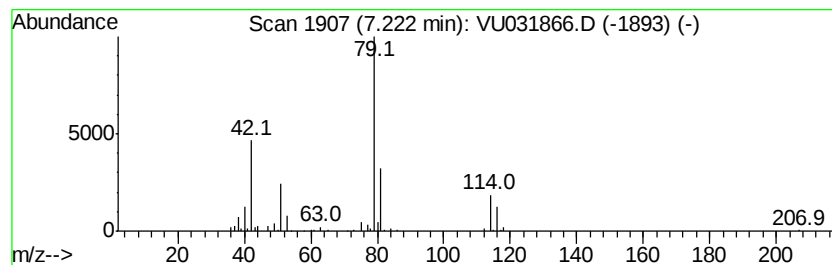

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU050819\
Data File : VU031866.D
Acq On : 09 May 2019 10:51
Operator : JC/SP
Sample : K2695-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XH2

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR050819WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	7.22	1.4	ug/L	300310	1	5.88	1064880	5.0