


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050819\
 Data File : VU031812.D
 Acq On : 08 May 2019 08:35
 Operator : JC/SP
 Sample : BFB05
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB05

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR050819WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu May 09 06:57:14 2019

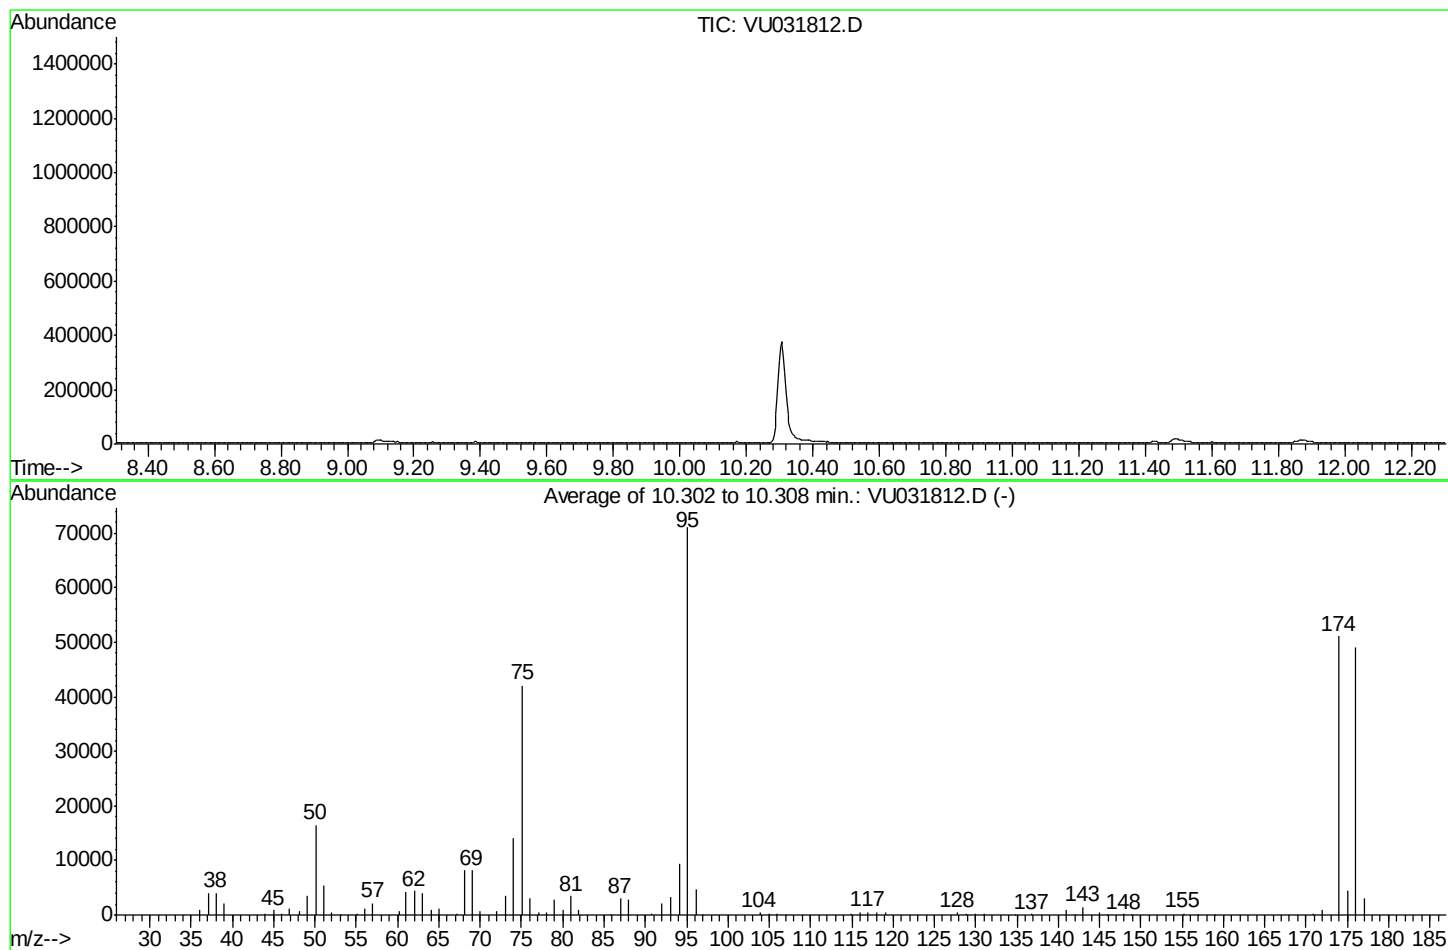

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2853

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.2	16473	PASS
75	95	30	80	59.3	42122	PASS
95	95	100	100	100.0	71077	PASS
96	95	5	9	6.7	4750	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	71.9	51090	PASS
175	174	5	9	8.6	4385	PASS
176	174	95	101	96.1	49080	PASS
177	176	5	9	6.4	3133	PASS

Scan 2853 (10.263 min): VU031812.D
BFB05

m/z	Abundance
35.90	105.0
40.00	4241.0
44.00	1493.0
207.00	104.0

Instrument :
MSVOA_U
ClientSampleId :
BFB05

m/z	Abundance
36.00	855.0
37.00	3893.0
38.00	4066.0
39.00	2196.0
40.00	3625.0
44.00	1916.0
44.90	880.0
46.00	217.0
46.90	1133.0
48.10	826.0
49.10	3392.0
50.00	16360.0
51.10	5499.0
52.00	312.0
53.00	144.0
55.10	459.0
56.00	1185.0
57.00	2130.0
60.10	676.0
61.00	4285.0
62.00	4258.0
63.10	3694.0
64.10	935.0
65.00	1162.0
67.20	213.0
68.10	8008.0
69.00	8158.0
70.00	756.0
72.00	618.0
73.10	3454.0
74.00	13560.0
75.10	41968.0
76.00	2771.0
77.20	366.0
78.00	453.0
78.90	2951.0
80.00	879.0
81.00	3449.0
81.90	836.0
87.00	2855.0
88.00	2517.0
90.80	286.0
92.00	2232.0
93.00	2834.0
94.10	9039.0
95.10	69808.0
96.10	4730.0
103.90	431.0
104.90	120.0
106.00	280.0
107.00	107.0
115.00	119.0
116.00	376.0
116.90	613.0
117.90	364.0
119.00	454.0
127.80	441.0
128.90	149.0
130.00	233.0
131.00	209.0
136.90	167.0
141.00	998.0
142.00	120.0
143.00	1350.0
144.90	404.0
147.90	212.0
148.80	115.0
155.20	236.0
156.90	115.0
171.00	236.0
172.00	815.0
174.00	49336.0
175.00	3980.0
176.00	46680.0
177.00	3167.0
207.20	138.0

Instrument :
MSVOA_U
ClientSampleId :
BFB05

m/z	Abundance
36.00	971.0
37.10	4097.0
38.00	4050.0
39.00	2266.0
39.90	3545.0
44.00	1859.0
44.90	926.0
46.00	183.0
46.90	1358.0
48.00	751.0
49.10	3605.0
50.10	17024.0
51.10	5449.0
52.00	405.0
55.10	348.0
56.00	1303.0
57.00	2211.0
60.20	682.0
61.00	4352.0
62.00	4577.0
63.00	4220.0
64.10	1015.0
65.00	1231.0
67.20	292.0
68.00	8348.0
69.00	8432.0
70.00	788.0
72.00	709.0
73.10	3544.0
74.00	14547.0
75.10	43920.0
76.00	2971.0
77.10	354.0
78.10	551.0
78.90	2872.0
80.00	903.0
81.00	3587.0
82.00	933.0
85.90	115.0
87.00	3206.0
88.00	2751.0
90.80	301.0
92.00	2304.0
93.00	3262.0
94.10	9974.0
95.10	72888.0
96.10	4892.0
97.00	139.0
103.90	471.0
105.00	151.0
106.00	240.0
115.00	183.0
116.00	385.0
116.90	620.0
118.00	440.0
119.10	434.0
127.80	454.0
128.90	267.0
130.00	267.0
131.00	212.0
134.80	134.0
136.80	186.0
141.00	945.0
143.00	1511.0
145.00	452.0
145.90	149.0
147.90	219.0
155.20	291.0
158.90	115.0
171.00	204.0
172.00	865.0
174.00	52856.0
175.10	4552.0
176.00	50488.0
177.00	3179.0
207.20	128.0

Instrument :
MSVOA_U
ClientSampleId :
BFB05

m/z	Abundance
36.00	990.0
37.00	4039.0
38.00	3939.0
39.00	2109.0
40.00	3499.0
44.00	1691.0
45.00	846.0
46.00	174.0
46.90	1244.0
48.00	627.0
49.00	3291.0
50.10	16036.0
51.10	4974.0
52.00	365.0
55.10	234.0
56.00	1327.0
57.00	2021.0
60.20	632.0
61.00	3979.0
62.00	4334.0
63.00	4183.0
64.10	962.0
65.00	1208.0
67.20	267.0
68.00	7978.0
69.00	7869.0
70.00	695.0
72.00	696.0
73.00	3481.0
74.00	13959.0
75.10	40480.0
76.00	3091.0
77.00	384.0
78.00	479.0
78.90	2700.0
80.00	998.0
81.00	3412.0
82.00	973.0
85.80	179.0
87.00	3015.0
88.00	2878.0
90.80	272.0
92.00	1909.0
93.00	3445.0
94.10	9316.0
95.10	70536.0
96.10	4629.0
97.00	191.0
103.80	429.0
105.00	161.0
105.80	178.0
114.90	202.0
116.00	376.0
117.00	544.0
118.10	393.0
119.00	404.0
127.80	377.0
128.90	283.0
129.90	219.0
131.00	161.0
134.80	160.0
136.80	129.0
140.90	693.0
143.00	1513.0
145.10	464.0
145.90	155.0
148.00	194.0
155.20	237.0
158.90	149.0
170.90	227.0
172.00	860.0
174.00	51080.0
175.10	4624.0
176.00	50072.0
177.00	3055.0

Instrument :
MSVOA_U
ClientSampleId :
BFB05