


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU050820\
 Data File : VU038079.D
 Acq On : 08 May 2020 09:17
 Operator : JC/MD
 Sample : BFB20
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB20

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR050720WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Sat May 09 00:11:09 2020

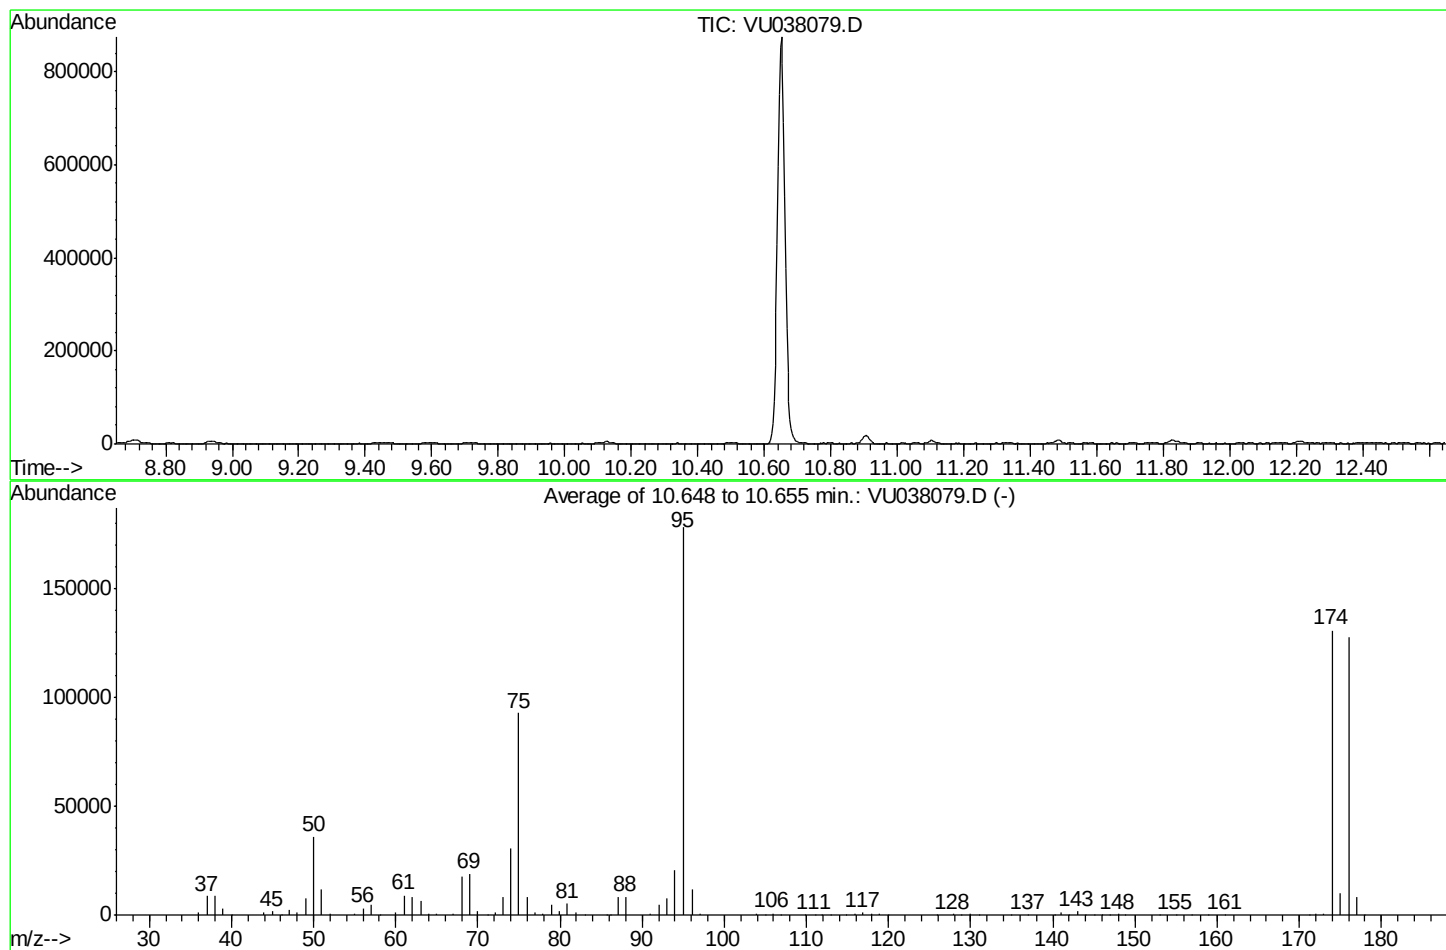

AutoFind: Scans 2895, 2896, 2897; Background Corrected with Scan 2881

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.3	36130	PASS
75	95	30	80	52.1	92922	PASS
95	95	100	100	100.0	178282	PASS
96	95	5	9	6.6	11737	PASS
173	174	0.00	2	0.3	449	PASS
174	95	50	120	73.4	130850	PASS
175	174	5	9	7.5	9871	PASS
176	174	95	101	97.6	127677	PASS
177	176	5	9	6.3	8045	PASS

m/z	Abundance
36.00	1408.0
37.00	8878.0
38.00	9037.0
39.00	3496.0
40.00	550.0
44.00	1921.0
45.00	1452.0
47.00	2374.0
47.90	1030.0
49.00	8413.0
50.00	37544.0
51.00	12112.0
52.00	557.0
55.00	570.0
56.00	2901.0
57.00	5047.0
58.10	267.0
60.00	1377.0
61.00	9268.0
62.00	8766.0
63.10	6727.0
64.00	741.0
65.00	778.0
67.10	554.0
68.00	17792.0
69.00	19592.0
70.00	1675.0
72.10	1066.0
73.00	8647.0
74.00	31040.0
75.00	94240.0
76.00	8190.0
77.00	1242.0
77.90	735.0
79.00	4636.0
79.90	1728.0
80.90	5220.0
81.90	1204.0
83.10	110.0
85.70	130.0
87.00	8113.0
88.00	8582.0
91.00	692.0
92.00	4571.0
93.00	7850.0
94.00	20784.0
95.00	179008.0
96.00	11943.0
97.00	339.0
103.90	652.0
105.00	180.0
105.90	723.0
106.90	118.0
111.00	114.0
111.90	114.0
112.90	102.0
114.80	221.0
115.90	659.0
116.90	1089.0
117.90	631.0
118.90	695.0
127.90	602.0
128.90	212.0
129.90	574.0
131.00	215.0
134.90	274.0
136.90	219.0
140.20	103.0
141.00	1360.0
141.90	159.0
142.90	1583.0
143.90	142.0
145.00	104.0
145.90	243.0
146.90	132.0
147.90	345.0
148.90	123.0
155.00	344.0
157.00	244.0
158.90	192.0
161.00	134.0
172.00	821.0
173.00	1348.0
174.00	128328.0
175.00	10006.0
176.00	125088.0
177.00	7884.0
177.90	181.0

Instrument :
MSVOA_U
ClientSampleId :
BFB20

m/z	Abundance
36.00	1307.0
37.00	8948.0
38.00	8996.0
39.00	3302.0
40.00	504.0
44.00	1909.0
45.00	1727.0
47.00	2333.0
47.90	1244.0
49.00	7942.0
50.00	37384.0
51.00	12224.0
52.00	542.0
55.00	547.0
56.00	3129.0
57.00	5070.0
58.10	206.0
60.00	1433.0
61.00	9287.0
62.00	8820.0
63.10	6669.0
64.00	737.0
65.00	762.0
67.00	520.0
68.00	18224.0
69.00	19472.0
70.00	1765.0
71.20	118.0
72.00	1029.0
73.00	8817.0
74.00	31160.0
75.00	96032.0
76.00	8496.0
77.00	1151.0
78.00	771.0
78.90	4669.0
79.90	1770.0
80.90	5501.0
81.90	1283.0
83.10	128.0
85.70	143.0
87.00	8219.0
88.00	8639.0
91.00	680.0
92.00	4740.0
93.00	8000.0
94.00	21456.0
95.00	183872.0
96.10	12089.0
97.00	410.0
103.90	668.0
105.00	218.0
105.90	696.0
106.90	131.0
109.90	171.0
111.00	119.0
114.90	210.0
115.90	679.0
116.90	1048.0
117.90	561.0
118.90	800.0
119.90	100.0
125.80	147.0
127.90	567.0
128.90	187.0
129.90	501.0
131.00	255.0
135.00	259.0
136.90	257.0
141.00	1362.0
141.90	175.0
143.00	1699.0
143.90	162.0
145.10	130.0
145.90	228.0
146.90	125.0
148.00	363.0
148.80	118.0
153.00	104.0
155.00	331.0
156.90	285.0
158.90	160.0
161.00	160.0
172.00	847.0
174.00	135168.0
175.00	10171.0
176.00	132416.0
177.00	8322.0
177.90	259.0

Instrument :
MSVOA_U
ClientSampleId :
BFB20

m/z	Abundance
36.00	1049.0
37.00	8371.0
38.00	7813.0
39.00	2701.0
40.00	448.0
44.00	1933.0
45.00	1670.0
46.10	123.0
47.00	2156.0
47.90	1267.0
49.00	6688.0
50.00	33464.0
51.00	11381.0
52.00	495.0
55.00	473.0
56.00	2961.0
57.00	4663.0
58.00	164.0
60.00	1426.0
61.00	8586.0
62.00	8081.0
63.00	6214.0
64.00	667.0
65.00	638.0
67.00	448.0
68.00	17056.0
69.00	18208.0
70.00	1658.0
72.00	918.0
73.00	7766.0
74.00	28832.0
75.00	88496.0
76.00	7686.0
77.00	1057.0
78.00	828.0
78.90	4427.0
79.90	1604.0
80.90	4998.0
81.90	1146.0
83.10	125.0
86.10	247.0
87.00	7747.0
88.00	7730.0
90.90	624.0
92.00	4764.0
93.00	7293.0
94.00	20232.0
95.00	171968.0
96.10	11180.0
97.00	450.0
103.90	578.0
104.90	217.0
105.90	574.0
106.90	158.0
109.90	191.0
111.00	123.0
114.90	211.0
115.90	600.0
116.90	920.0
117.90	464.0
118.90	856.0
119.90	131.0
125.80	189.0
127.90	465.0
128.90	170.0
129.90	413.0
131.00	253.0
135.00	242.0
137.00	322.0
141.00	1310.0
141.90	156.0
143.00	1585.0
143.90	183.0
145.10	136.0
146.00	236.0
148.00	285.0
155.00	249.0
156.90	357.0
160.90	133.0
171.20	148.0
172.00	787.0
174.00	129056.0
175.00	9438.0
176.00	125528.0
177.00	7929.0
177.90	257.0

Instrument :
MSVOA_U
ClientSampleId :
BFB20

Scan 2881 (10.603 min): VU038079.D
BFB20

m/z	Abundance
39.90	256.0
41.10	109.0
43.90	762.0

Instrument :
MSVOA_U
ClientSampleId :
BFB20