

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050823\
 Data File : VU054109.D
 Acq On : 09 May 2023 03:00
 Operator : JC/MD
 Sample : 02663-19
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: May 09 06:14:13 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat May 06 01:14:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.244	114	219799	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.411	117	210754	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.806	152	106477	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	60571	36.437	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	72.880%		
7) Chloroethane-d5	1.906	69	53744	49.252	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	98.500%		
11) 1,1-Dichloroethene-d2	2.562	63	94119	31.922	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	63.840%		
21) 2-Butanone-d5	4.617	46	98185	103.559	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	103.560%		
24) Chloroform-d	5.057	84	147125	48.188	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	96.380%		
26) 1,2-Dichloroethane-d4	5.694	65	96536	49.246	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	98.500%		
32) Benzene-d6	5.723	84	284972	45.937	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	91.880%		
36) 1,2-Dichloropropane-d6	6.684	67	93243	47.612	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	95.220%		
41) Toluene-d8	7.893	98	251542	44.912	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	89.820%		
43) trans-1,3-Dichloroprop...	8.173	79	43230	44.605	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	89.220%		
47) 2-Hexanone-d5	8.629	63	63538	90.581	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	90.580%		
56) 1,1,2,2-Tetrachloroeth...	10.751	84	130023	50.404	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	100.800%		
66) 1,2-Dichlorobenzene-d4	12.185	152	105384	50.664	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	101.320%		
Target Compounds						Qvalue
12) 1,1-Dichloroethene	2.559	96	848	0.665	ug/L #	1
37) 1,2-Dichloropropane	6.684	63	10129	5.836	ug/L #	87
60) 1,2,3-Trichloropropane	11.806	75	11146	5.636	ug/L #	64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050823\
Data File : VU054109.D
Acq On : 09 May 2023 03:00
Operator : JC/MD
Sample : 02663-19
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: May 09 06:14:13 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis
QLast Update : Sat May 06 01:14:00 2023
Response via : Initial Calibration

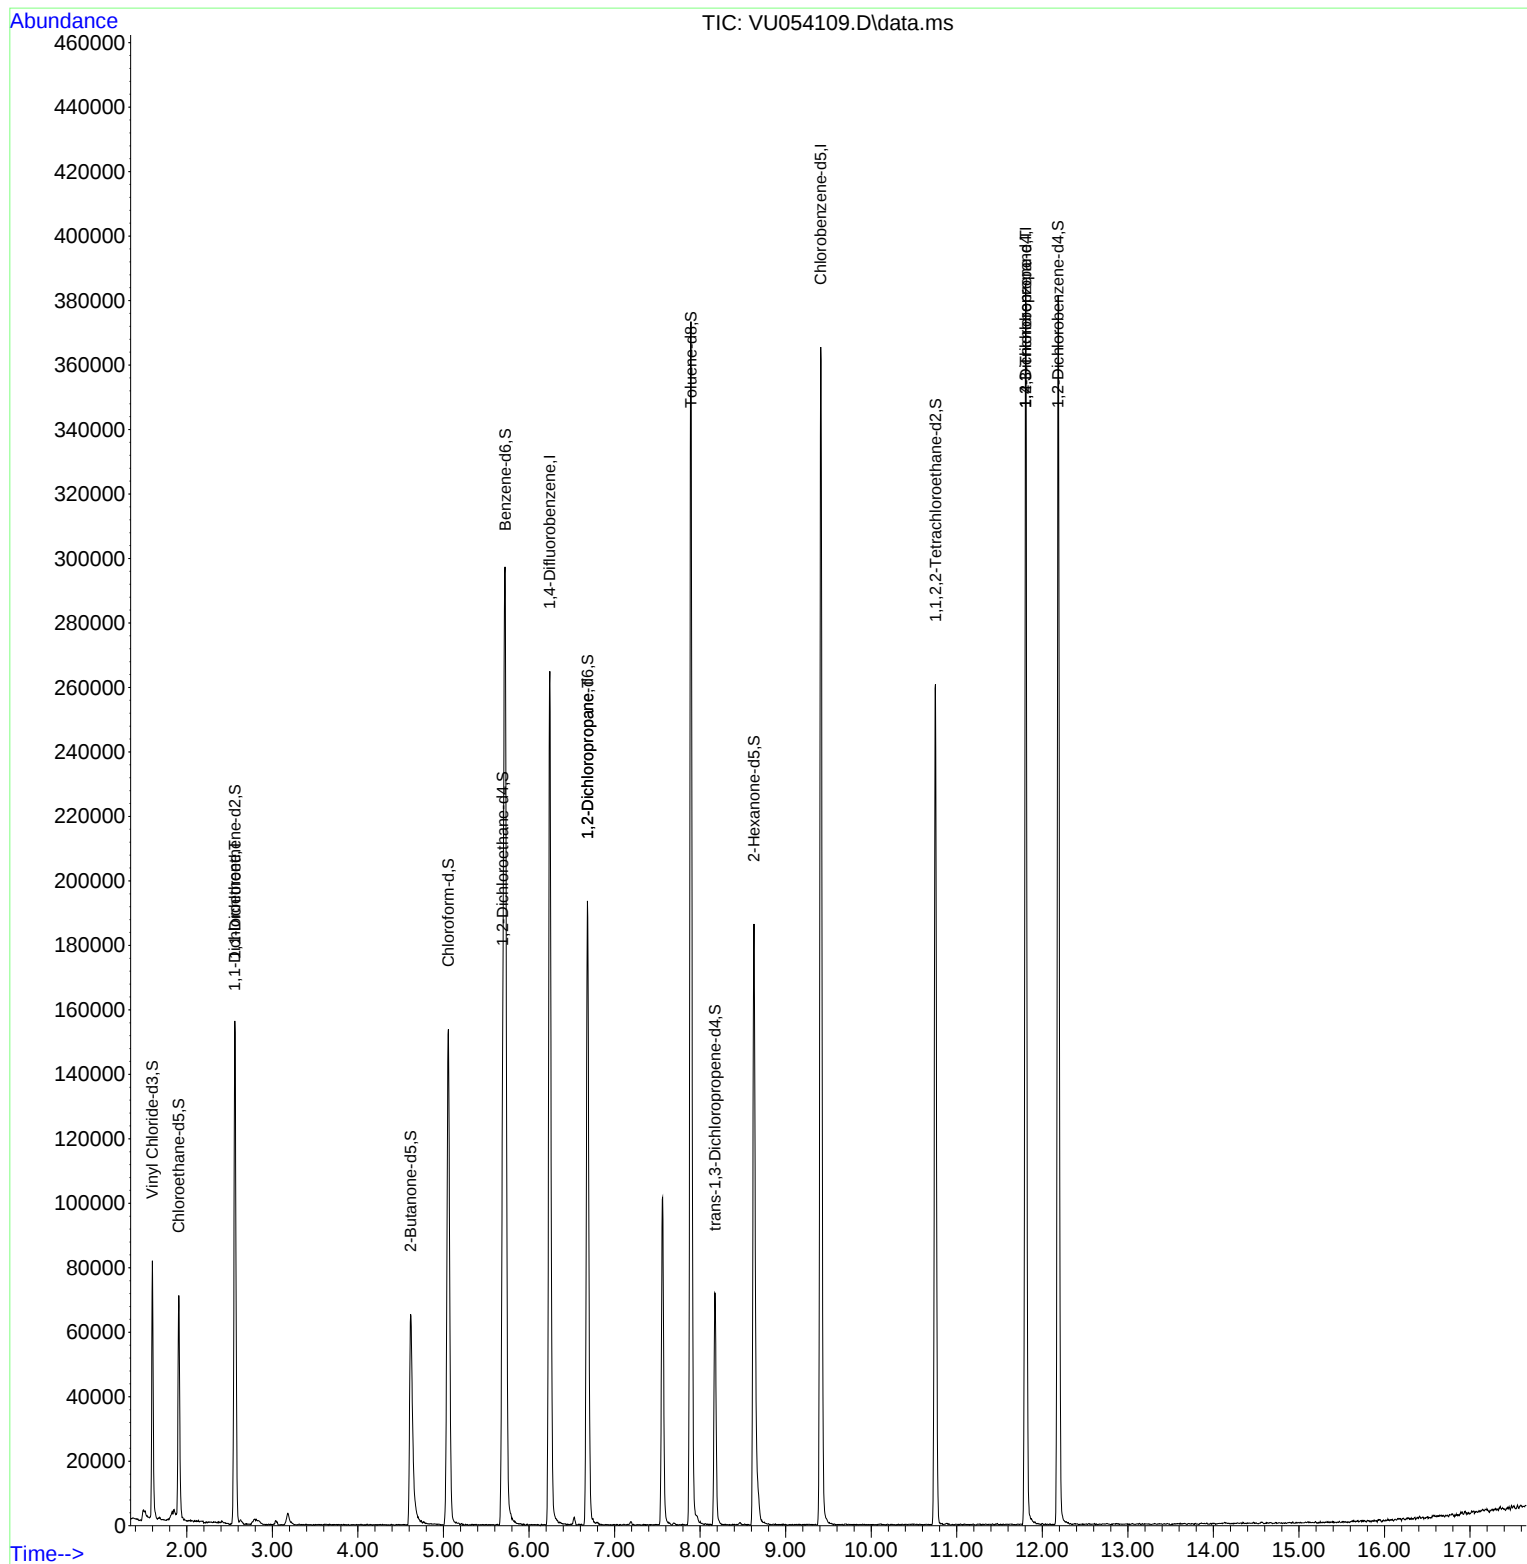

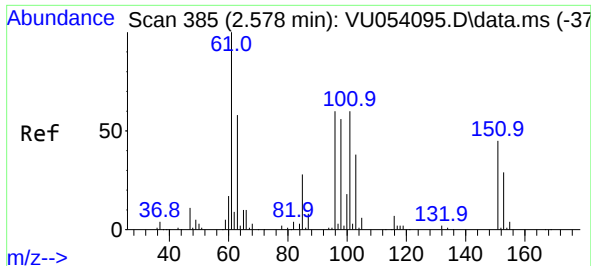

#12

1,1-Dichloroethene

Concen: 0.665 ug/L

RT: 2.559 min Scan# 31

Delta R.T. -0.019 min

Lab File: VU054109.D

Acq: 09 May 2023 03:00

Instrument :

MSVOA_U

ClientSampleId :


Tgt Ion: 96 Resp: 848

Ion Ratio Lower Upper




96 100

61 1337.0 118.3 219.7#

63 10989.9 92.3 171.5#

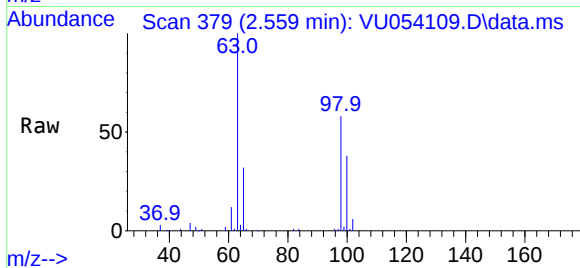

Abundance

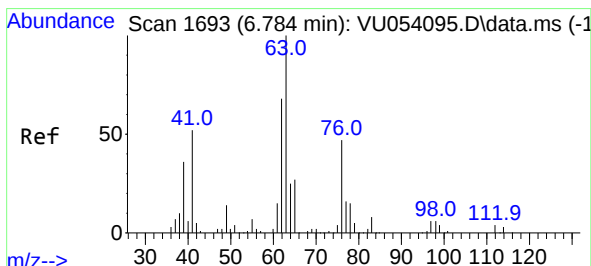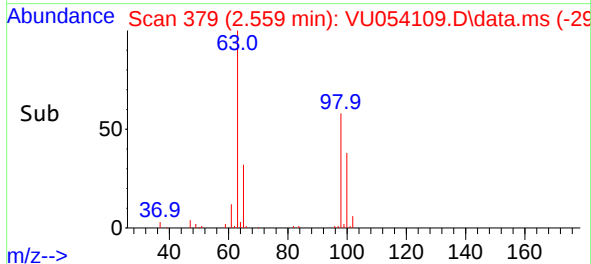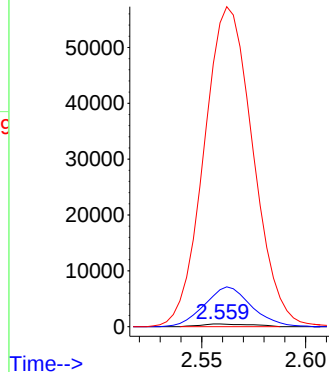

#37

1,2-Dichloropropane

Concen: 5.836 ug/L

RT: 6.684 min Scan# 1662

Delta R.T. -0.103 min

Lab File: VU054109.D


Acq: 09 May 2023 03:00

Tgt Ion: 63 Resp: 10129



Ion Ratio Lower Upper


63 100

112 0.0 3.4 5.0#

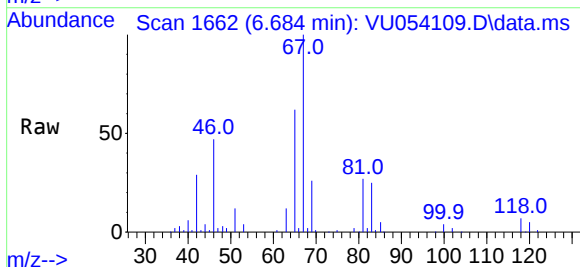


Abundance

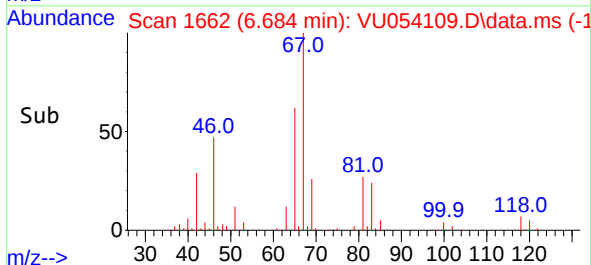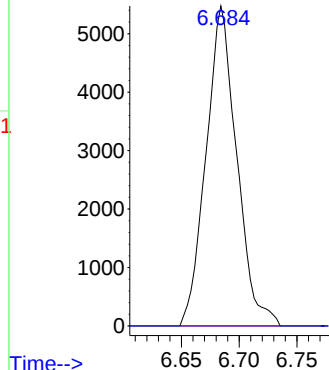

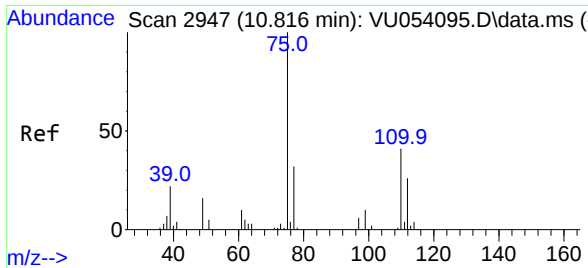

#60
1,2,3-Trichloropropane
Concen: 5.636 ug/L
RT: 11.806 min Scan# 31
Delta R.T. 0.990 min
Lab File: VU054109.D
Acq: 09 May 2023 03:00

Instrument :
MSVOA_U
ClientSampleId :

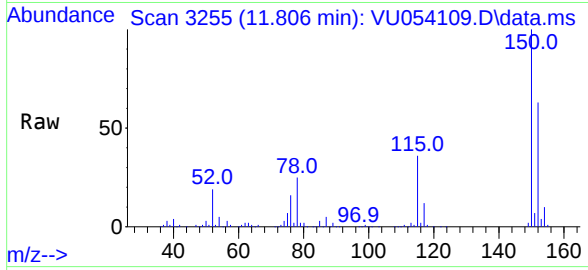

Tgt Ion: 75 Resp: 11146
Ion Ratio Lower Upper
75 100
77 34.5 26.0 39.0
110 1.7 31.8 47.8#

