

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050823\
 Data File : VU054084.D
 Acq On : 08 May 2023 16:43
 Operator : JC/MD
 Sample : 02662-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AZ6

Quant Time: May 09 04:39:48 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat May 06 01:14:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.243	114	164040	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.414	117	158340	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	78586	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	46565	37.533	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	75.060%
7) Chloroethane-d5	1.906	69	40283	49.464	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	98.920%
11) 1,1-Dichloroethene-d2	2.562	63	68889	31.306	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	62.620%
21) 2-Butanone-d5	4.620	46	71883	101.589	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	101.590%
24) Chloroform-d	5.057	84	101883	44.713	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.420%
26) 1,2-Dichloroethane-d4	5.697	65	67697	46.273	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.540%
32) Benzene-d6	5.723	84	197569	42.390	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	84.780%
36) 1,2-Dichloropropane-d6	6.684	67	65429	44.469	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	88.940%
41) Toluene-d8	7.893	98	172431	40.978	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	81.960%
43) trans-1,3-Dichloroprop...	8.176	79	31070	42.670	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	85.340%
47) 2-Hexanone-d5	8.626	63	45530	86.395	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	86.390%
56) 1,1,2,2-Tetrachloroeth...	10.751	84	90430	46.660	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	93.320%
66) 1,2-Dichlorobenzene-d4	12.189	152	72708	47.360	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	94.720%
Target Compounds						
13) Acetone	2.626	43	2708	3.899	ug/L	Qvalue 69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050823\
Data File : VU054084.D
Acq On : 08 May 2023 16:43
Operator : JC/MD
Sample : 02662-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AZ6

Quant Time: May 09 04:39:48 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis
QLast Update : Sat May 06 01:14:00 2023
Response via : Initial Calibration

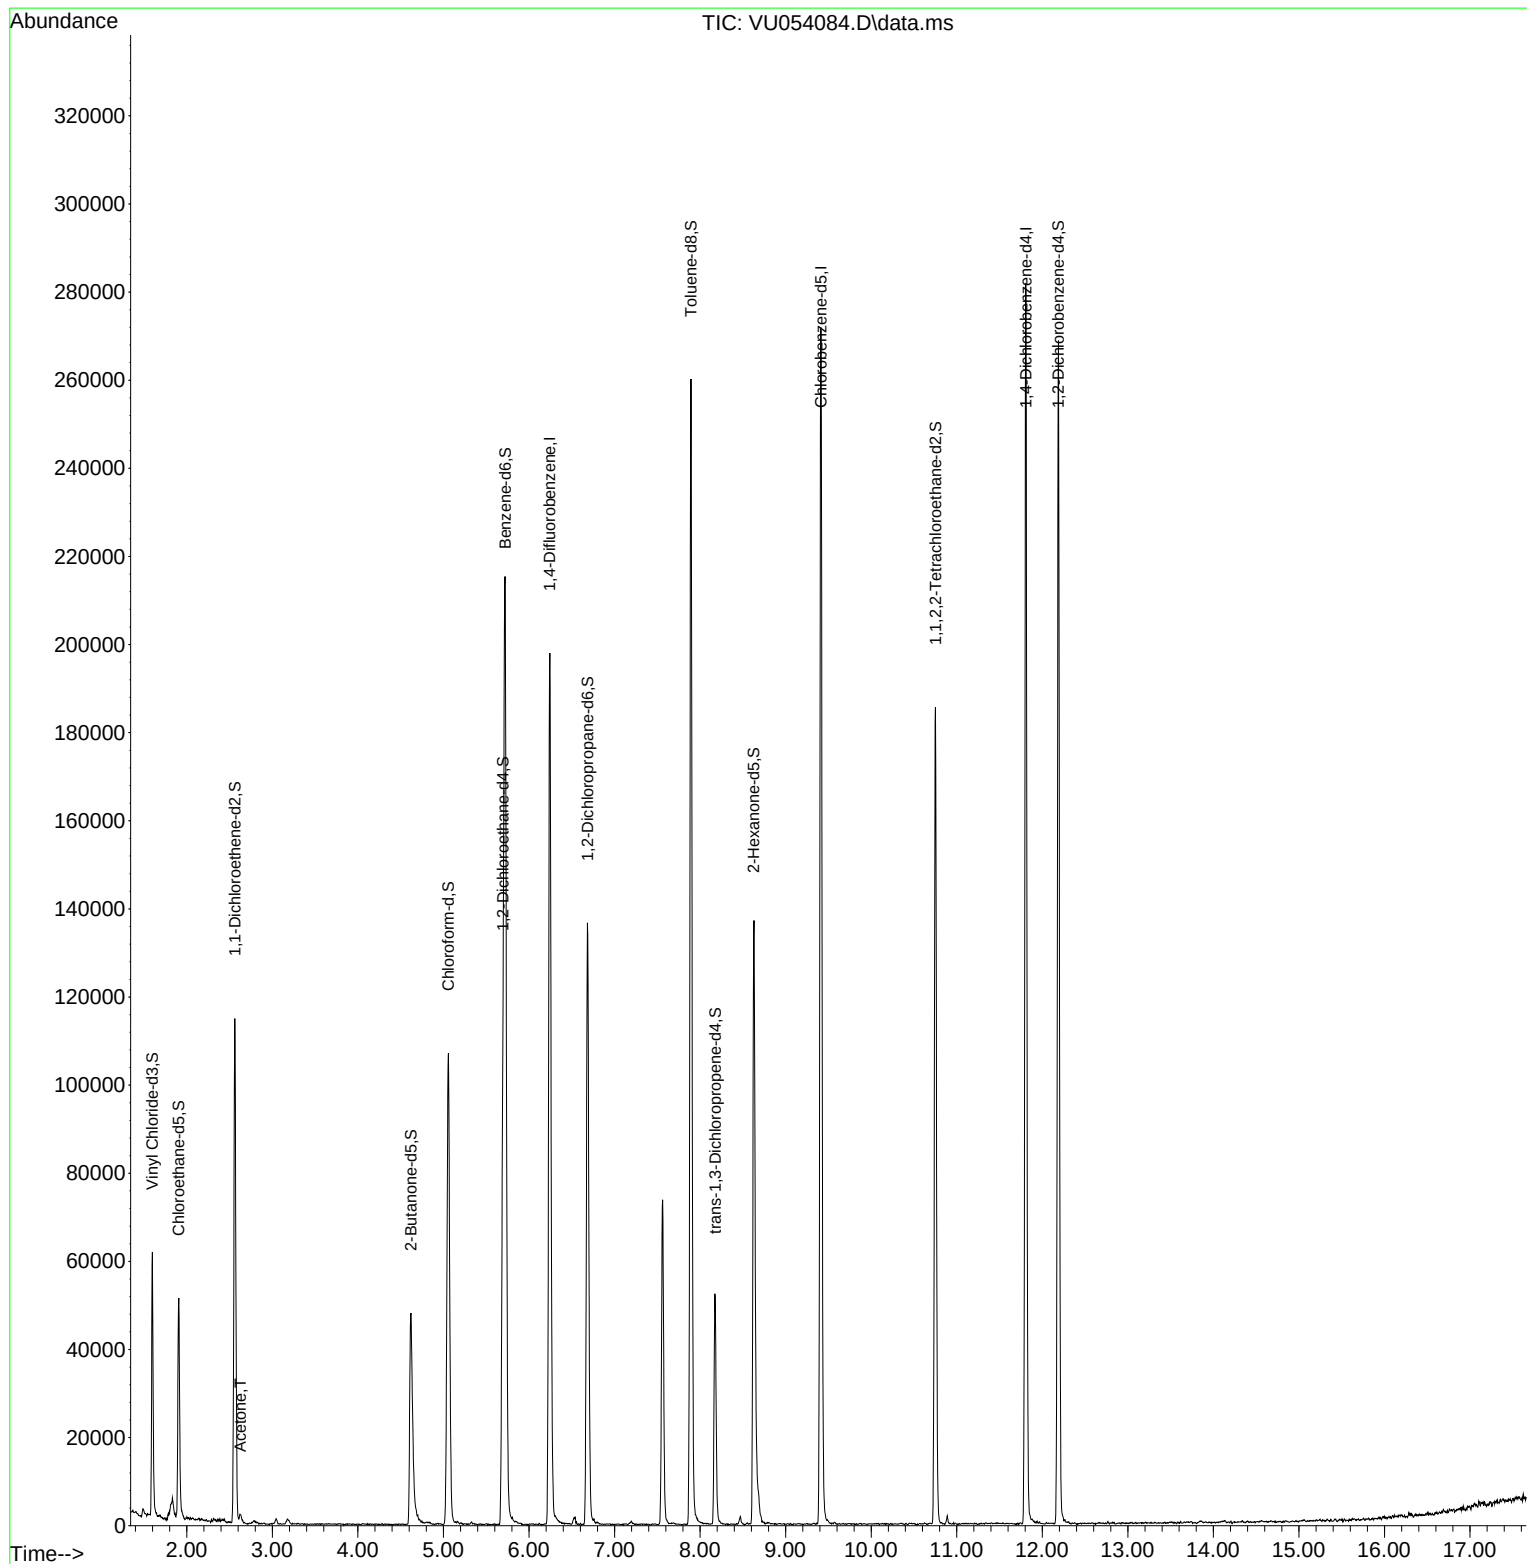

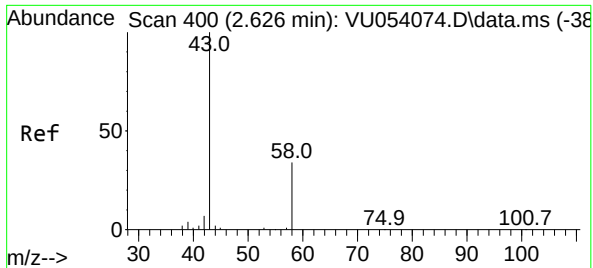

#13
 Acetone
 Concen: 3.899 ug/L
 RT: 2.626 min Scan# 40
 Delta R.T. -0.006 min
 Lab File: VU054084.D
 Acq: 08 May 2023 16:43

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AZ6

Tgt Ion: 43 Resp: 2708
 Ion Ratio Lower Upper
 43 100
 58 16.2 0.0 67.4

