

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050823\
 Data File : VU054089.D
 Acq On : 08 May 2023 18:41
 Operator : JC/MD
 Sample : 02663-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 JREC2

Quant Time: May 09 04:40:23 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat May 06 01:14:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.243	114	206309	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.414	117	196193	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	99484	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	60570	38.819	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	77.640%
7) Chloroethane-d5	1.903	69	53378	52.115	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	104.240%
11) 1,1-Dichloroethene-d2	2.562	63	89859	32.470	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	64.940%
21) 2-Butanone-d5	4.613	46	97505	109.566	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	109.570%
24) Chloroform-d	5.057	84	137385	47.941	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.880%
26) 1,2-Dichloroethane-d4	5.693	65	93331	50.724	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	101.440%
32) Benzene-d6	5.719	84	267210	46.270	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.540%
36) 1,2-Dichloropropane-d6	6.684	67	84997	46.622	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	93.240%
41) Toluene-d8	7.893	98	235363	45.142	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	90.280%
43) trans-1,3-Dichloroprop...	8.172	79	41858	46.395	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	92.780%
47) 2-Hexanone-d5	8.626	63	65407	100.166	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	100.170%
56) 1,1,2,2-Tetrachloroeth...	10.751	84	125673	52.333	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	104.660%
66) 1,2-Dichlorobenzene-d4	12.188	152	105153	54.106	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	108.220%
Target Compounds						
					Qvalue	
13) Acetone	2.623	43	3535	4.047	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050823\
Data File : VU054089.D
Acq On : 08 May 2023 18:41
Operator : JC/MD
Sample : 02663-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
JREC2

Quant Time: May 09 04:40:23 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis
QLast Update : Sat May 06 01:14:00 2023
Response via : Initial Calibration

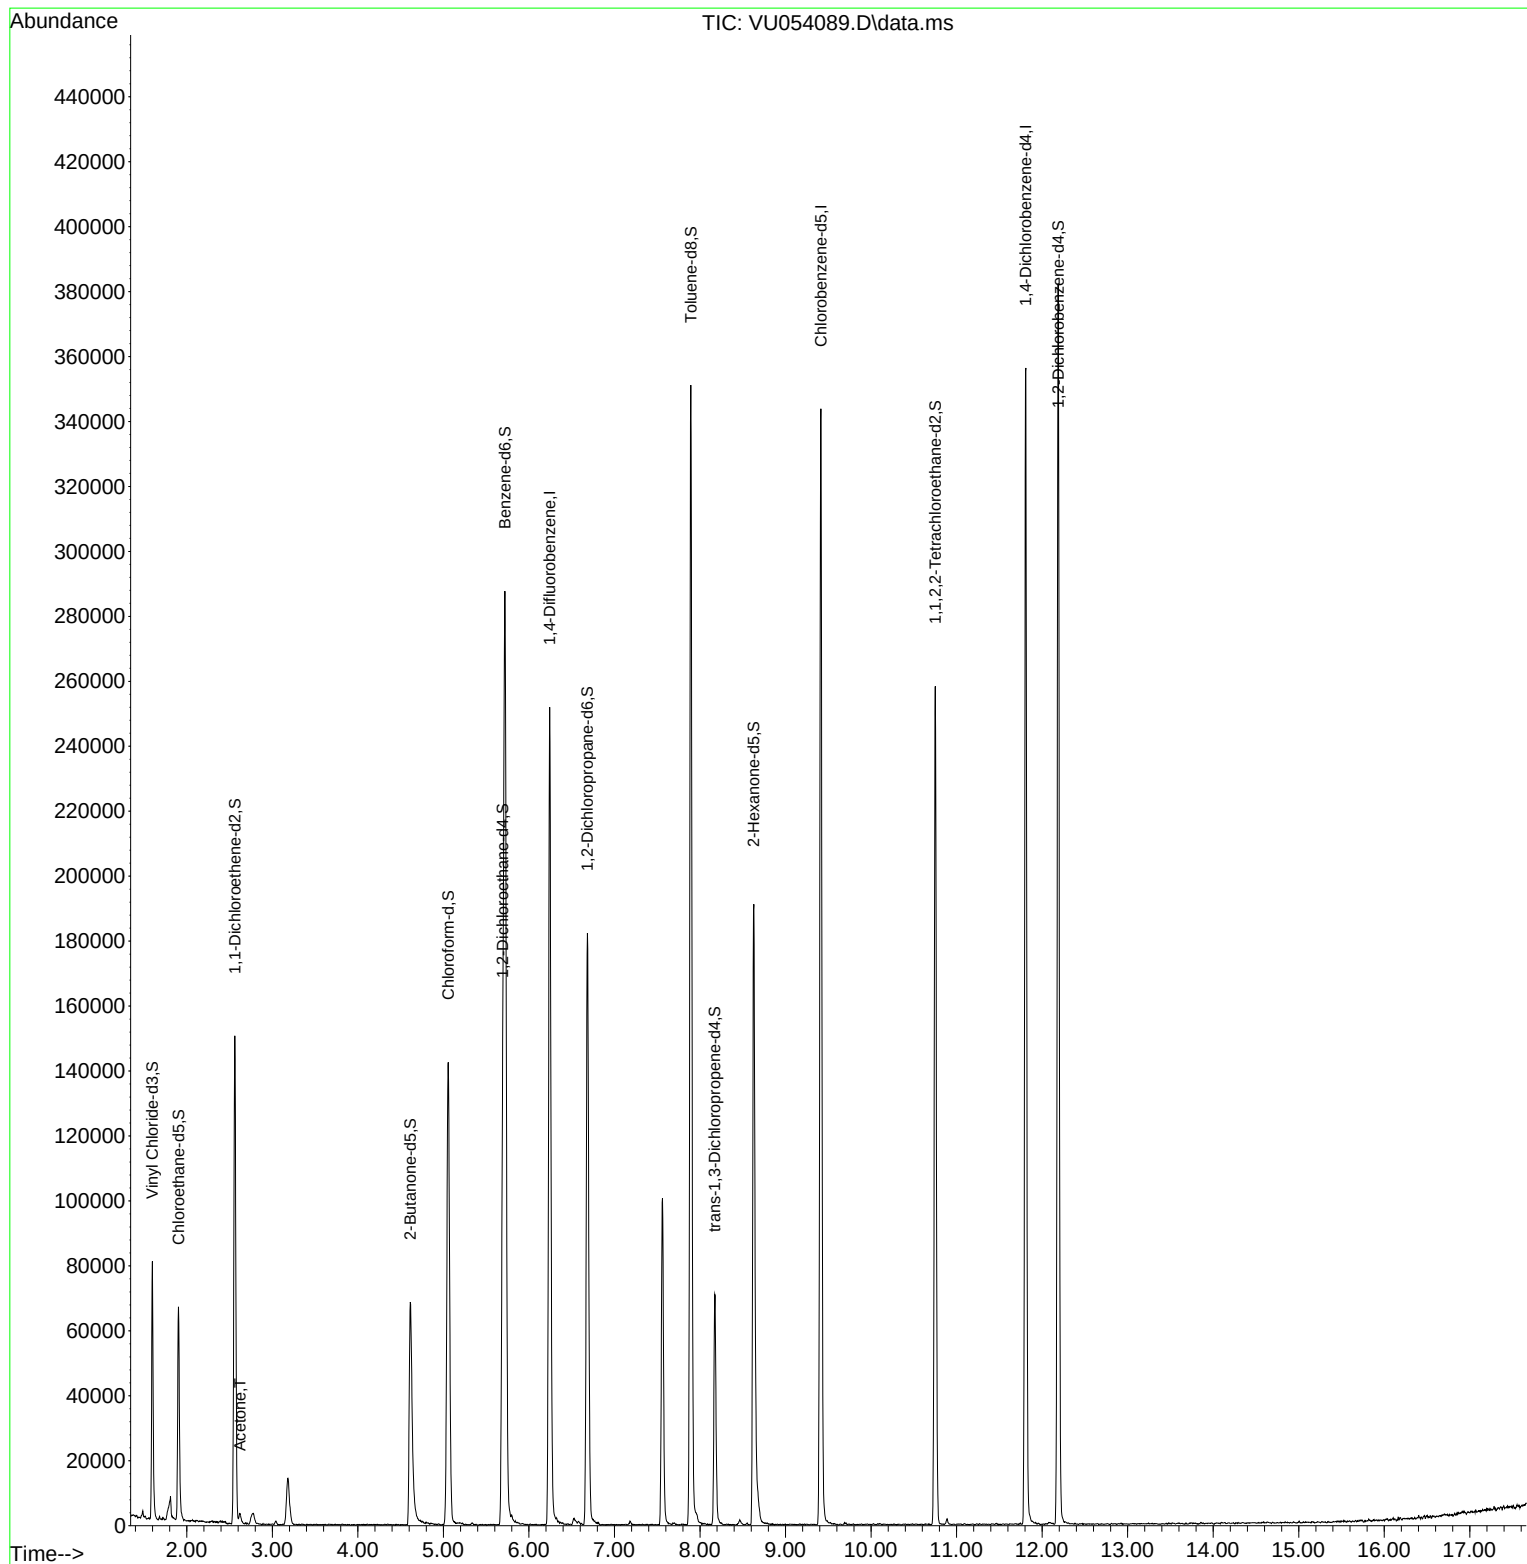

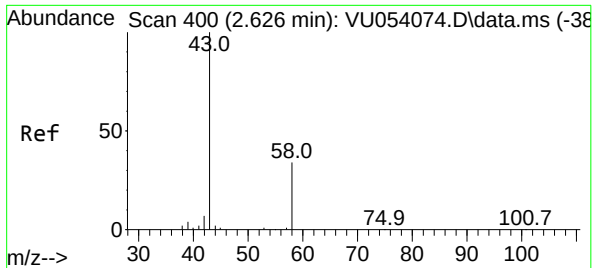

#13
 Acetone
 Concen: 4.047 ug/L
 RT: 2.623 min Scan# 399
 Delta R.T. -0.010 min
 Lab File: VU054089.D
 Acq: 08 May 2023 18:41

Instrument :
 MSVOA_U
 ClientSampleId :
 JREC2

Tgt Ion: 43 Resp: 3535
 Ion Ratio Lower Upper
 43 100
 58 33.7 0.0 67.4

