

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050823\
 Data File : VU054076.D
 Acq On : 08 May 2023 13:28
 Operator : JC/MD
 Sample : VU0508WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK092

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

Signal : TIC: VU054076.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	93	rBV	98728	118929	12.63%	1.712%
2	1.906	167	176	196	rVB	80704	114845	12.20%	1.653%
3	2.221	271	274	279	rBV3	348	346	0.04%	0.005%
4	2.359	313	317	320	rBV3	666	675	0.07%	0.010%
5	2.562	368	380	399	rBV	184406	302167	32.09%	4.349%
6	2.726	428	431	433	rBV2	396	270	0.03%	0.004%
7	2.787	445	450	458	rBV	627	843	0.09%	0.012%
8	2.855	469	471	475	rBV2	200	202	0.02%	0.003%
9	3.041	520	529	541	rVB3	3866	7508	0.80%	0.108%
10	3.166	565	568	570	rBV	887	645	0.07%	0.009%
11	3.411	638	644	654	rBV2	320	516	0.05%	0.007%
12	3.453	654	657	661	rBV	225	158	0.02%	0.002%
13	3.707	731	736	739	rBV	171	215	0.02%	0.003%
14	3.748	744	749	752	rBV	287	303	0.03%	0.004%
15	3.916	798	801	803	rBV2	269	188	0.02%	0.003%
16	4.083	847	853	859	rBV2	298	474	0.05%	0.007%
17	4.154	871	875	880	rBV	262	294	0.03%	0.004%
18	4.192	883	887	890	rBV2	206	230	0.02%	0.003%
19	4.285	911	916	918	rBV	159	169	0.02%	0.002%
20	4.346	931	935	937	rBV2	236	203	0.02%	0.003%
21	4.459	965	970	975	rBV2	241	312	0.03%	0.004%
22	4.485	975	978	982	rVB	181	166	0.02%	0.002%
23	4.572	998	1005	1007	rBV2	284	362	0.04%	0.005%
24	4.620	1008	1020	1052	rBV	73380	188789	20.05%	2.717%
25	4.887	1098	1103	1107	rBV3	320	381	0.04%	0.005%
26	5.057	1140	1156	1182	rVV	172416	381352	40.51%	5.488%
27	5.256	1215	1218	1220	rVV	232	146	0.02%	0.002%
28	5.282	1224	1226	1231	rVB	254	219	0.02%	0.003%
29	5.517	1296	1299	1303	rBV2	164	157	0.02%	0.002%
30	5.719	1340	1362	1385	rBV2	339029	941486	100.00%	13.550%
31	5.935	1425	1429	1434	rVB3	318	303	0.03%	0.004%
32	6.009	1449	1452	1454	rBV	262	214	0.02%	0.003%
33	6.243	1511	1525	1543	rBV	269573	510627	54.24%	7.349%
34	6.462	1589	1593	1595	rVB2	263	216	0.02%	0.003%
35	6.485	1595	1600	1603	rBV2	202	174	0.02%	0.003%
36	6.526	1605	1613	1614	rBV3	2928	3204	0.34%	0.046%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050823\
 Data File : VU054076.D
 Acq On : 08 May 2023 13:28
 Operator : JC/MD
 Sample : VU0508WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK092

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

37	6.684	1647	1662	1686	rBV	217639	429521	45.62%	6.182%
38	7.102	1790	1792	1796	rBV	161	147	0.02%	0.002%
39	7.195	1812	1821	1823	rBV5	925	1302	0.14%	0.019%
40	7.346	1863	1868	1871	rBV	246	238	0.03%	0.003%
41	7.427	1888	1893	1895	rBV	135	160	0.02%	0.002%
42	7.562	1922	1935	1954	rBV	124550	219466	23.31%	3.159%
43	7.677	1968	1971	1974	rBV2	260	216	0.02%	0.003%
44	7.697	1974	1977	1988	rVB4	855	910	0.10%	0.013%
45	7.790	2002	2006	2008	rBV2	382	323	0.03%	0.005%
46	7.893	2023	2038	2068	rBV	435264	754208	80.11%	10.854%
47	8.176	2112	2126	2154	rVB	87562	149135	15.84%	2.146%
48	8.301	2161	2165	2169	rBV3	243	195	0.02%	0.003%
49	8.340	2174	2177	2181	rBV	137	144	0.02%	0.002%
50	8.382	2187	2190	2193	rVB	275	186	0.02%	0.003%
51	8.401	2193	2196	2199	rBV	296	232	0.02%	0.003%
52	8.475	2217	2219	2224	rBV	202	153	0.02%	0.002%
53	8.584	2248	2253	2256	rBV	225	268	0.03%	0.004%
54	8.629	2256	2267	2301	rVV2	219006	415391	44.12%	5.978%
55	8.780	2311	2314	2318	rVB2	487	356	0.04%	0.005%
56	8.800	2318	2320	2326	rVB2	275	204	0.02%	0.003%
57	8.845	2330	2334	2339	rVB2	301	267	0.03%	0.004%
58	8.874	2339	2343	2348	rVB	350	285	0.03%	0.004%
59	8.973	2371	2374	2377	rVB2	291	166	0.02%	0.002%
60	9.038	2388	2394	2397	rBV2	299	339	0.04%	0.005%
61	9.112	2413	2417	2420	rBV2	212	191	0.02%	0.003%
62	9.414	2498	2511	2537	rBV	363608	609479	64.74%	8.771%
63	9.571	2558	2560	2567	rVB2	489	448	0.05%	0.006%
64	9.690	2589	2597	2598	rBV2	740	581	0.06%	0.008%
65	9.784	2621	2626	2633	rBV	199	327	0.03%	0.005%
66	10.102	2721	2725	2726	rBV	282	155	0.02%	0.002%
67	10.224	2760	2763	2766	rBV2	180	177	0.02%	0.003%
68	10.349	2797	2802	2805	rBV2	193	221	0.02%	0.003%
69	10.446	2824	2832	2836	rBV	259	400	0.04%	0.006%
70	10.468	2837	2839	2840	rBV	427	162	0.02%	0.002%
71	10.642	2889	2893	2898	rBV4	727	670	0.07%	0.010%
72	10.751	2914	2927	2945	rBV	297167	476173	50.58%	6.853%
73	10.906	2972	2975	2980	rVV	241	195	0.02%	0.003%
74	11.224	3069	3074	3075	rBV	250	194	0.02%	0.003%
75	11.324	3101	3105	3107	rBV2	206	195	0.02%	0.003%
76	11.417	3129	3134	3137	rBV2	268	278	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050823\
 Data File : VU054076.D
 Acq On : 08 May 2023 13:28
 Operator : JC/MD
 Sample : VU0508WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK092

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

77	11.472	3146	3151	3161	rVB3	729	983	0.10%	0.014%
78	11.568	3178	3181	3183	rBV	287	214	0.02%	0.003%
79	11.603	3189	3192	3195	rBV	351	309	0.03%	0.004%
80	11.693	3217	3220	3223	rBV2	245	195	0.02%	0.003%
81	11.716	3223	3227	3229	rBV	225	193	0.02%	0.003%
82	11.748	3229	3237	3243	rBV4	990	1492	0.16%	0.021%
83	11.809	3243	3256	3273	rBV	364385	593123	63.00%	8.536%
84	12.060	3330	3334	3341	rBV2	264	401	0.04%	0.006%
85	12.099	3343	3346	3348	rBV	254	174	0.02%	0.003%
86	12.189	3361	3374	3399	rBV	422550	692090	73.51%	9.960%
87	12.291	3404	3406	3410	rVB2	735	499	0.05%	0.007%
88	12.410	3441	3443	3448	rBV2	261	151	0.02%	0.002%
89	12.703	3531	3534	3540	rVB2	202	200	0.02%	0.003%
90	12.732	3540	3543	3552	rBV2	271	308	0.03%	0.004%
91	13.144	3667	3671	3676	rBV2	245	281	0.03%	0.004%
92	13.182	3680	3683	3686	rVB	337	221	0.02%	0.003%
93	13.224	3690	3696	3708	rVB2	981	1644	0.17%	0.024%
94	13.844	3880	3889	3898	rBV4	2283	3943	0.42%	0.057%
95	13.938	3912	3918	3923	rBV2	436	668	0.07%	0.010%
96	14.095	3959	3967	3980	rBV2	3423	5410	0.57%	0.078%
97	14.336	4032	4042	4049	rBV3	2775	4026	0.43%	0.058%
98	14.420	4065	4068	4071	rBV	333	216	0.02%	0.003%
99	14.947	4229	4232	4236	rBV3	391	365	0.04%	0.005%
100	15.812	4499	4501	4503	rBV3	596	362	0.04%	0.005%




Sum of corrected areas: 6948414

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050823\
Data File : VU054076.D
Acq On : 08 May 2023 13:28
Operator : JC/MD
Sample : VU0508WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK092

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

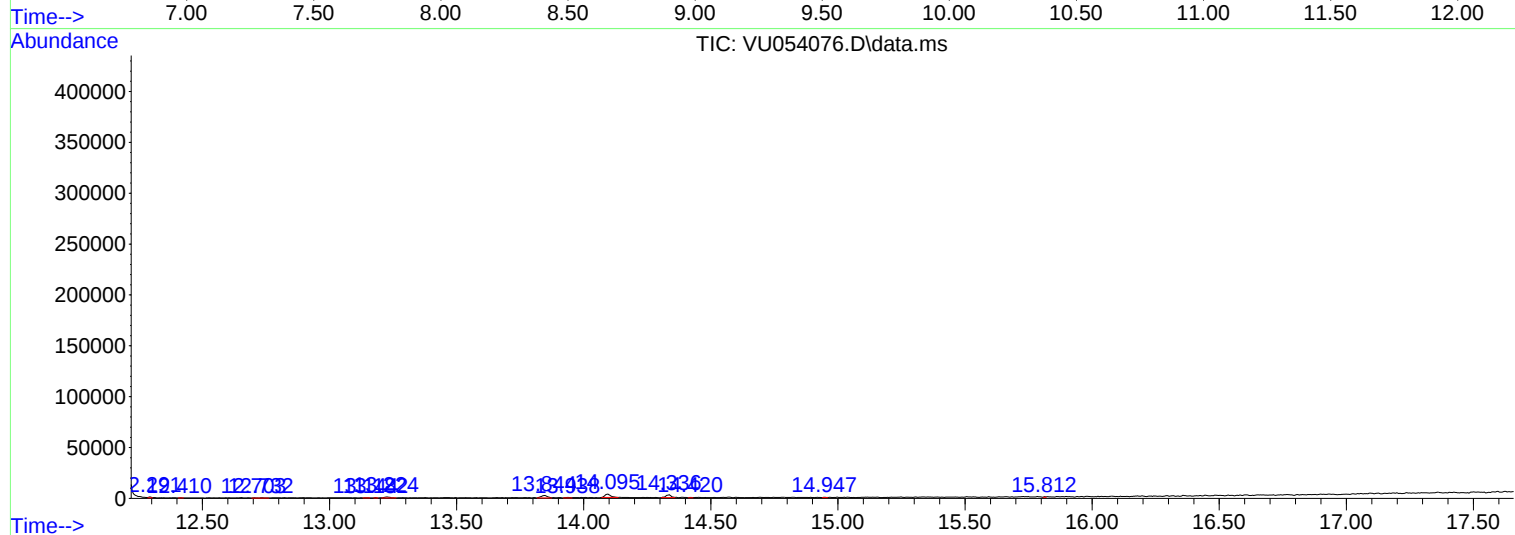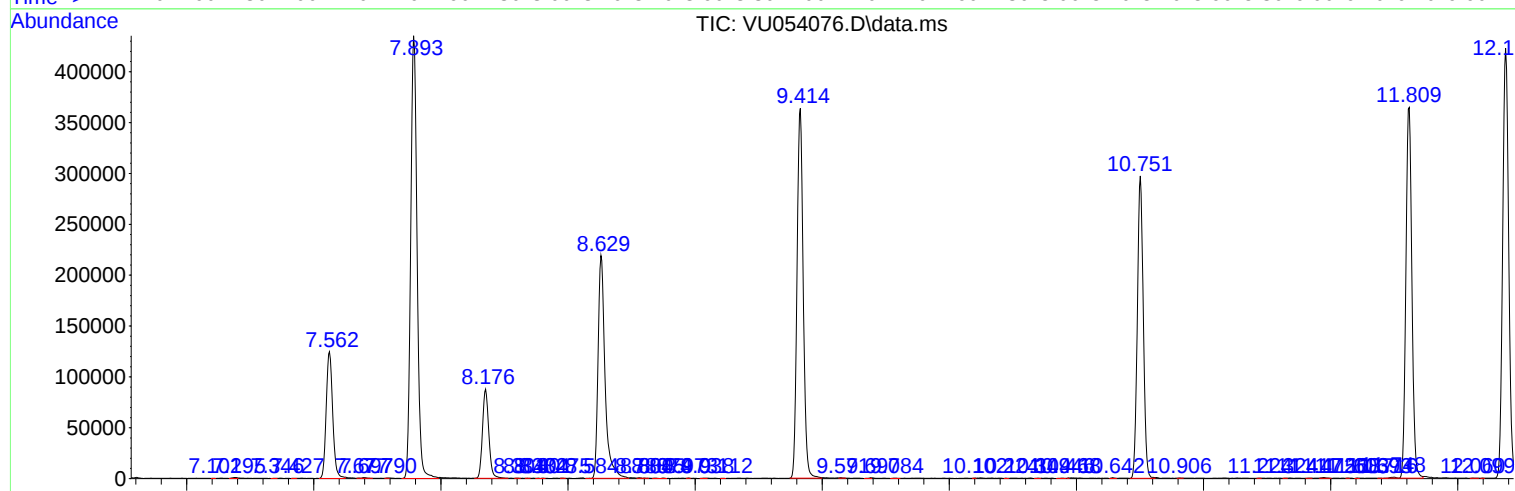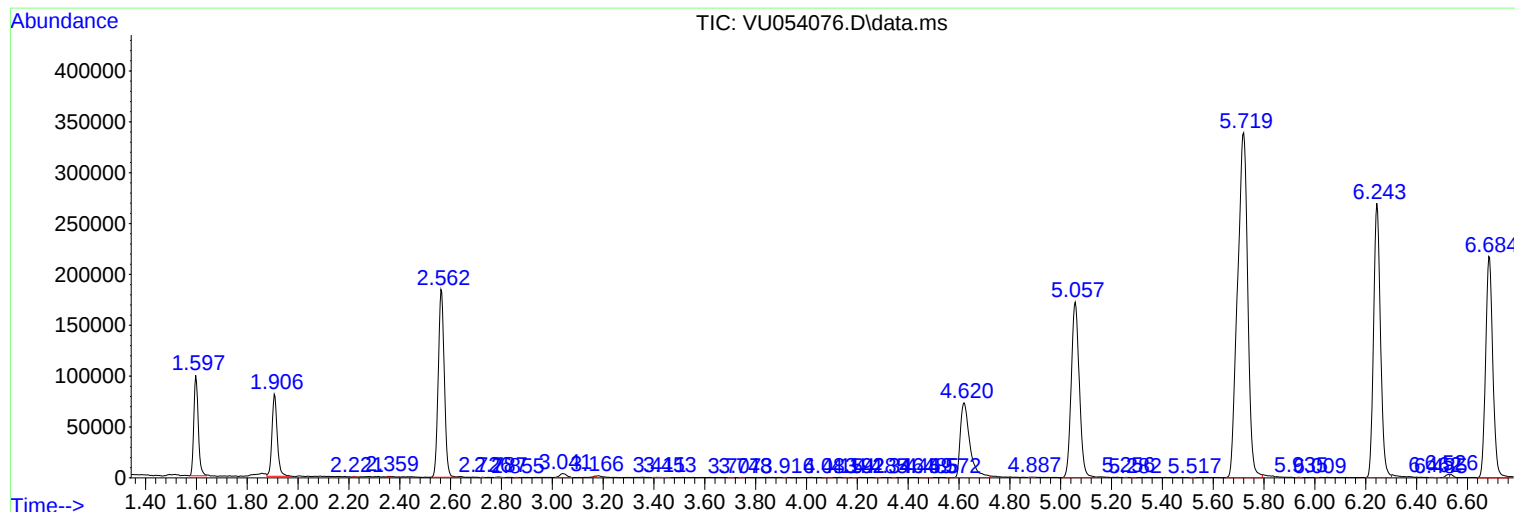

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050823\
Data File : VU054076.D
Acq On : 08 May 2023 13:28
Operator : JC/MD
Sample : VU0508WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK092

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050823\
Data File : VU054076.D
Acq On : 08 May 2023 13:28
Operator : JC/MD
Sample : VU0508WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK092

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc