

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050823\
 Data File : VU054082.D
 Acq On : 08 May 2023 15:56
 Operator : JC/MD
 Sample : 02662-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AZ4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

Signal : TIC: VU054082.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	100	rVB	87828	106274	12.62%	1.645%
2	1.906	167	176	195	rVB	71521	101080	12.00%	1.565%
3	2.006	205	207	213	rBV3	493	429	0.05%	0.007%
4	2.289	293	295	298	rBV2	282	193	0.02%	0.003%
5	2.372	319	321	323	rBV	496	212	0.03%	0.003%
6	2.562	368	380	395	rBV	165276	265481	31.52%	4.110%
7	2.723	427	430	434	rBV	380	301	0.04%	0.005%
8	2.787	443	450	456	rBV4	591	923	0.11%	0.014%
9	2.890	478	482	485	rBV2	230	216	0.03%	0.003%
10	2.954	499	502	508	rVB2	196	205	0.02%	0.003%
11	3.044	527	530	537	rVB3	831	967	0.11%	0.015%
12	3.176	563	571	585	rVB4	1293	3040	0.36%	0.047%
13	3.607	700	705	708	rVV2	166	199	0.02%	0.003%
14	3.970	814	818	822	rBV	204	245	0.03%	0.004%
15	4.112	858	862	867	rBV2	192	228	0.03%	0.004%
16	4.182	879	884	887	rBV2	297	321	0.04%	0.005%
17	4.237	898	901	907	rBV2	158	183	0.02%	0.003%
18	4.510	981	986	989	rBV	198	197	0.02%	0.003%
19	4.620	1008	1020	1053	rBV	71790	182245	21.64%	2.821%
20	4.941	1114	1120	1122	rBV	354	314	0.04%	0.005%
21	4.983	1130	1133	1139	rVB2	408	438	0.05%	0.007%
22	5.057	1139	1156	1175	rBV	155122	344302	40.88%	5.330%
23	5.311	1224	1235	1246	rBV5	2814	5830	0.69%	0.090%
24	5.382	1253	1257	1259	rBV	203	180	0.02%	0.003%
25	5.420	1266	1269	1272	rBV	264	210	0.02%	0.003%
26	5.456	1276	1280	1282	rBV2	184	194	0.02%	0.003%
27	5.481	1285	1288	1293	rVV2	240	242	0.03%	0.004%
28	5.514	1296	1298	1303	rVB2	235	207	0.02%	0.003%
29	5.597	1321	1324	1333	rBV2	236	402	0.05%	0.006%
30	5.719	1341	1362	1387	rBV2	305971	842299	100.00%	13.038%
31	5.964	1433	1438	1442	rBV2	269	293	0.03%	0.005%
32	6.124	1486	1488	1493	rVB2	320	243	0.03%	0.004%
33	6.243	1512	1525	1546	rBV	267025	503293	59.75%	7.791%
34	6.536	1604	1616	1629	rVB8	12181	23376	2.78%	0.362%
35	6.684	1648	1662	1681	rBV	197252	383537	45.53%	5.937%
36	6.793	1693	1696	1699	rBV3	451	295	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050823\
 Data File : VU054082.D
 Acq On : 08 May 2023 15:56
 Operator : JC/MD
 Sample : 02662-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AZ4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

37	6.944	1736	1743	1747	rBV	239	263	0.03%	0.004%
38	6.976	1747	1753	1756	rBV2	215	284	0.03%	0.004%
39	7.192	1812	1820	1825	rVV2	1126	1717	0.20%	0.027%
40	7.253	1833	1839	1844	rVB2	255	270	0.03%	0.004%
41	7.292	1844	1851	1856	rBV2	271	395	0.05%	0.006%
42	7.562	1922	1935	1963	rBV	109667	194571	23.10%	3.012%
43	7.690	1970	1975	1977	rBV2	440	395	0.05%	0.006%
44	7.893	2024	2038	2074	rBV	378258	666828	79.17%	10.322%
45	8.025	2077	2079	2084	rVB2	360	197	0.02%	0.003%
46	8.073	2091	2094	2097	rVB2	269	181	0.02%	0.003%
47	8.134	2108	2113	2115	rBV2	237	248	0.03%	0.004%
48	8.176	2115	2126	2147	rVV	77762	133144	15.81%	2.061%
49	8.414	2196	2200	2205	rBV3	336	376	0.04%	0.006%
50	8.465	2208	2216	2229	rBV3	2238	4069	0.48%	0.063%
51	8.539	2232	2239	2240	rBV2	328	296	0.04%	0.005%
52	8.629	2256	2267	2297	rBV2	212676	397710	47.22%	6.156%
53	8.732	2297	2299	2305	rVB4	885	588	0.07%	0.009%
54	9.131	2420	2423	2427	rBV2	285	288	0.03%	0.004%
55	9.166	2431	2434	2438	rVV	226	238	0.03%	0.004%
56	9.414	2498	2511	2541	rBV	360796	603009	71.59%	9.334%
57	9.571	2557	2560	2562	rBV	257	184	0.02%	0.003%
58	9.626	2574	2577	2584	rVB2	292	304	0.04%	0.005%
59	9.697	2593	2599	2607	rBV	416	596	0.07%	0.009%
60	9.877	2650	2655	2657	rBV2	313	284	0.03%	0.004%
61	10.009	2690	2696	2699	rBV2	194	221	0.03%	0.003%
62	10.095	2719	2723	2728	rBV2	534	560	0.07%	0.009%
63	10.185	2745	2751	2756	rBV	283	333	0.04%	0.005%
64	10.240	2761	2768	2773	rBV	322	343	0.04%	0.005%
65	10.298	2779	2786	2789	rBV2	242	317	0.04%	0.005%
66	10.484	2838	2844	2850	rBV3	312	457	0.05%	0.007%
67	10.558	2857	2867	2869	rBV2	250	382	0.05%	0.006%
68	10.578	2869	2873	2876	rBV2	300	262	0.03%	0.004%
69	10.623	2879	2887	2890	rBV2	287	455	0.05%	0.007%
70	10.684	2901	2906	2909	rBV	264	240	0.03%	0.004%
71	10.751	2914	2927	2943	rBV	273839	440858	52.34%	6.824%
72	10.828	2950	2951	2955	rBV2	263	186	0.02%	0.003%
73	10.880	2963	2967	2970	rBV4	1585	1396	0.17%	0.022%
74	10.986	2996	3000	3004	rBV2	357	370	0.04%	0.006%
75	11.092	3030	3033	3037	rVB2	385	275	0.03%	0.004%
76	11.172	3054	3058	3060	rBV2	223	179	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050823\
 Data File : VU054082.D
 Acq On : 08 May 2023 15:56
 Operator : JC/MD
 Sample : 02662-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AZ4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

77	11.471	3148	3151	3155	rBV3	372	279	0.03%	0.004%
78	11.513	3160	3164	3166	rBV	241	191	0.02%	0.003%
79	11.684	3215	3217	3220	rVB2	427	223	0.03%	0.003%
80	11.706	3220	3224	3225	rBV2	351	250	0.03%	0.004%
81	11.742	3230	3235	3237	rBV3	591	516	0.06%	0.008%
82	11.806	3243	3255	3275	rBV	375709	593058	70.41%	9.180%
83	12.188	3361	3374	3395	rBV	392736	637405	75.67%	9.867%
84	12.307	3409	3411	3415	rVB2	443	260	0.03%	0.004%
85	12.533	3479	3481	3484	rBV	374	218	0.03%	0.003%
86	12.613	3503	3506	3509	rBV	222	180	0.02%	0.003%
87	12.893	3589	3593	3598	rBV2	251	296	0.04%	0.005%
88	13.143	3667	3671	3676	rBV3	450	439	0.05%	0.007%
89	13.188	3682	3685	3691	rVB2	357	324	0.04%	0.005%
90	13.368	3738	3741	3746	rBV2	183	199	0.02%	0.003%
91	13.414	3751	3755	3759	rBV2	251	291	0.03%	0.005%
92	13.545	3792	3796	3802	rBV	294	338	0.04%	0.005%
93	13.651	3827	3829	3833	rVB2	255	185	0.02%	0.003%
94	13.983	3928	3932	3934	rBV3	322	294	0.03%	0.005%
95	14.574	4110	4116	4122	rBV2	818	1171	0.14%	0.018%
96	15.108	4280	4282	4285	rBV2	360	270	0.03%	0.004%
97	15.282	4333	4336	4338	rBV	358	278	0.03%	0.004%
98	15.494	4396	4402	4406	rBV3	761	909	0.11%	0.014%
99	15.902	4526	4529	4531	rBV2	571	416	0.05%	0.006%
100	16.098	4588	4590	4593	rBV	604	284	0.03%	0.004%




Sum of corrected areas: 6460137

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050823\
Data File : VU054082.D
Acq On : 08 May 2023 15:56
Operator : JC/MD
Sample : 02662-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AZ4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

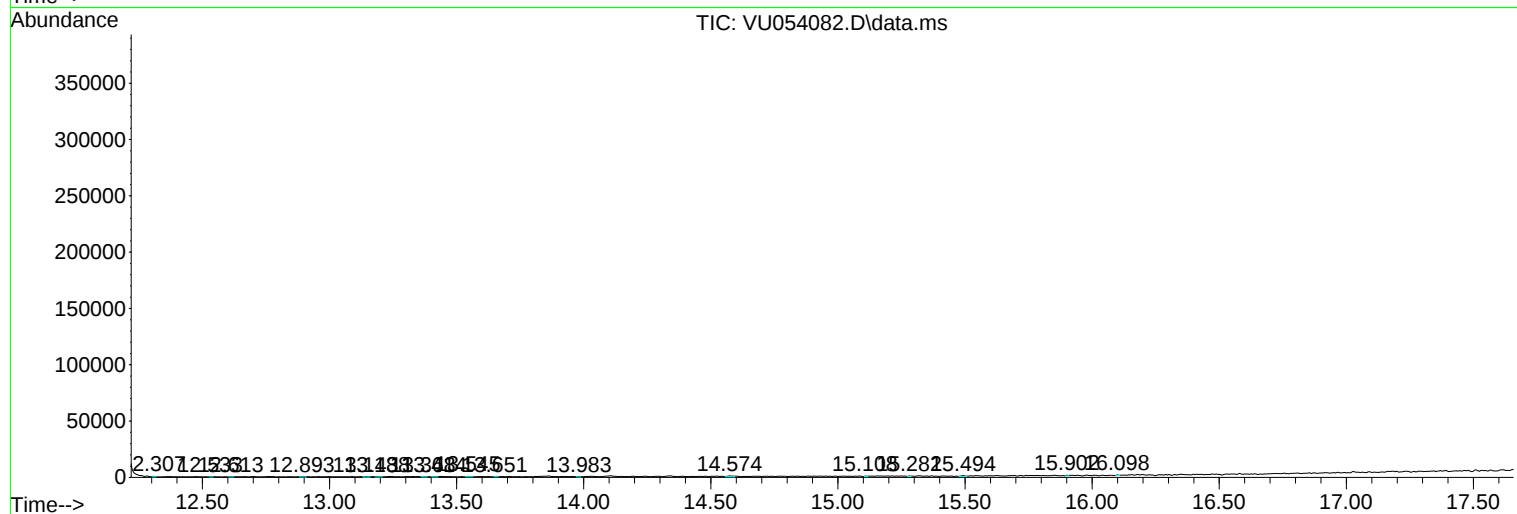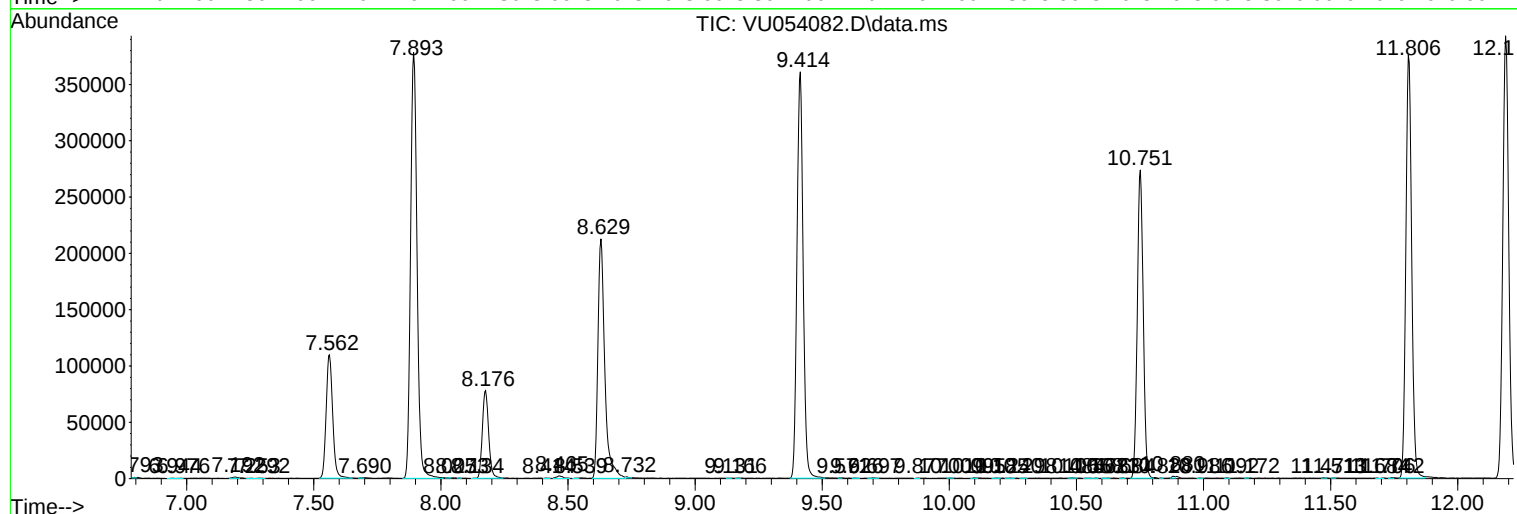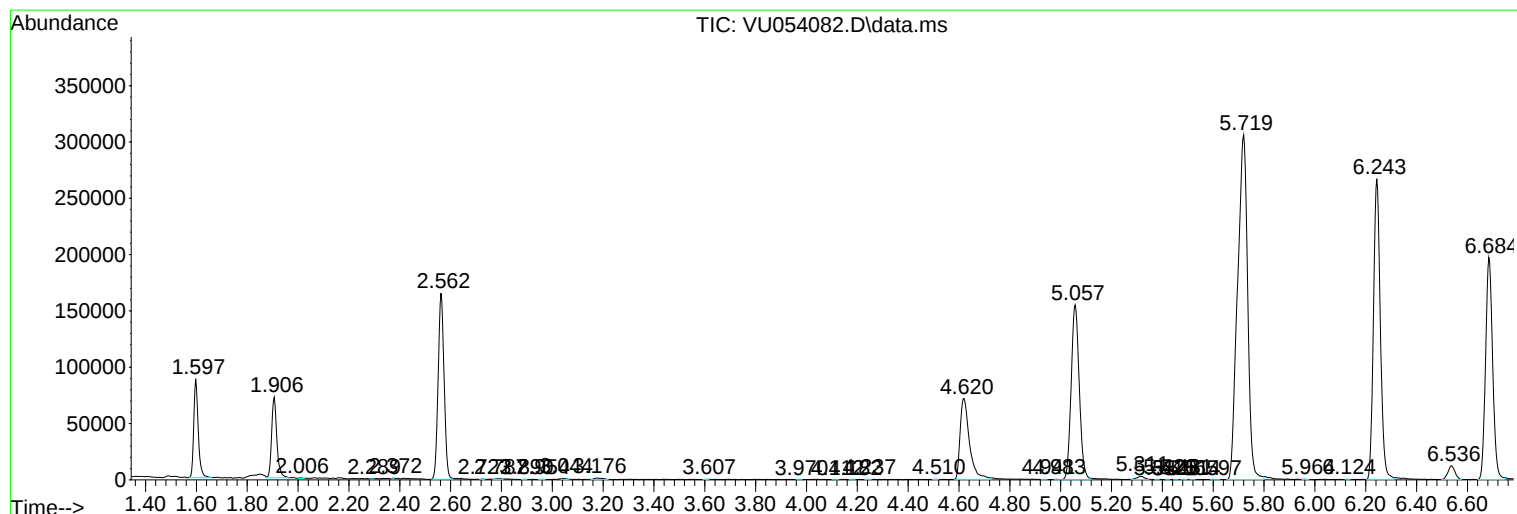

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050823\
Data File : VU054082.D
Acq On : 08 May 2023 15:56
Operator : JC/MD
Sample : 02662-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AZ4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050823\
Data File : VU054082.D
Acq On : 08 May 2023 15:56
Operator : JC/MD
Sample : 02662-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AZ4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------