

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050823\
 Data File : VU054084.D
 Acq On : 08 May 2023 16:43
 Operator : JC/MD
 Sample : 02662-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AZ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

Signal : TIC: VU054084.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	94	rBV	59684	71361	12.30%	1.581%
2	1.781	134	137	139	rBV2	1100	734	0.13%	0.016%
3	1.906	168	176	195	rVB	49994	72055	12.42%	1.597%
4	2.289	292	295	297	rBV2	665	399	0.07%	0.009%
5	2.314	300	303	306	rVV3	637	454	0.08%	0.010%
6	2.359	315	317	320	rBV2	502	290	0.05%	0.006%
7	2.491	354	358	360	rBV	258	205	0.04%	0.005%
8	2.562	368	380	394	rBV	114425	185285	31.95%	4.106%
9	2.623	395	399	407	rVB3	1502	2270	0.39%	0.050%
10	2.736	428	434	436	rBV2	259	266	0.05%	0.006%
11	2.974	505	508	512	rBV2	263	293	0.05%	0.006%
12	3.009	516	519	521	rVV	340	245	0.04%	0.005%
13	3.044	523	530	538	rVV4	1310	2040	0.35%	0.045%
14	3.176	562	571	575	rBV3	1085	1674	0.29%	0.037%
15	3.301	606	610	615	rVB2	247	239	0.04%	0.005%
16	3.523	675	679	683	rBV2	231	227	0.04%	0.005%
17	3.864	779	785	788	rVV2	237	263	0.05%	0.006%
18	4.057	837	845	850	rBV2	258	385	0.07%	0.009%
19	4.282	912	915	920	rVB	381	328	0.06%	0.007%
20	4.311	920	924	926	rBV	285	220	0.04%	0.005%
21	4.620	1008	1020	1043	rBV	47887	117851	20.32%	2.612%
22	4.745	1057	1059	1063	rVB2	430	254	0.04%	0.006%
23	4.932	1113	1117	1120	rVB3	243	201	0.03%	0.004%
24	5.057	1139	1156	1179	rBV	106863	235188	40.55%	5.212%
25	5.163	1186	1189	1190	rBV2	365	204	0.04%	0.005%
26	5.327	1234	1240	1244	rBV3	525	570	0.10%	0.013%
27	5.414	1261	1267	1270	rBV2	173	176	0.03%	0.004%
28	5.600	1322	1325	1330	rVB	324	253	0.04%	0.006%
29	5.629	1330	1334	1337	rBV	220	269	0.05%	0.006%
30	5.719	1341	1362	1386	rBV2	215189	579940	100.00%	12.852%
31	6.006	1447	1451	1455	rVV	216	232	0.04%	0.005%
32	6.121	1482	1487	1490	rBV2	286	217	0.04%	0.005%
33	6.170	1496	1502	1504	rBV2	199	240	0.04%	0.005%
34	6.243	1511	1525	1543	rBV	197699	381414	65.77%	8.452%
35	6.526	1602	1613	1614	rBV4	1467	1605	0.28%	0.036%
36	6.555	1620	1622	1625	rVB3	637	313	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050823\
 Data File : VU054084.D
 Acq On : 08 May 2023 16:43
 Operator : JC/MD
 Sample : 02662-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AZ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

37	6.600	1634	1636	1640	rVB2	420	288	0.05%	0.006%
38	6.684	1649	1662	1681	rBV	136533	263290	45.40%	5.835%
39	6.973	1747	1752	1756	rBV	192	221	0.04%	0.005%
40	7.112	1792	1795	1798	rBV2	250	251	0.04%	0.006%
41	7.131	1798	1801	1809	rVB2	220	264	0.05%	0.006%
42	7.176	1809	1815	1816	rBV3	423	354	0.06%	0.008%
43	7.195	1818	1821	1825	rVB3	573	468	0.08%	0.010%
44	7.562	1922	1935	1950	rBV	73578	127996	22.07%	2.836%
45	7.893	2025	2038	2054	rBV	259958	447135	77.10%	9.909%
46	8.173	2115	2125	2142	rBV2	52273	87550	15.10%	1.940%
47	8.427	2200	2204	2207	rBV2	318	256	0.04%	0.006%
48	8.472	2208	2218	2228	rVB3	1839	2860	0.49%	0.063%
49	8.555	2233	2244	2248	rBV3	479	790	0.14%	0.018%
50	8.629	2255	2267	2298	rBV2	136954	260219	44.87%	5.767%
51	8.771	2308	2311	2314	rBV	314	241	0.04%	0.005%
52	9.018	2384	2388	2391	rBV	197	177	0.03%	0.004%
53	9.366	2492	2496	2498	rBV	300	205	0.04%	0.005%
54	9.414	2498	2511	2532	rBV	271277	460247	79.36%	10.199%
55	9.542	2548	2551	2555	rBV2	225	191	0.03%	0.004%
56	9.613	2569	2573	2576	rBV	202	180	0.03%	0.004%
57	10.108	2723	2727	2730	rBV	262	302	0.05%	0.007%
58	10.128	2730	2733	2736	rVV	314	257	0.04%	0.006%
59	10.160	2740	2743	2746	rVB	366	248	0.04%	0.005%
60	10.182	2746	2750	2753	rBV2	339	321	0.06%	0.007%
61	10.230	2759	2765	2768	rBV2	321	324	0.06%	0.007%
62	10.407	2814	2820	2824	rBV2	332	383	0.07%	0.008%
63	10.446	2827	2832	2835	rBV2	294	328	0.06%	0.007%
64	10.571	2864	2871	2874	rBV2	261	352	0.06%	0.008%
65	10.677	2900	2904	2906	rBV2	229	213	0.04%	0.005%
66	10.751	2914	2927	2945	rBV	185258	299578	51.66%	6.639%
67	10.890	2961	2970	2975	rBV3	1925	2353	0.41%	0.052%
68	10.986	2996	3000	3005	rVB2	295	294	0.05%	0.007%
69	11.031	3010	3014	3017	rBV	277	222	0.04%	0.005%
70	11.063	3019	3024	3028	rBV	185	204	0.04%	0.005%
71	11.285	3089	3093	3096	rVV	263	214	0.04%	0.005%
72	11.340	3105	3110	3115	rBV2	328	407	0.07%	0.009%
73	11.404	3127	3130	3135	rBV	227	204	0.04%	0.005%
74	11.713	3223	3226	3230	rVB2	377	274	0.05%	0.006%
75	11.806	3243	3255	3276	rBV	281447	450304	77.65%	9.979%
76	11.938	3293	3296	3300	rVB3	477	310	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050823\
 Data File : VU054084.D
 Acq On : 08 May 2023 16:43
 Operator : JC/MD
 Sample : 02662-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AZ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

77	12.050	3327	3331	3335	rBV2	305	250	0.04%	0.006%
78	12.189	3361	3374	3394	rBV	268541	436524	75.27%	9.674%
79	12.652	3509	3518	3521	rBV2	355	545	0.09%	0.012%
80	12.767	3549	3554	3559	rVB2	568	450	0.08%	0.010%
81	12.793	3559	3562	3564	rBV	218	176	0.03%	0.004%
82	12.822	3569	3571	3573	rVV	384	225	0.04%	0.005%
83	12.838	3574	3576	3581	rVB	394	237	0.04%	0.005%
84	12.931	3601	3605	3608	rBV	408	349	0.06%	0.008%
85	13.037	3635	3638	3643	rVV2	241	203	0.04%	0.004%
86	13.208	3689	3691	3695	rVB	291	184	0.03%	0.004%
87	13.272	3708	3711	3714	rVB2	319	182	0.03%	0.004%
88	13.539	3791	3794	3797	rBV	301	185	0.03%	0.004%
89	13.581	3804	3807	3810	rBV2	368	271	0.05%	0.006%
90	13.616	3814	3818	3822	rBV2	465	346	0.06%	0.008%
91	13.767	3862	3865	3869	rBV2	240	267	0.05%	0.006%
92	13.816	3877	3880	3882	rBV3	289	206	0.04%	0.005%
93	14.243	4005	4013	4015	rBV2	489	635	0.11%	0.014%
94	14.385	4054	4057	4059	rBV2	290	200	0.03%	0.004%
95	14.822	4190	4193	4196	rBV3	373	254	0.04%	0.006%
96	15.275	4332	4334	4339	rBV	406	338	0.06%	0.007%
97	15.372	4361	4364	4370	rVB2	465	284	0.05%	0.006%
98	15.533	4408	4414	4418	rBV4	751	874	0.15%	0.019%
99	15.587	4428	4431	4434	rBV3	548	393	0.07%	0.009%
100	15.623	4439	4442	4446	rBV2	552	472	0.08%	0.010%




Sum of corrected areas: 4512485

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050823\
Data File : VU054084.D
Acq On : 08 May 2023 16:43
Operator : JC/MD
Sample : 02662-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AZ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

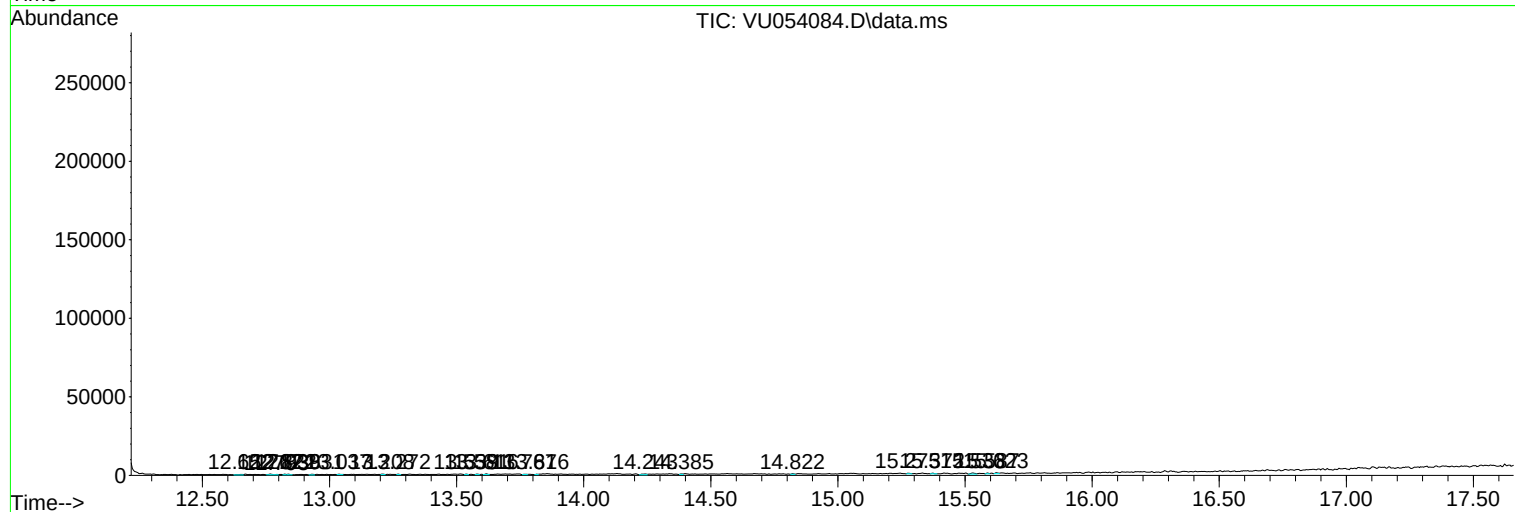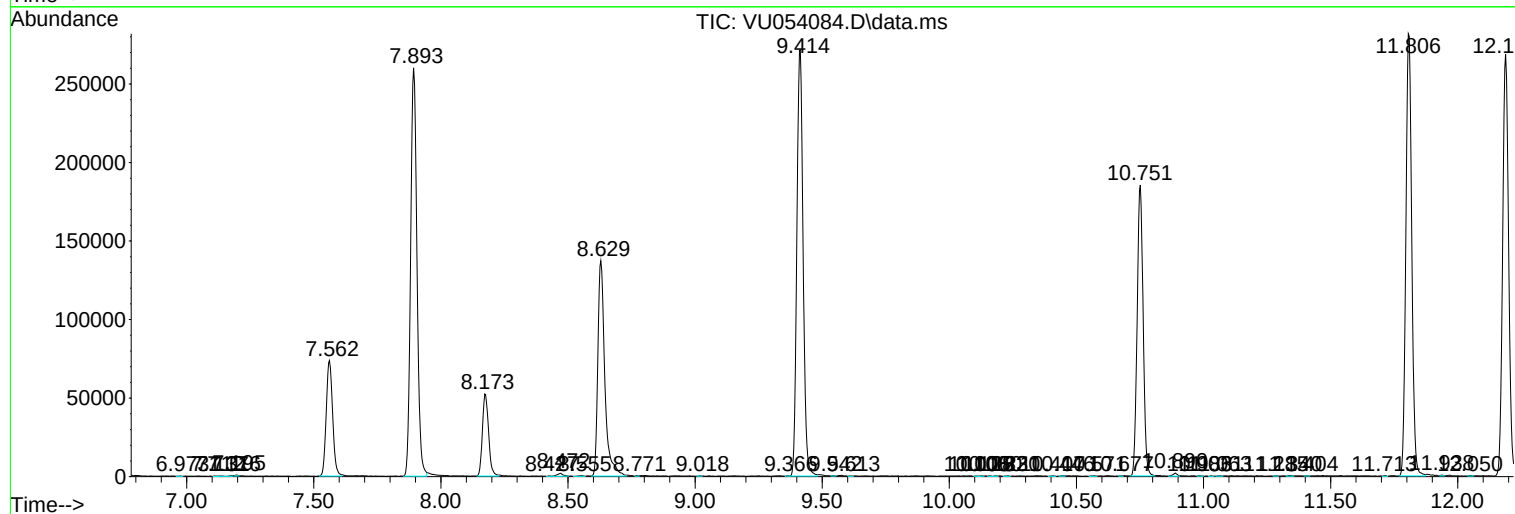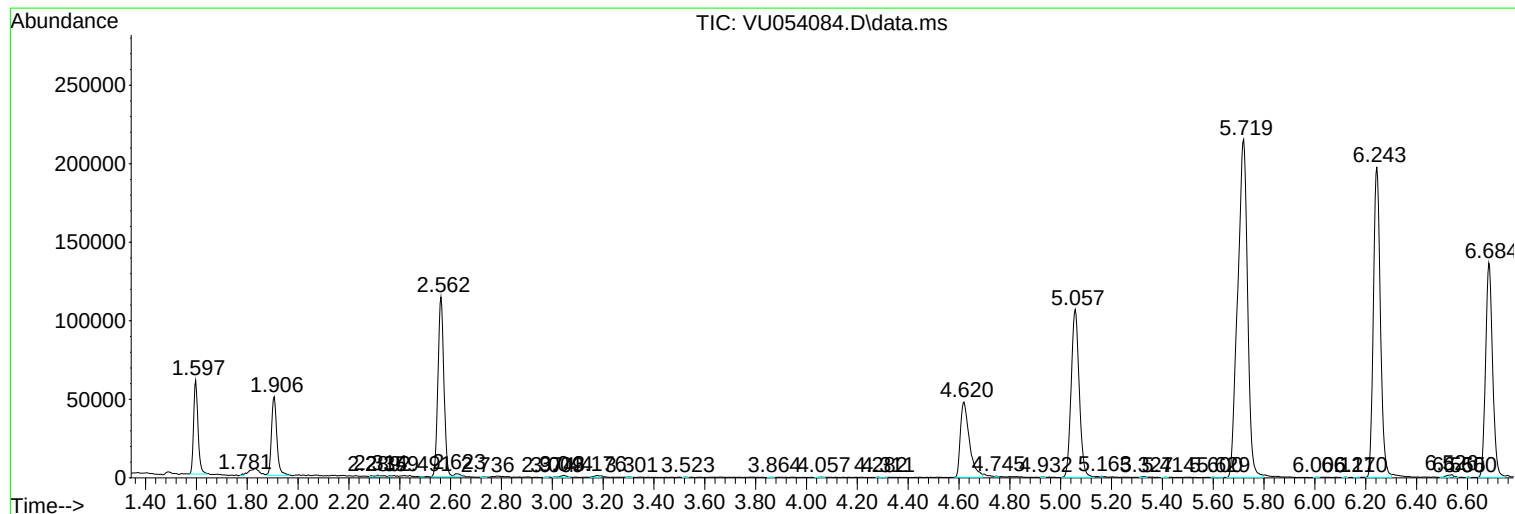

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050823\
Data File : VU054084.D
Acq On : 08 May 2023 16:43
Operator : JC/MD
Sample : 02662-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AZ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050823\
Data File : VU054084.D
Acq On : 08 May 2023 16:43
Operator : JC/MD
Sample : 02662-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AZ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------