

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050823\
 Data File : VU054086.D
 Acq On : 08 May 2023 17:31
 Operator : JC/MD
 Sample : 02662-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AZ8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

Signal : TIC: VU054086.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	96	rBV	79383	100008	11.91%	1.537%
2	1.781	135	137	139	rBV	717	492	0.06%	0.008%
3	1.903	166	175	191	rVB	69531	97019	11.55%	1.491%
4	2.221	268	274	276	rBV3	433	460	0.05%	0.007%
5	2.337	306	310	313	rVB2	922	695	0.08%	0.011%
6	2.363	313	318	319	rBV2	420	358	0.04%	0.006%
7	2.510	361	364	367	rVB2	361	219	0.03%	0.003%
8	2.562	367	380	396	rBV	160127	260742	31.04%	4.007%
9	2.697	419	422	425	rVB2	406	185	0.02%	0.003%
10	2.774	443	446	447	rBV	506	280	0.03%	0.004%
11	3.038	522	528	539	rBV4	1140	2017	0.24%	0.031%
12	3.182	561	573	581	rBV2	1413	3532	0.42%	0.054%
13	3.282	600	604	607	rVB2	323	213	0.03%	0.003%
14	3.298	607	609	611	rBV	261	164	0.02%	0.003%
15	3.337	615	621	624	rBV2	223	288	0.03%	0.004%
16	3.430	644	650	652	rBV	220	231	0.03%	0.004%
17	3.465	658	661	666	rVB	172	164	0.02%	0.003%
18	3.546	683	686	692	rBV2	175	200	0.02%	0.003%
19	3.623	707	710	712	rBV2	295	247	0.03%	0.004%
20	3.703	732	735	739	rVV2	265	238	0.03%	0.004%
21	3.752	744	750	752	rVV2	263	225	0.03%	0.003%
22	3.768	752	755	763	rVB2	196	240	0.03%	0.004%
23	3.877	784	789	794	rBV2	242	293	0.03%	0.005%
24	3.922	800	803	809	rVB2	162	181	0.02%	0.003%
25	4.025	833	835	838	rBV	238	175	0.02%	0.003%
26	4.234	897	900	905	rVB2	218	233	0.03%	0.004%
27	4.375	939	944	945	rBV2	187	165	0.02%	0.003%
28	4.420	951	958	961	rBV2	265	343	0.04%	0.005%
29	4.449	961	967	970	rBV2	271	343	0.04%	0.005%
30	4.504	980	984	989	rBV2	171	187	0.02%	0.003%
31	4.571	1001	1005	1007	rBV2	203	191	0.02%	0.003%
32	4.620	1008	1020	1046	rBV	73984	184371	21.95%	2.834%
33	4.870	1095	1098	1101	rBV3	289	247	0.03%	0.004%
34	5.057	1140	1156	1175	rBV	154063	337783	40.21%	5.191%
35	5.263	1217	1220	1227	rBV3	359	434	0.05%	0.007%
36	5.327	1234	1240	1244	rVV3	504	665	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050823\
 Data File : VU054086.D
 Acq On : 08 May 2023 17:31
 Operator : JC/MD
 Sample : 02662-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AZ8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

37	5.350	1244	1247	1250	rVV2	414	262	0.03%	0.004%
38	5.411	1263	1266	1268	rBV	267	195	0.02%	0.003%
39	5.433	1270	1273	1279	rVB2	182	217	0.03%	0.003%
40	5.719	1341	1362	1386	rBV2	303504	840049	100.00%	12.911%
41	5.874	1407	1410	1413	rVB3	364	178	0.02%	0.003%
42	6.099	1476	1480	1485	rBV2	176	193	0.02%	0.003%
43	6.124	1485	1488	1493	rBV3	296	268	0.03%	0.004%
44	6.243	1508	1525	1556	rBV	282314	540002	64.28%	8.299%
45	6.530	1605	1614	1623	rVB5	2709	5013	0.60%	0.077%
46	6.684	1647	1662	1685	rBV	198295	385124	45.85%	5.919%
47	6.986	1753	1756	1764	rBV2	143	182	0.02%	0.003%
48	7.189	1813	1819	1827	rBV4	1324	1713	0.20%	0.026%
49	7.440	1892	1897	1902	rVV2	188	270	0.03%	0.004%
50	7.558	1923	1934	1951	rBV	107867	190620	22.69%	2.930%
51	7.806	2007	2011	2015	rBV2	306	286	0.03%	0.004%
52	7.893	2024	2038	2071	rBV	378454	657161	78.23%	10.100%
53	8.176	2114	2126	2145	rBV	77670	131998	15.71%	2.029%
54	8.308	2163	2167	2171	rBV2	389	351	0.04%	0.005%
55	8.439	2205	2208	2209	rBV	265	171	0.02%	0.003%
56	8.465	2210	2216	2218	rBV5	1576	1687	0.20%	0.026%
57	8.552	2238	2243	2244	rBV2	330	265	0.03%	0.004%
58	8.629	2255	2267	2298	rBV2	212178	402914	47.96%	6.192%
59	8.774	2310	2312	2316	rVB2	379	204	0.02%	0.003%
60	8.854	2335	2337	2340	rBV	325	244	0.03%	0.004%
61	8.964	2368	2371	2377	rVB	359	329	0.04%	0.005%
62	9.128	2418	2422	2429	rBV2	164	221	0.03%	0.003%
63	9.411	2498	2510	2545	rBV	389328	645895	76.89%	9.927%
64	9.565	2554	2558	2564	rVB2	464	498	0.06%	0.008%
65	9.607	2568	2571	2576	rBV2	217	213	0.03%	0.003%
66	9.803	2630	2632	2638	rVB2	248	216	0.03%	0.003%
67	9.838	2638	2643	2646	rBV2	194	224	0.03%	0.003%
68	9.989	2687	2690	2695	rVB2	355	324	0.04%	0.005%
69	10.025	2699	2701	2707	rVB2	221	219	0.03%	0.003%
70	10.436	2824	2829	2830	rBV	234	221	0.03%	0.003%
71	10.500	2846	2849	2854	rVB3	503	423	0.05%	0.007%
72	10.661	2896	2899	2902	rBV	241	201	0.02%	0.003%
73	10.751	2915	2927	2942	rBV	278558	443813	52.83%	6.821%
74	10.886	2961	2969	2978	rVV3	1991	2778	0.33%	0.043%
75	10.941	2983	2986	2988	rBV	249	187	0.02%	0.003%
76	11.012	3005	3008	3014	rVB2	283	279	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050823\
 Data File : VU054086.D
 Acq On : 08 May 2023 17:31
 Operator : JC/MD
 Sample : 02662-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AZ8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

77	11.086	3028	3031	3035	rBV	338	293	0.03%	0.005%
78	11.475	3148	3152	3157	rVB2	421	368	0.04%	0.006%
79	11.497	3157	3159	3163	rBV2	238	189	0.02%	0.003%
80	11.745	3229	3236	3239	rBV4	572	636	0.08%	0.010%
81	11.806	3239	3255	3284	rBV	392925	624667	74.36%	9.601%
82	11.976	3305	3308	3312	rBV3	228	225	0.03%	0.003%
83	12.037	3324	3327	3330	rBV	253	175	0.02%	0.003%
84	12.189	3361	3374	3398	rBV	383427	625638	74.48%	9.616%
85	12.500	3467	3471	3478	rBV2	278	323	0.04%	0.005%
86	13.246	3700	3703	3708	rVB2	375	264	0.03%	0.004%
87	13.333	3724	3730	3732	rBV	299	312	0.04%	0.005%
88	13.356	3733	3737	3740	rVV3	309	289	0.03%	0.004%
89	13.529	3788	3791	3799	rVB2	261	268	0.03%	0.004%
90	13.751	3856	3860	3865	rVV2	344	283	0.03%	0.004%
91	13.780	3865	3869	3873	rBV2	248	274	0.03%	0.004%
92	13.851	3889	3891	3896	rVB3	619	434	0.05%	0.007%
93	14.105	3967	3970	3974	rVB3	392	378	0.04%	0.006%
94	14.571	4111	4115	4120	rBV4	435	542	0.06%	0.008%
95	14.709	4156	4158	4161	rVB	431	180	0.02%	0.003%
96	14.889	4211	4214	4215	rBV	360	215	0.03%	0.003%
97	14.954	4231	4234	4237	rBV2	385	275	0.03%	0.004%
98	15.176	4300	4303	4305	rVB2	387	218	0.03%	0.003%
99	15.484	4396	4399	4404	rBV2	497	366	0.04%	0.006%
100	15.539	4414	4416	4418	rBV2	452	271	0.03%	0.004%




Sum of corrected areas: 6506519

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050823\
Data File : VU054086.D
Acq On : 08 May 2023 17:31
Operator : JC/MD
Sample : 02662-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AZ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

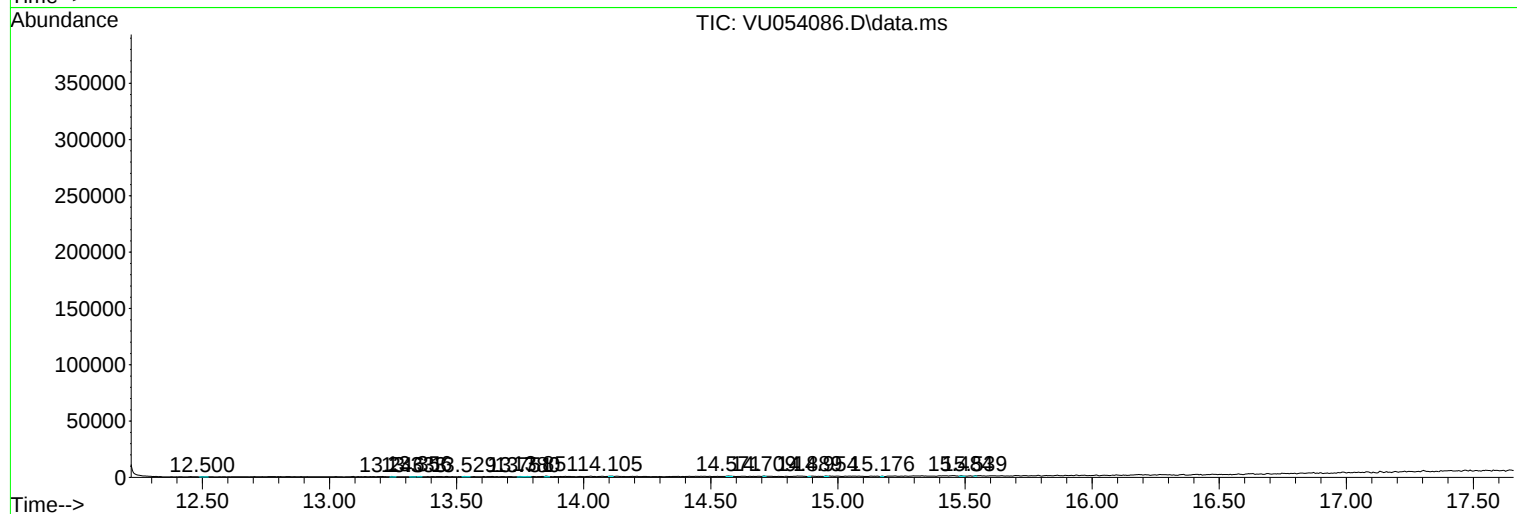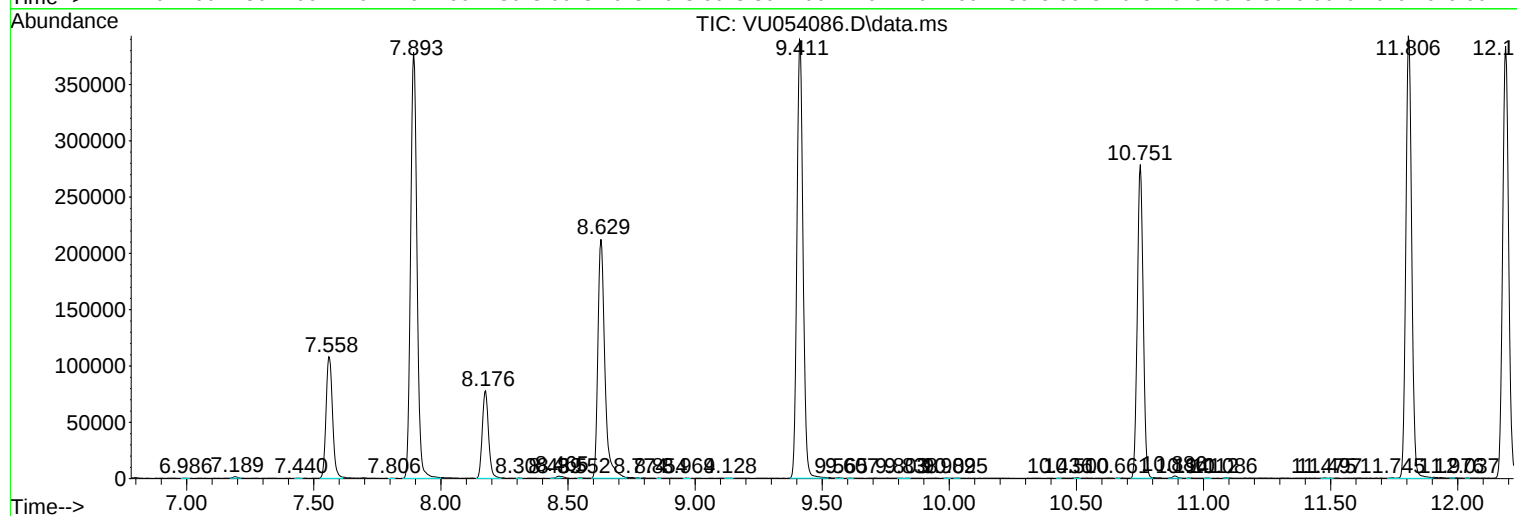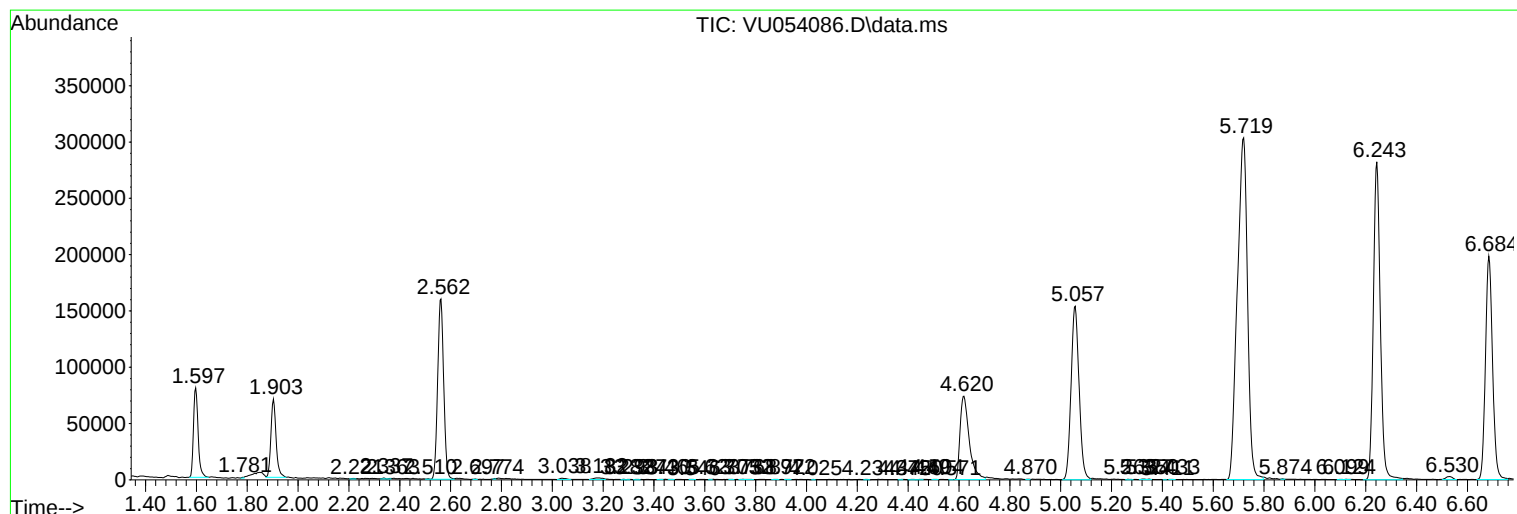

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050823\
Data File : VU054086.D
Acq On : 08 May 2023 17:31
Operator : JC/MD
Sample : 02662-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AZ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050823\
Data File : VU054086.D
Acq On : 08 May 2023 17:31
Operator : JC/MD
Sample : 02662-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AZ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc