

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050823\
 Data File : VU054088.D
 Acq On : 08 May 2023 18:18
 Operator : JC/MD
 Sample : 02662-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B00

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

Signal : TIC: VU054088.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	41	45	52	rVB4	2190	2173	0.28%	0.036%
2	1.598	72	80	94	rBV	75631	92669	12.01%	1.526%
3	1.781	132	137	138	rBV4	1893	1575	0.20%	0.026%
4	1.903	165	175	195	rVB	63817	92785	12.03%	1.528%
5	2.122	241	243	245	rBV2	497	218	0.03%	0.004%
6	2.341	309	311	314	rVB3	523	296	0.04%	0.005%
7	2.366	315	319	320	rBV	703	384	0.05%	0.006%
8	2.418	332	335	336	rBV3	530	289	0.04%	0.005%
9	2.514	362	365	368	rBV2	302	272	0.04%	0.004%
10	2.562	368	380	395	rVV	150788	244011	31.63%	4.018%
11	2.762	434	442	446	rBV2	887	1199	0.16%	0.020%
12	2.788	447	450	458	rVB4	1368	1467	0.19%	0.024%
13	2.968	504	506	512	rVB2	297	190	0.02%	0.003%
14	3.042	522	529	538	rVB3	1066	1516	0.20%	0.025%
15	3.099	544	547	549	rBV	280	174	0.02%	0.003%
16	3.183	561	573	577	rBV2	2143	3252	0.42%	0.054%
17	3.328	616	618	624	rVB2	219	215	0.03%	0.004%
18	3.543	680	685	688	rBV2	220	230	0.03%	0.004%
19	3.614	701	707	710	rBV	226	236	0.03%	0.004%
20	3.656	717	720	728	rVB2	293	437	0.06%	0.007%
21	3.707	728	736	737	rBV2	243	369	0.05%	0.006%
22	4.109	855	861	864	rBV2	270	381	0.05%	0.006%
23	4.617	1008	1019	1047	rBV	65284	163020	21.13%	2.684%
24	5.054	1136	1155	1176	rBV	147627	328537	42.59%	5.410%
25	5.283	1221	1226	1228	rBV2	379	291	0.04%	0.005%
26	5.321	1228	1238	1240	rBV2	611	698	0.09%	0.011%
27	5.366	1249	1252	1256	rBV2	206	206	0.03%	0.003%
28	5.450	1273	1278	1283	rBV2	274	436	0.06%	0.007%
29	5.578	1315	1318	1325	rVB2	259	353	0.05%	0.006%
30	5.627	1327	1333	1338	rBV2	260	411	0.05%	0.007%
31	5.720	1341	1362	1382	rBV2	279813	771426	100.00%	12.702%
32	5.877	1408	1411	1418	rVB3	611	397	0.05%	0.007%
33	6.112	1479	1484	1487	rVV2	361	368	0.05%	0.006%
34	6.244	1511	1525	1550	rBV	256711	496964	64.42%	8.183%
35	6.566	1621	1625	1631	rBV2	244	264	0.03%	0.004%
36	6.594	1631	1634	1639	rBV3	198	176	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050823\
 Data File : VU054088.D
 Acq On : 08 May 2023 18:18
 Operator : JC/MD
 Sample : 02662-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B00

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

37	6.684	1649	1662	1682	rBV	182967	353593	45.84%	5.822%
38	6.874	1716	1721	1723	rBV	268	253	0.03%	0.004%
39	7.070	1775	1782	1786	rBV2	118	175	0.02%	0.003%
40	7.193	1812	1820	1828	rBV3	1030	1734	0.22%	0.029%
41	7.488	1907	1912	1914	rBV2	220	198	0.03%	0.003%
42	7.559	1921	1934	1954	rBV	100714	177197	22.97%	2.918%
43	7.697	1975	1977	1983	rVB2	514	451	0.06%	0.007%
44	7.797	2004	2008	2011	rVB2	289	228	0.03%	0.004%
45	7.893	2024	2038	2062	rBV	349920	607904	78.80%	10.010%
46	8.173	2113	2125	2146	rVV	71784	119880	15.54%	1.974%
47	8.392	2189	2193	2196	rBV2	225	205	0.03%	0.003%
48	8.414	2196	2200	2208	rVV2	218	395	0.05%	0.007%
49	8.456	2208	2213	2214	rVV2	813	588	0.08%	0.010%
50	8.469	2214	2217	2225	rVB5	1332	1679	0.22%	0.028%
51	8.630	2255	2267	2297	rBV2	199561	373690	48.44%	6.153%
52	8.794	2315	2318	2322	rVV2	387	220	0.03%	0.004%
53	9.035	2387	2393	2399	rBV2	287	462	0.06%	0.008%
54	9.315	2475	2480	2483	rBV2	221	229	0.03%	0.004%
55	9.331	2483	2485	2488	rVB	398	228	0.03%	0.004%
56	9.360	2488	2494	2497	rBV2	315	382	0.05%	0.006%
57	9.411	2497	2510	2532	rBV	356361	596271	77.29%	9.818%
58	9.562	2553	2557	2558	rBV	368	226	0.03%	0.004%
59	9.594	2562	2567	2575	rVB3	440	625	0.08%	0.010%
60	9.720	2603	2606	2610	rBV2	210	200	0.03%	0.003%
61	9.797	2626	2630	2633	rBV2	207	176	0.02%	0.003%
62	9.964	2678	2682	2685	rVV	249	221	0.03%	0.004%
63	10.006	2691	2695	2698	rVV2	245	178	0.02%	0.003%
64	10.022	2698	2700	2707	rVB	239	262	0.03%	0.004%
65	10.061	2707	2712	2717	rBV	283	330	0.04%	0.005%
66	10.192	2747	2753	2755	rBV2	200	185	0.02%	0.003%
67	10.318	2785	2792	2797	rBV2	303	468	0.06%	0.008%
68	10.485	2836	2844	2847	rBV3	666	832	0.11%	0.014%
69	10.540	2857	2861	2865	rBV2	253	246	0.03%	0.004%
70	10.620	2883	2886	2889	rBV2	217	186	0.02%	0.003%
71	10.752	2914	2927	2942	rBV	260690	416693	54.02%	6.861%
72	10.887	2961	2969	2978	rVB2	1557	2353	0.31%	0.039%
73	11.099	3030	3035	3039	rBV2	281	250	0.03%	0.004%
74	11.308	3096	3100	3102	rBV2	227	189	0.02%	0.003%
75	11.614	3190	3195	3204	rBV2	284	419	0.05%	0.007%
76	11.806	3242	3255	3276	rBV	370125	593872	76.98%	9.779%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050823\
 Data File : VU054088.D
 Acq On : 08 May 2023 18:18
 Operator : JC/MD
 Sample : 02662-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B00

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

77	12.054	3327	3332	3335	rBV2	340	335	0.04%	0.006%
78	12.077	3335	3339	3342	rBV2	346	380	0.05%	0.006%
79	12.128	3352	3355	3359	rBV2	356	369	0.05%	0.006%
80	12.189	3361	3374	3395	rVV	367116	604094	78.31%	9.947%
81	12.347	3418	3423	3426	rBV2	373	446	0.06%	0.007%
82	12.405	3438	3441	3445	rVB	499	309	0.04%	0.005%
83	12.459	3454	3458	3461	rBV	259	218	0.03%	0.004%
84	12.549	3482	3486	3488	rBV2	365	232	0.03%	0.004%
85	12.993	3622	3624	3631	rVB2	289	216	0.03%	0.004%
86	13.144	3667	3671	3675	rVB	358	338	0.04%	0.006%
87	13.173	3675	3680	3681	rBV	513	397	0.05%	0.007%
88	13.289	3713	3716	3720	rBV2	244	190	0.02%	0.003%
89	13.324	3723	3727	3734	rBV	351	459	0.06%	0.008%
90	13.446	3761	3765	3768	rBV2	234	216	0.03%	0.004%
91	13.861	3892	3894	3898	rVB2	402	253	0.03%	0.004%
92	13.935	3913	3917	3920	rBV2	393	325	0.04%	0.005%
93	13.986	3929	3933	3938	rBV2	280	266	0.03%	0.004%
94	14.012	3938	3941	3943	rBV2	354	263	0.03%	0.004%
95	14.044	3948	3951	3955	rVB2	245	199	0.03%	0.003%
96	14.276	4020	4023	4029	rBV3	389	490	0.06%	0.008%
97	14.440	4071	4074	4077	rBV	327	232	0.03%	0.004%
98	14.601	4121	4124	4127	rBV2	344	245	0.03%	0.004%
99	15.800	4492	4497	4498	rBV3	541	502	0.07%	0.008%
100	16.260	4638	4640	4643	rBV3	775	443	0.06%	0.007%




Sum of corrected areas: 6073175

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050823\
Data File : VU054088.D
Acq On : 08 May 2023 18:18
Operator : JC/MD
Sample : 02662-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B00

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

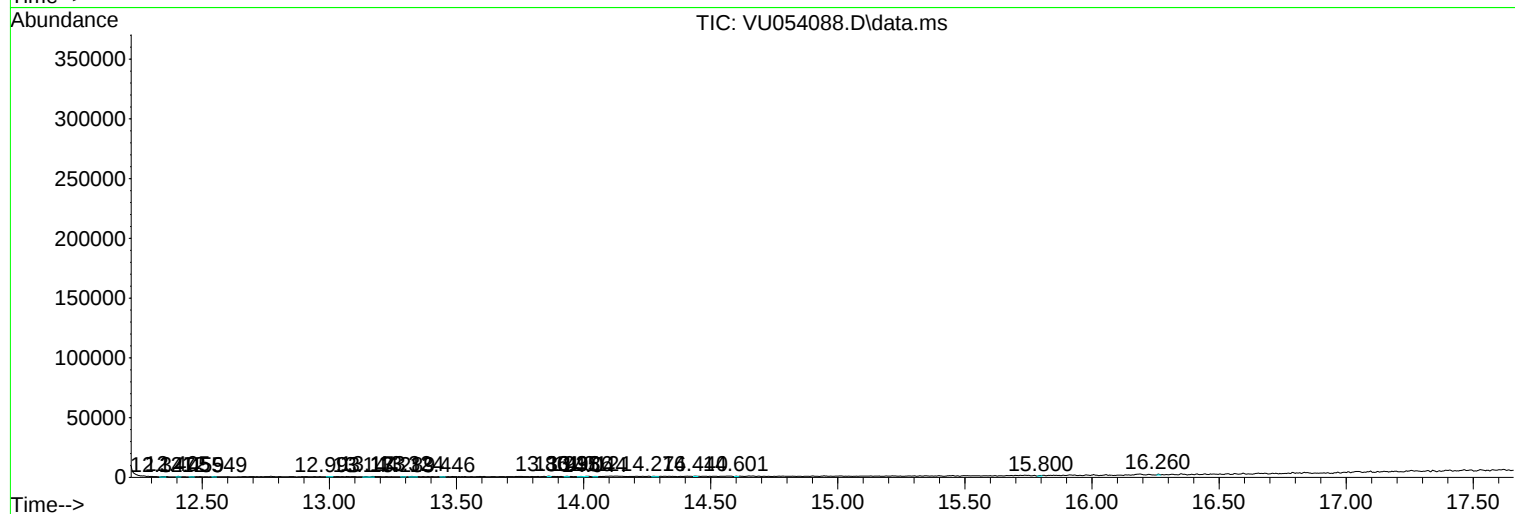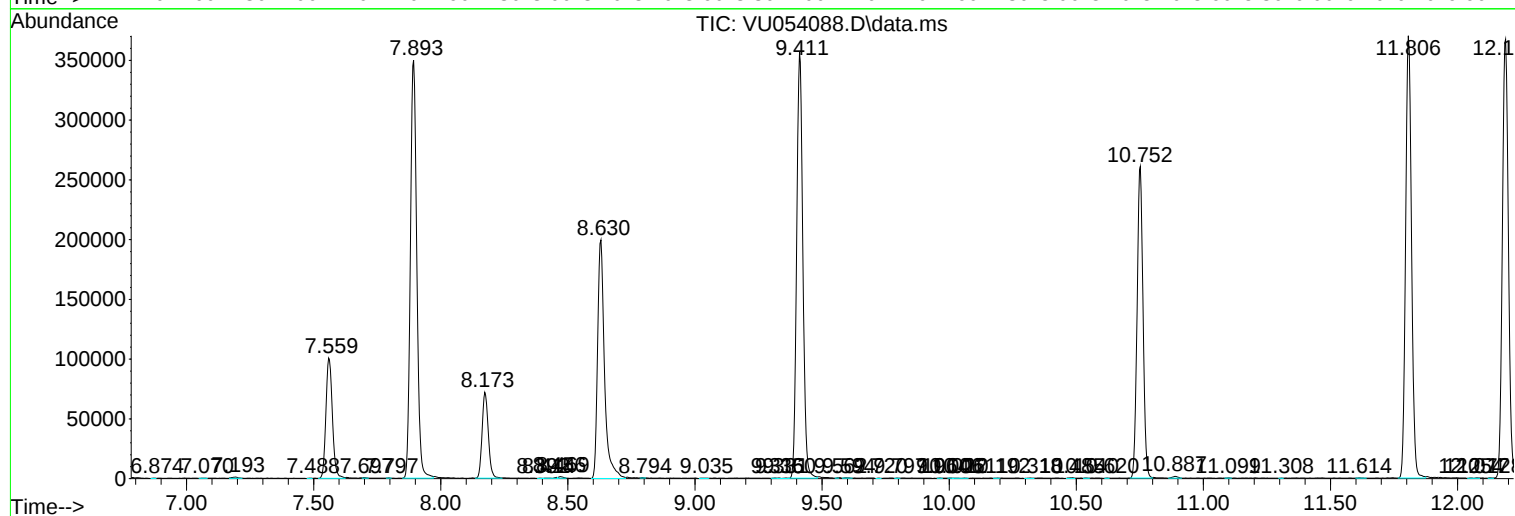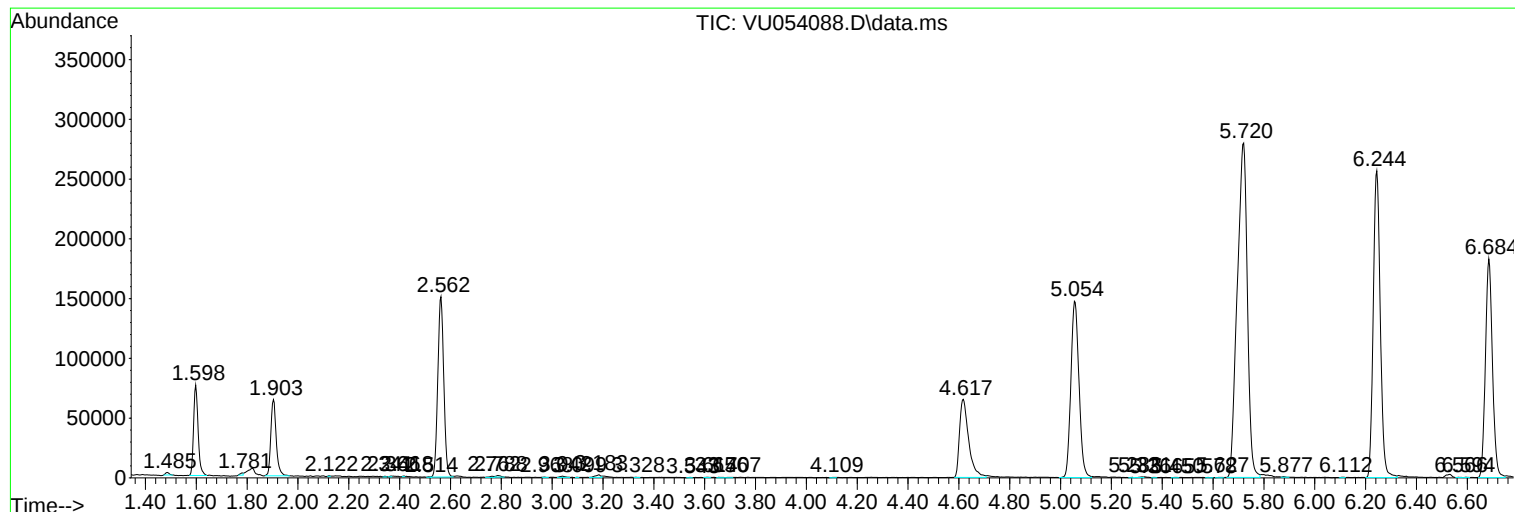

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050823\
Data File : VU054088.D
Acq On : 08 May 2023 18:18
Operator : JC/MD
Sample : 02662-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B00

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050823\
Data File : VU054088.D
Acq On : 08 May 2023 18:18
Operator : JC/MD
Sample : 02662-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B00

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc