
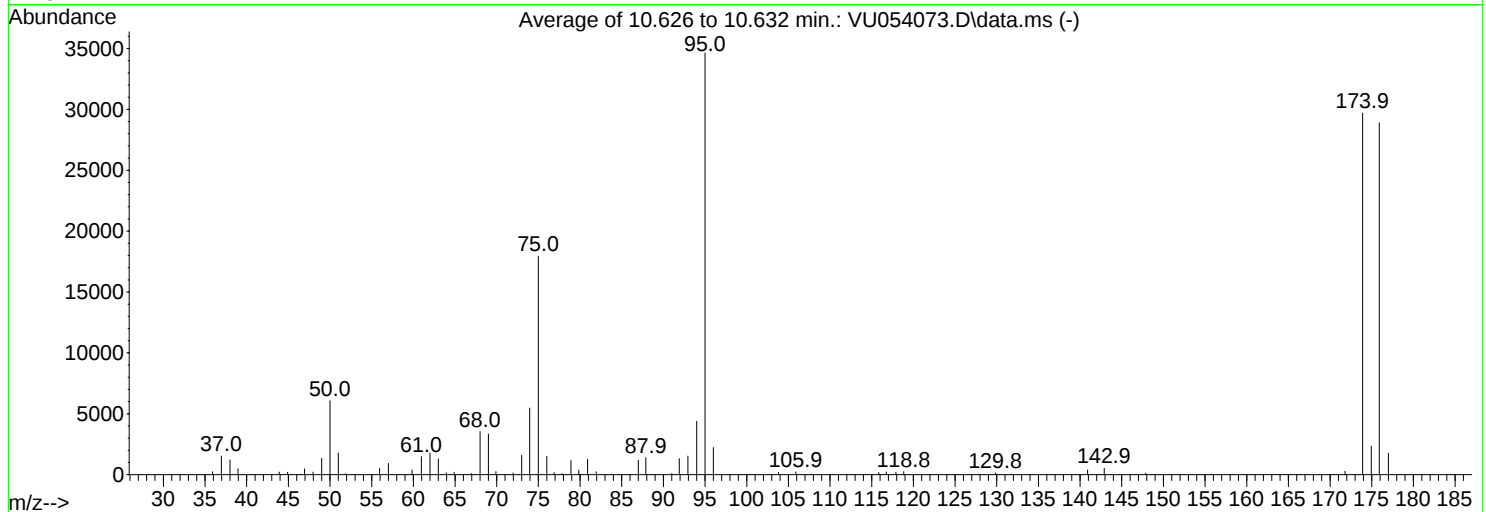


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050823\
 Data File : VU054073.D
 Acq On : 08 May 2023 11:41
 Operator : JC/MD
 Sample : BFB187
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB187

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis
 Last Update : Sat May 06 01:14:00 2023

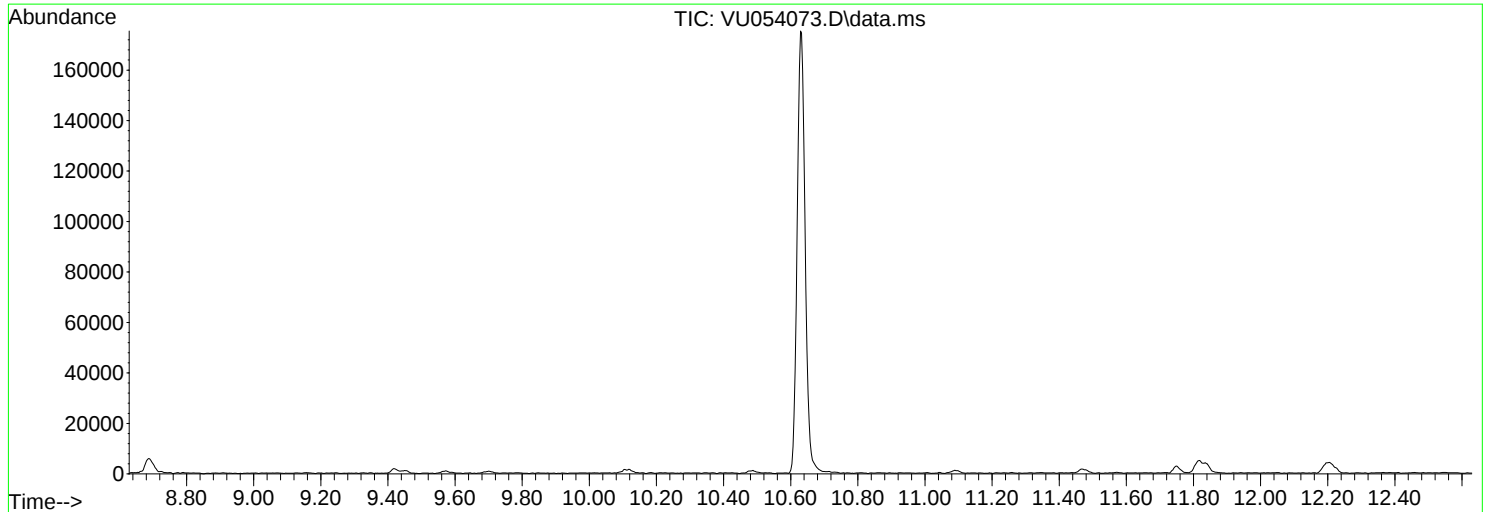

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	6077	PASS
75	95	30	80	51.8	17941	PASS
95	95	100	100	100.0	34645	PASS
96	95	5	9	6.4	2225	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	85.7	29691	PASS
175	174	5	9	7.9	2337	PASS
176	174	95	101	97.3	28904	PASS
177	176	5	9	6.1	1756	PASS

m/z	Abundance
40.00	102.0
44.00	229.0

Instrument :
MSVOA_U
ClientSampleId :
BFB187

m/z	Abundance
35.90	214.0
36.90	1565.0
38.00	1146.0
39.00	455.0
40.00	110.0
43.90	412.0
44.90	203.0
46.90	435.0
48.00	186.0
49.00	1271.0
50.00	5742.0
51.00	1734.0
56.00	464.0
57.00	903.0
59.90	416.0
61.00	1411.0
62.00	1758.0
63.00	1346.0
63.90	151.0
64.90	193.0
68.00	3391.0
69.00	3167.0
69.90	278.0
72.00	128.0
73.00	1497.0
73.90	5348.0
75.00	17240.0
76.00	1529.0
77.00	146.0
77.90	115.0
78.90	1103.0
79.90	371.0
80.90	1189.0
81.90	204.0
87.00	1051.0
87.90	1210.0
91.90	1322.0
92.90	1438.0
94.00	4244.0
95.00	32648.0
96.00	2314.0
103.80	159.0
105.90	237.0
115.80	132.0
116.70	193.0
117.90	160.0
118.90	267.0
127.80	101.0
129.90	157.0
140.90	323.0
142.90	508.0
147.90	123.0
171.80	300.0
173.90	27280.0
174.90	2189.0
175.90	26680.0
177.00	1693.0

Instrument :
MSVOA_U
ClientSampleId :
BFB187

m/z	Abundance
35.90	238.0
36.90	1552.0
38.00	1231.0
39.00	482.0
40.00	120.0
43.90	448.0
44.90	205.0
46.90	479.0
48.00	220.0
49.00	1379.0
50.00	6260.0
51.00	1868.0
51.90	117.0
56.00	511.0
57.00	939.0
59.80	408.0
60.90	1534.0
62.00	1844.0
63.00	1345.0
64.00	159.0
64.90	212.0
67.00	116.0
68.00	3622.0
69.00	3409.0
69.90	244.0
72.00	126.0
73.00	1662.0
74.00	5546.0
75.00	18384.0
76.00	1552.0
76.90	168.0
77.80	117.0
78.90	1211.0
79.90	403.0
80.90	1325.0
82.00	250.0
87.00	1232.0
87.90	1462.0
91.00	126.0
91.90	1355.0
92.90	1553.0
94.00	4486.0
95.00	35824.0
96.00	2224.0
103.80	192.0
105.90	269.0
115.90	171.0
116.80	213.0
117.90	201.0
118.90	256.0
129.90	138.0
140.90	400.0
142.90	505.0
147.90	126.0
171.80	313.0
173.90	30672.0
175.00	2423.0
175.90	29824.0
177.00	1821.0

Instrument :
MSVOA_U
ClientSampleId :
BFB187

m/z	Abundance
35.90	266.0
37.00	1475.0
38.00	1264.0
38.90	526.0
40.00	110.0
43.90	460.0
44.90	205.0
47.00	500.0
47.90	218.0
49.00	1367.0
50.00	6228.0
51.00	1763.0
51.90	110.0
55.90	572.0
57.00	911.0
59.80	341.0
61.00	1525.0
62.00	1669.0
63.00	1186.0
64.00	154.0
64.90	205.0
66.90	157.0
68.00	3590.0
69.00	3419.0
69.90	224.0
71.90	134.0
73.00	1614.0
74.00	5522.0
75.00	18200.0
76.00	1410.0
76.80	216.0
78.90	1179.0
79.80	367.0
80.90	1268.0
82.00	269.0
87.00	1282.0
87.90	1525.0
91.00	137.0
91.90	1272.0
93.00	1574.0
94.00	4417.0
95.00	35464.0
96.00	2138.0
103.80	185.0
105.90	222.0
115.90	196.0
116.80	222.0
117.90	225.0
118.80	239.0
129.70	124.0
140.90	436.0
142.90	532.0
147.90	116.0
171.80	274.0
173.90	31120.0
175.00	2400.0
175.90	30208.0
177.00	1754.0

Instrument :
MSVOA_U
ClientSampleId :
BFB187