


Data Path : W:\HPCHEM1\MSVOA U\DATA\VU050918\
 Data File : VU023753.D
 Acq On : 09 May 2018 10:20
 Operator : MD/SY
 Sample : BFB51
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Integration File: LSCINT.P

Method : W:\HPCHEM1\MSVOA_U\METHOD\SOMULM050818WMA.M
 Title : VOC Analysis
 Last Update : Thu May 10 01:29:49 2018

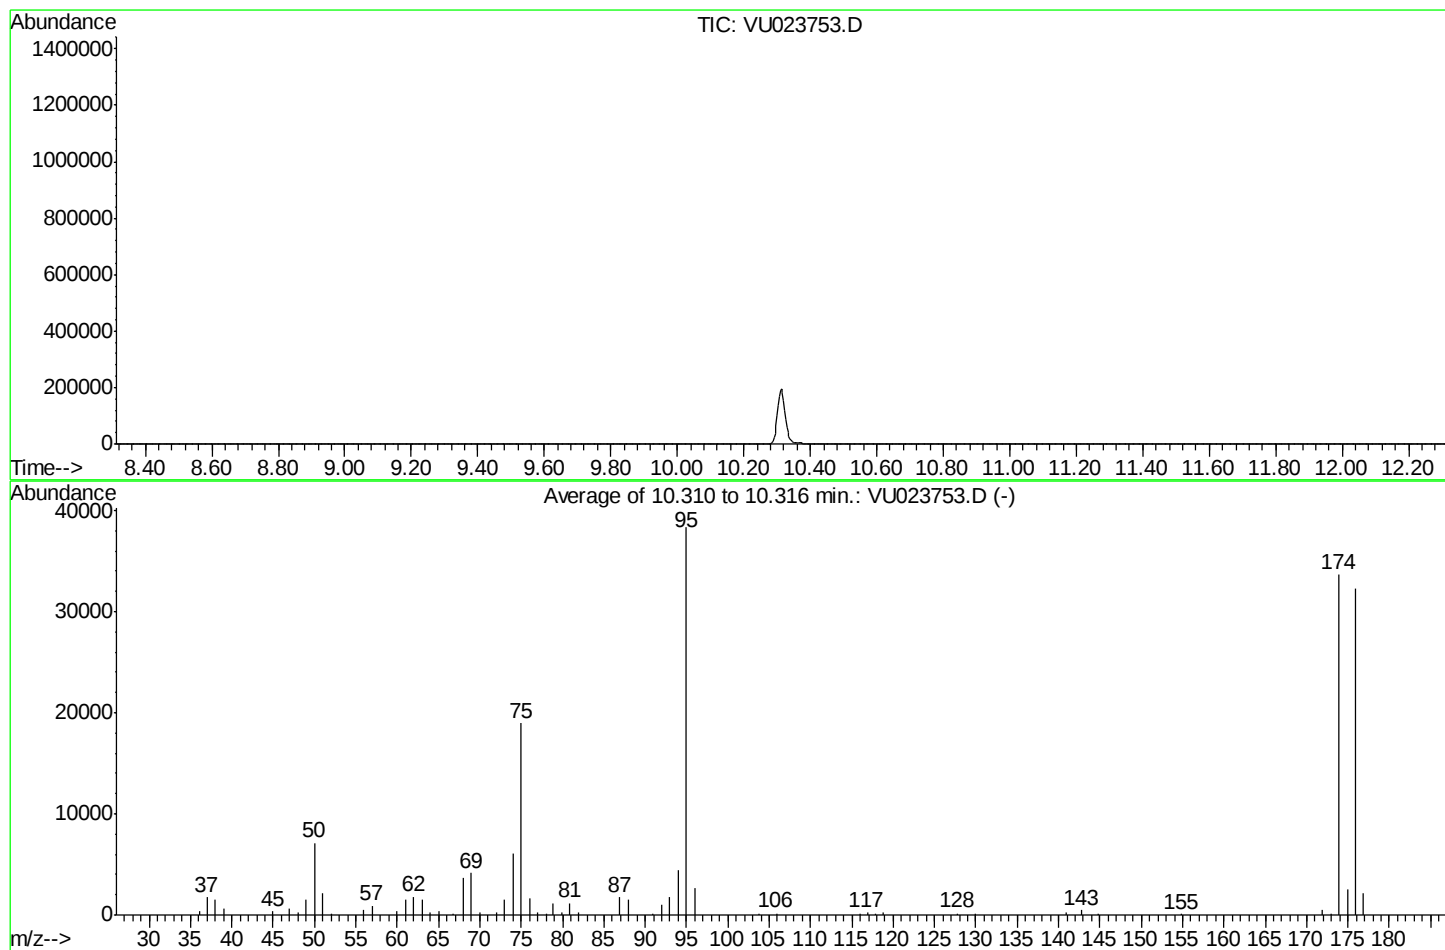

AutoFind: Scans 3023, 3024, 3025; Background Corrected with Scan 3011

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	7099	PASS
75	95	30	80	49.5	18960	PASS
95	95	100	100	100.0	38328	PASS
96	95	5	9	6.8	2608	PASS
173	174	0.00	2	0.5	153	PASS
174	95	50	120	87.8	33648	PASS
175	174	5	9	7.7	2586	PASS
176	174	95	101	95.8	32250	PASS
177	176	5	9	6.8	2202	PASS

Scan 3011 (10.271 min): VU023753.D
BFB51

m/z	Abundance
39.90	757.0
44.00	727.0

m/z	Abundance
36.00	353.0
37.00	1937.0
38.00	1567.0
39.00	720.0
39.90	515.0
43.90	677.0
45.00	354.0
47.00	599.0
48.00	226.0
49.00	1557.0
50.00	7339.0
51.00	2227.0
52.00	100.0
56.00	555.0
57.00	877.0
60.00	413.0
61.00	1607.0
62.00	1874.0
63.00	1624.0
63.90	250.0
65.00	373.0
66.80	117.0
68.00	3738.0
69.00	4216.0
70.00	288.0
72.00	256.0
73.00	1621.0
74.00	6292.0
75.00	19600.0
76.00	1632.0
77.00	215.0
78.00	209.0
78.90	1146.0
79.90	354.0
80.90	1240.0
81.90	255.0
86.90	1804.0
88.00	1613.0
90.90	141.0
92.00	982.0
93.00	1721.0
94.00	4447.0
95.00	39352.0
96.00	2733.0
103.80	143.0
105.90	134.0
116.00	120.0
116.90	272.0
117.80	119.0
118.90	227.0
127.80	178.0
129.90	137.0
140.90	281.0
142.90	452.0
144.80	158.0
154.90	106.0
172.00	416.0
172.90	459.0
173.90	33168.0
175.00	2599.0
175.90	31640.0
176.90	2254.0

m/z	Abundance
36.10	352.0
37.00	1800.0
38.00	1624.0
39.00	683.0
39.90	437.0
43.90	690.0
45.00	346.0
47.00	593.0
48.00	227.0
49.00	1584.0
50.00	7292.0
51.00	2289.0
52.00	107.0
56.00	566.0
57.00	909.0
60.00	367.0
61.00	1563.0
62.00	1920.0
63.00	1628.0
63.90	242.0
65.00	449.0
66.80	108.0
68.00	3856.0
69.00	4302.0
70.00	263.0
72.00	235.0
73.00	1603.0
74.00	6278.0
75.00	19464.0
76.00	1687.0
77.00	224.0
78.00	186.0
78.90	1236.0
79.90	312.0
80.90	1196.0
81.90	293.0
87.00	1815.0
88.00	1599.0
90.90	129.0
92.10	994.0
93.00	1795.0
94.00	4588.0
95.00	39560.0
96.00	2682.0
103.80	162.0
105.90	165.0
116.00	157.0
116.90	240.0
117.80	140.0
118.90	209.0
127.80	167.0
129.80	142.0
140.90	302.0
142.90	491.0
144.80	167.0
154.90	124.0
171.90	505.0
173.90	34832.0
174.90	2701.0
175.90	33376.0
176.90	2268.0

Scan 3025 (10.316 min): VU023753.D
BFB51

m/z	Abundance
36.10	295.0
37.00	1551.0
38.00	1542.0
39.00	616.0
39.90	397.0
44.00	713.0
45.00	302.0
46.90	531.0
48.00	199.0
49.00	1419.0
50.00	6666.0
51.00	2132.0
56.00	513.0
57.00	880.0
60.00	289.0
61.00	1457.0
62.00	1711.0
63.00	1421.0
63.90	235.0
65.00	449.0
68.00	3506.0
69.00	3897.0
70.00	229.0
72.00	202.0
73.00	1499.0
74.00	5739.0
75.00	17816.0
76.00	1596.0
77.00	219.0
78.00	145.0
78.90	1141.0
79.90	269.0
80.90	988.0
81.90	282.0
87.00	1680.0
88.00	1489.0
90.90	103.0
92.10	958.0
93.00	1675.0
94.00	4311.0
95.00	36072.0
96.00	2411.0
103.80	143.0
105.90	164.0
116.00	170.0
116.90	231.0
117.80	131.0
118.80	195.0
127.80	148.0
129.80	126.0
140.90	323.0
142.80	490.0
144.80	153.0
154.90	111.0
171.90	557.0
173.90	32944.0
174.90	2460.0
175.90	31736.0
176.90	2084.0