

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU050923\  
 Data File : VU054133.D  
 Acq On : 09 May 2023 20:08  
 Operator : JC/MD  
 Sample : 02694-13  
 Misc : 5.0mL/MSVOA\_U/WATER  
 ALS Vial : 22 Sample Multiplier: 1

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 JREN5

Quant Time: May 10 04:36:30 2023  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMULM042923WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Sat May 06 01:14:00 2023  
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	6.244	114	216279	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.411	117	206405	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.806	152	108283	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	48603	29.713	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery =	59.420%#		
7) Chloroethane-d5	1.906	69	45152	42.052	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery =	84.100%		
11) 1,1-Dichloroethene-d2	2.562	63	76920	26.513	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery =	53.020%#		
21) 2-Butanone-d5	4.613	46	112387	120.468	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery =	120.470%		
24) Chloroform-d	5.057	84	132002	43.939	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery =	87.880%		
26) 1,2-Dichloroethane-d4	5.694	65	86575	44.883	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery =	89.760%		
32) Benzene-d6	5.719	84	244815	40.295	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery =	80.600%		
36) 1,2-Dichloropropane-d6	6.684	67	83407	43.487	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery =	86.980%		
41) Toluene-d8	7.893	98	218512	39.837	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery =	79.680%#		
43) trans-1,3-Dichloroprop...	8.173	79	40214	42.367	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery =	84.740%		
47) 2-Hexanone-d5	8.626	63	72299	105.243	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery =	105.240%		
56) 1,1,2,2-Tetrachloroeth...	10.751	84	126886	50.224	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery =	100.440%		
66) 1,2-Dichlorobenzene-d4	12.189	152	101751	48.101	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery =	96.200%		
Target Compounds						
13) Acetone	2.623	43	38695	42.258	ug/L	100
15) Methyl Acetate	2.945	43	17562	12.247	ug/L	93
22) 2-Butanone	4.703	43	20641	19.093	ug/L	99
33) Benzene	5.768	78	11845	1.972	ug/L	100
40) 4-Methyl-2-pentanone	7.790	43	12445	6.283	ug/L	98
42) Toluene	7.964	91	71872	11.491	ug/L	97
52) Ethylbenzene	9.565	91	14039	1.994	ug/L	96
53) m,p-Xylene	9.687	106	17569	6.647	ug/L	97
54) o-Xylene	10.096	106	10007	3.870	ug/L	89
63) 1,2,4-Trimethylbenzene	11.462	105	12523	2.268	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU050923\  
 Data File : VU054133.D  
 Acq On : 09 May 2023 20:08  
 Operator : JC/MD  
 Sample : 02694-13  
 Misc : 5.0mL/MSVOA\_U/WATER  
 ALS Vial : 22 Sample Multiplier: 1

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 JREN5


Quant Time: May 10 04:36:30 2023  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMULM042923WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Sat May 06 01:14:00 2023  
 Response via : Initial Calibration

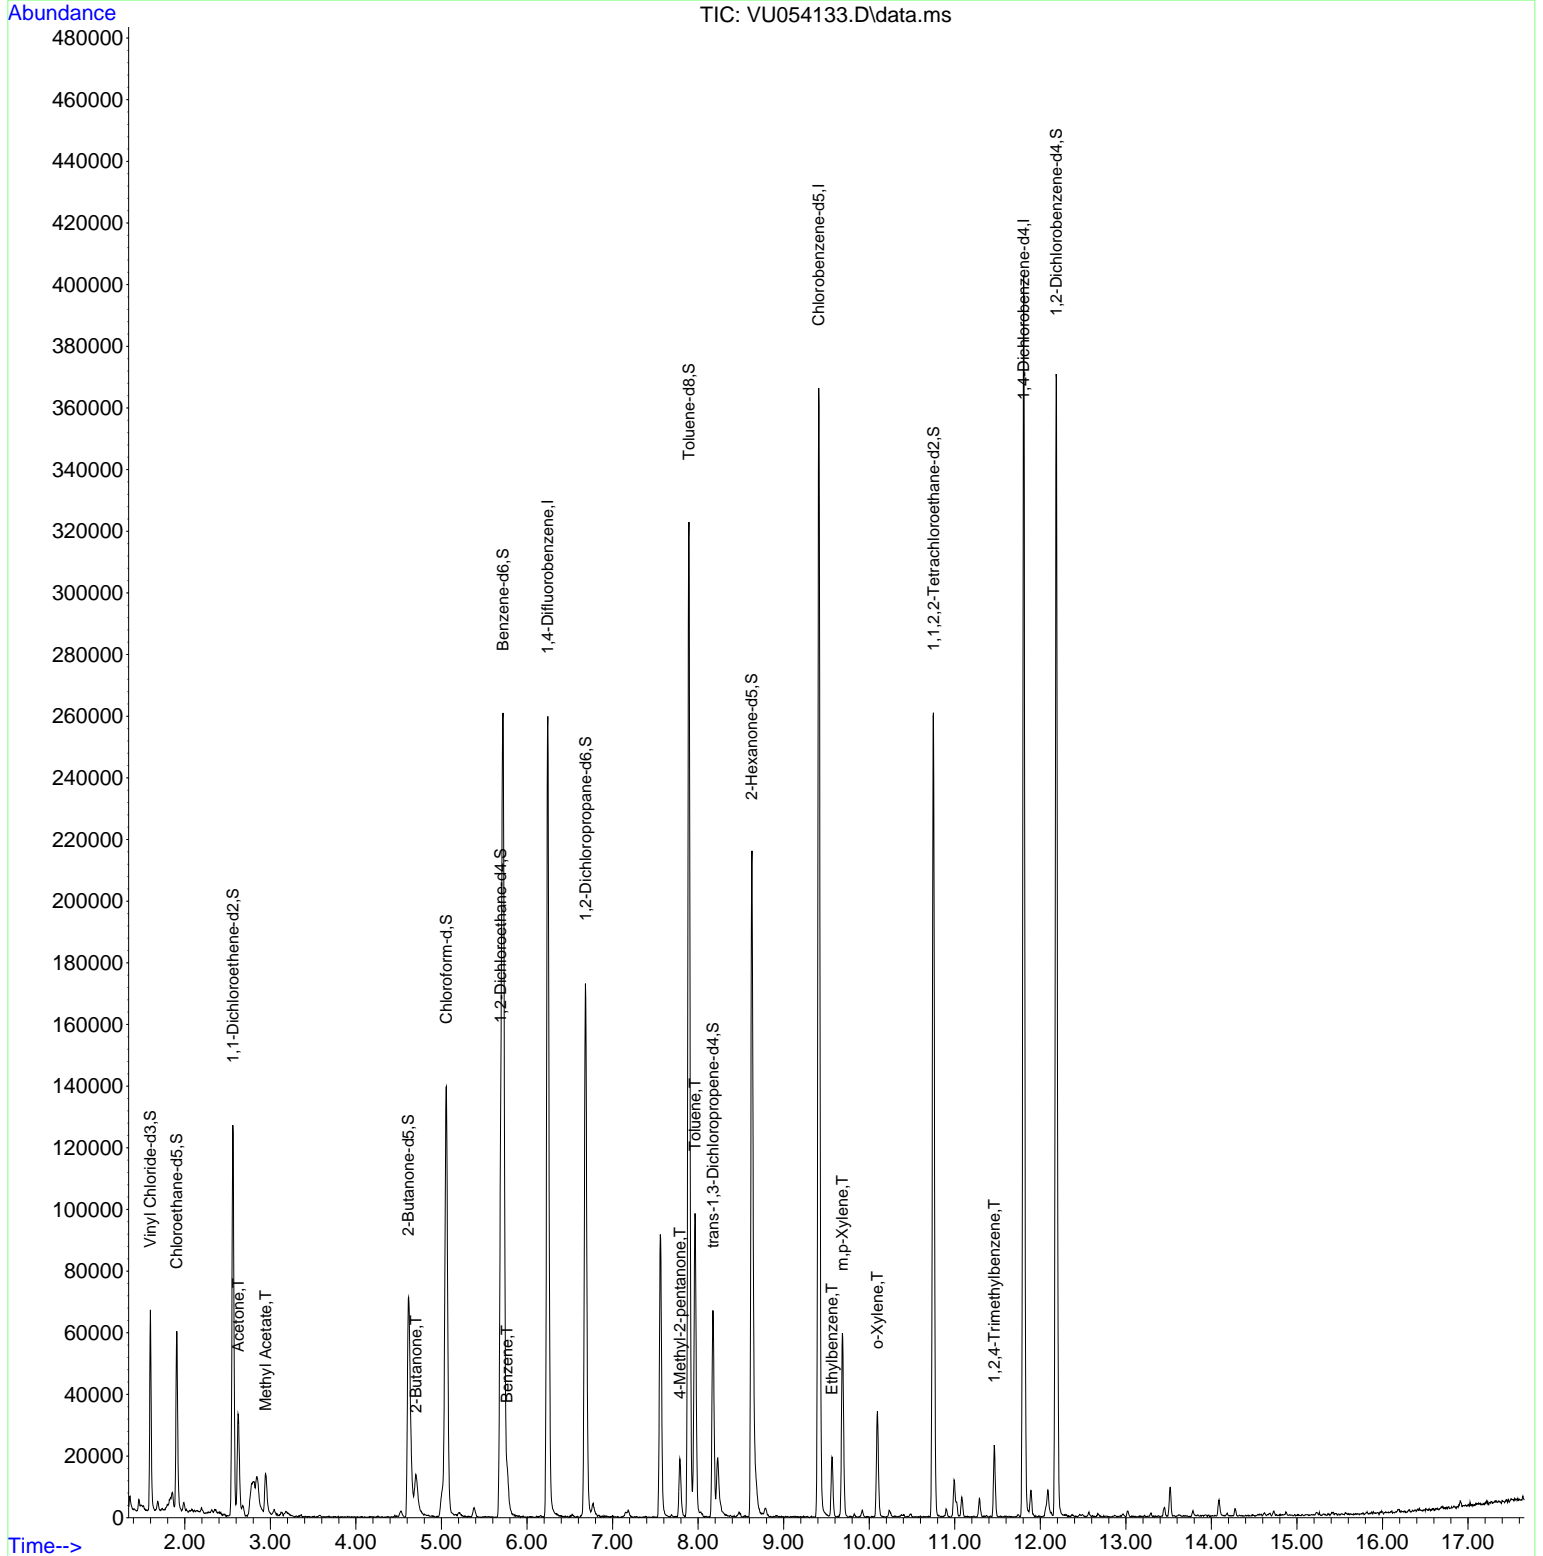



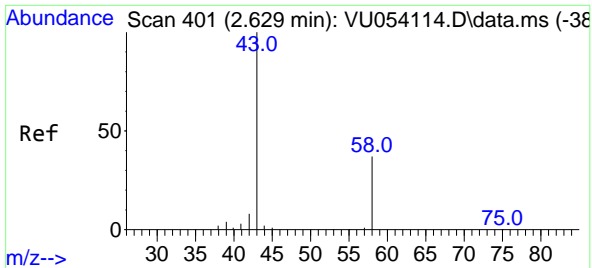


#13  
 Acetone  
 Concen: 42.258 ug/L  
 RT: 2.623 min Scan# 399  
 Delta R.T. -0.009 min  
 Lab File: VU054133.D  
 Acq: 09 May 2023 20:08


Instrument : MSVOA\_U  
 ClientSampleId : JREN5

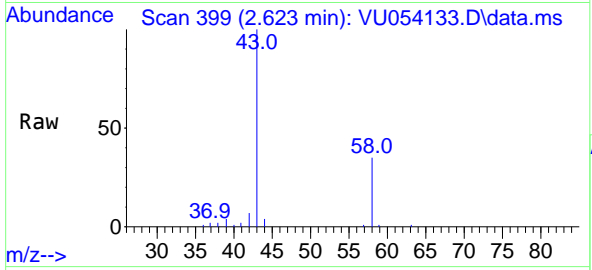



Tgt Ion: 43 Resp: 38695  
 Ion Ratio Lower Upper  
 43 100  
 58 33.6 0.0 67.4

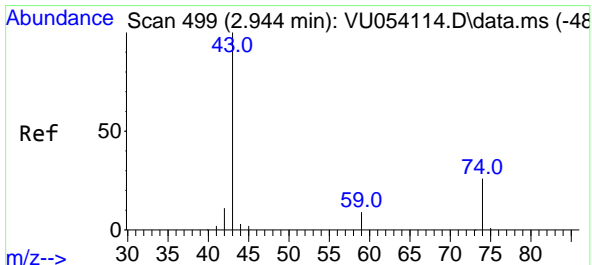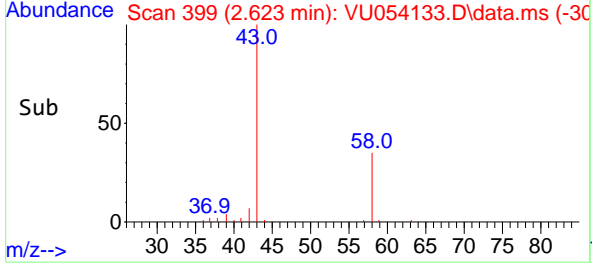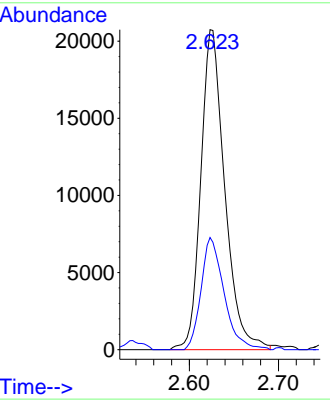


#15  
 Methyl Acetate  
 Concen: 12.247 ug/L  
 RT: 2.945 min Scan# 499  
 Delta R.T. -0.003 min  
 Lab File: VU054133.D  
 Acq: 09 May 2023 20:08

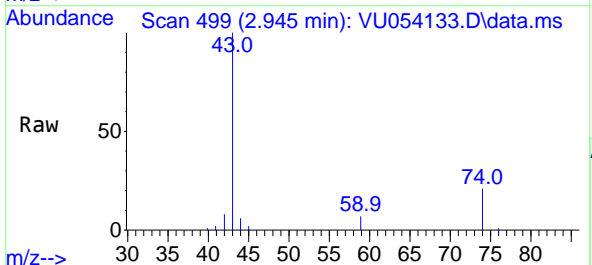

Tgt Ion: 43 Resp: 17562  
 Ion Ratio Lower Upper  
 43 100  
 74 23.1 21.2 31.8



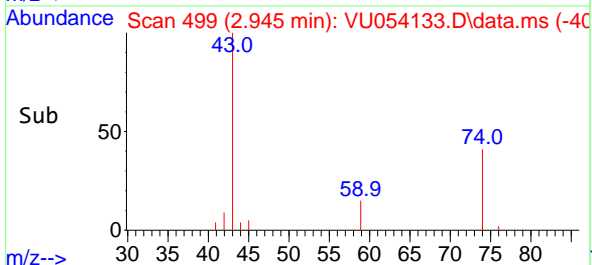
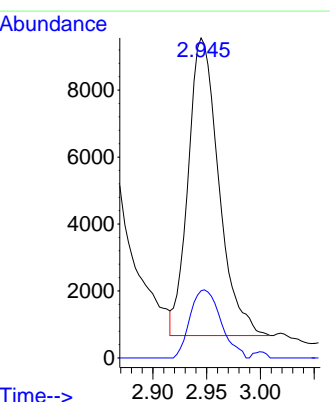


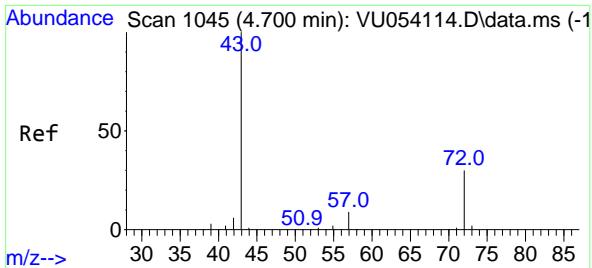

#22  
 2-Butanone  
 Concen: 19.093 ug/L  
 RT: 4.703 min Scan# 1046  
 Delta R.T. 0.000 min  
 Lab File: VU054133.D  
 Acq: 09 May 2023 20:08




Instrument : MSVOA\_U  
 ClientSampleId : JREN5


Tgt Ion: 43 Resp: 20641  
 Ion Ratio Lower Upper  
 43 100  
 72 28.2 14.0 41.9

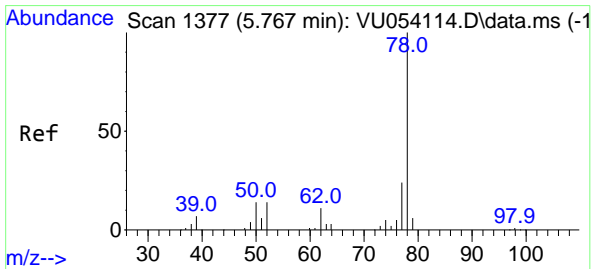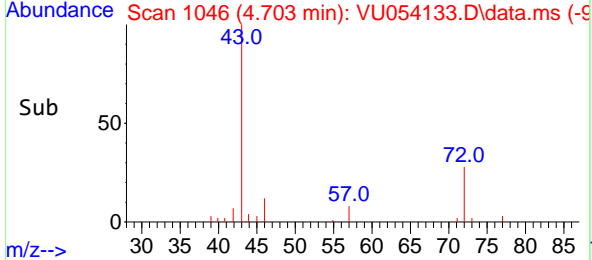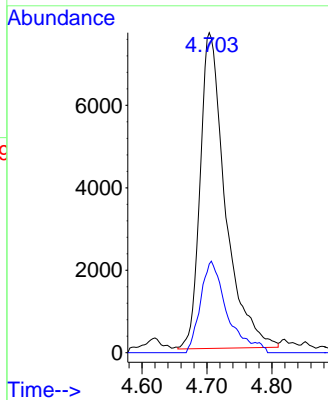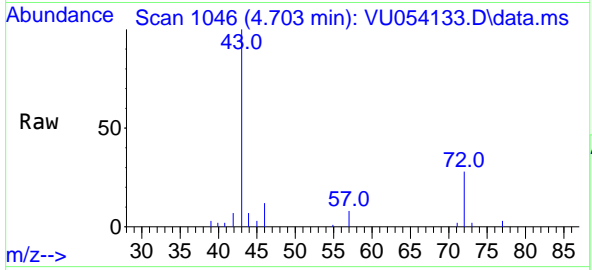

#33  
 Benzene  
 Concen: 1.972 ug/L  
 RT: 5.768 min Scan# 1377  
 Delta R.T. -0.003 min  
 Lab File: VU054133.D  
 Acq: 09 May 2023 20:08


Tgt Ion: 78 Resp: 11845

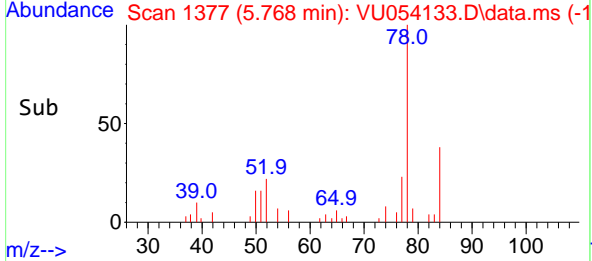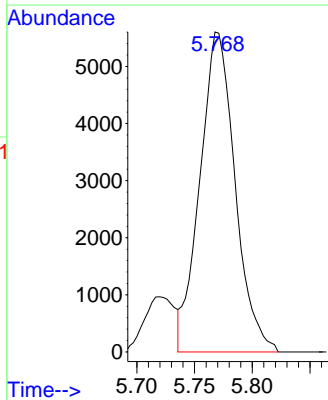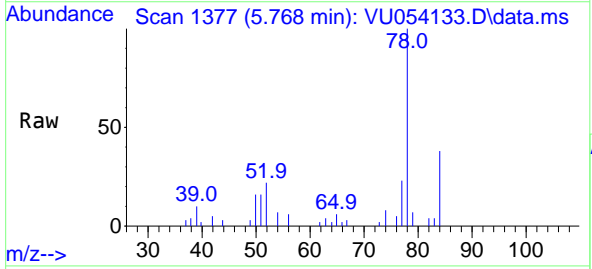

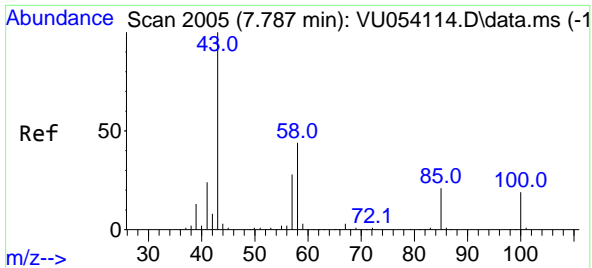




#40  
 4-Methyl-2-pentanone  
 Concen: 6.283 ug/L  
 RT: 7.790 min Scan# 2005  
 Delta R.T. 0.003 min  
 Lab File: VU054133.D  
 Acq: 09 May 2023 20:08

Instrument : MSVOA\_U  
 ClientSampleId : JREN5

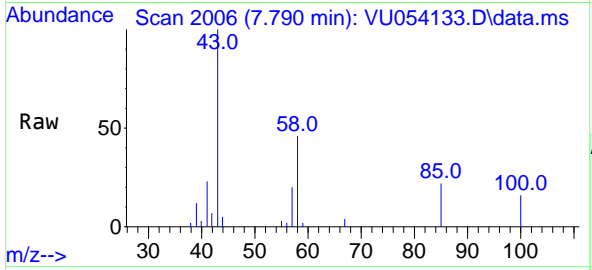

Tgt Ion: 43 Resp: 12445




Ion	Ratio	Lower	Upper
43	100		
58	43.9	34.5	51.7
100	15.6	13.8	20.6

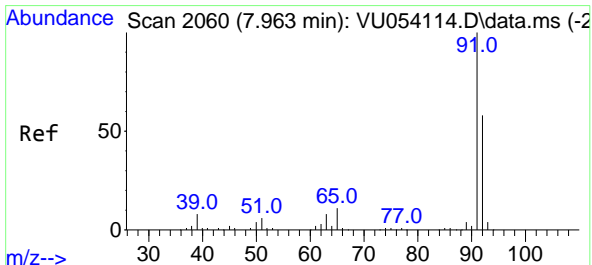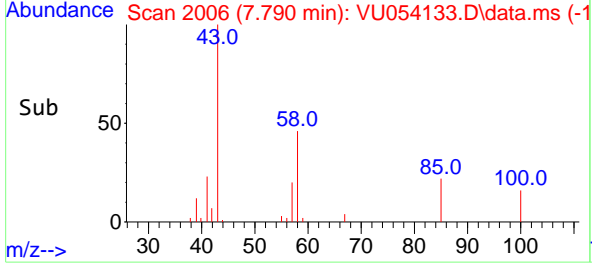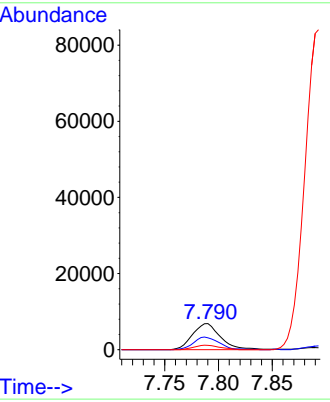


#42  
 Toluene  
 Concen: 11.491 ug/L  
 RT: 7.964 min Scan# 2060  
 Delta R.T. -0.003 min  
 Lab File: VU054133.D  
 Acq: 09 May 2023 20:08

Tgt Ion: 91 Resp: 71872

Ion	Ratio	Lower	Upper
91	100		
92	60.0	40.5	75.3


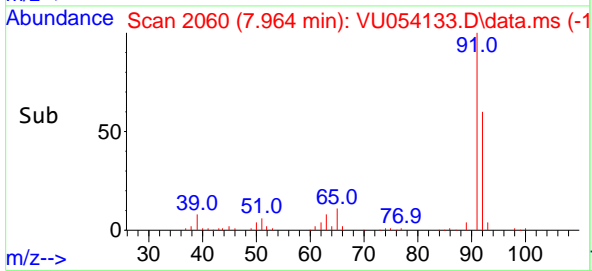
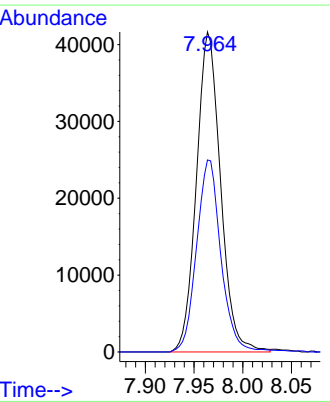
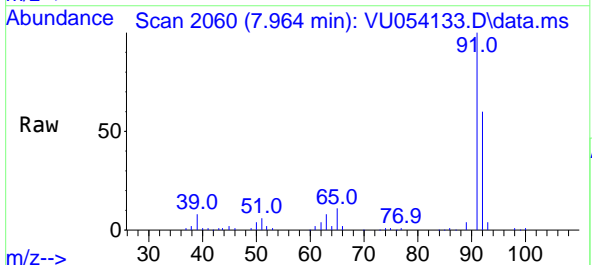


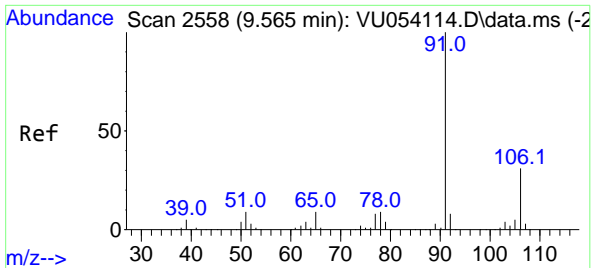

#52  
 Ethylbenzene  
 Concen: 1.994 ug/L  
 RT: 9.565 min Scan# 21  
 Delta R.T. 0.000 min  
 Lab File: VU054133.D  
 Acq: 09 May 2023 20:08




Instrument : MSVOA\_U  
 ClientSampleId : JREN5


Tgt Ion: 91 Resp: 14039  
 Ion Ratio Lower Upper  
 91 100  
 106 32.5 21.3 39.6

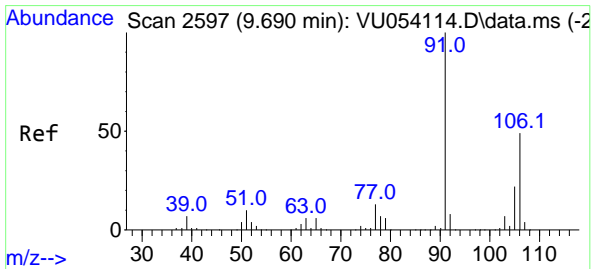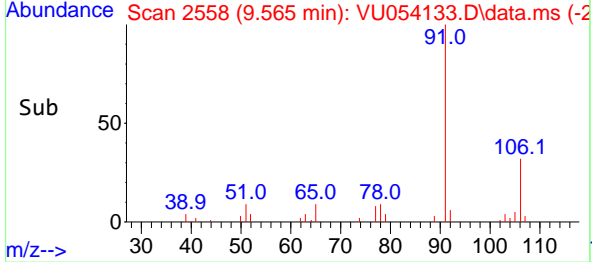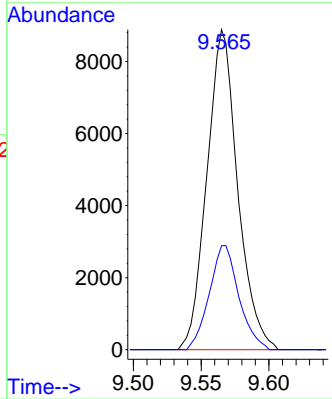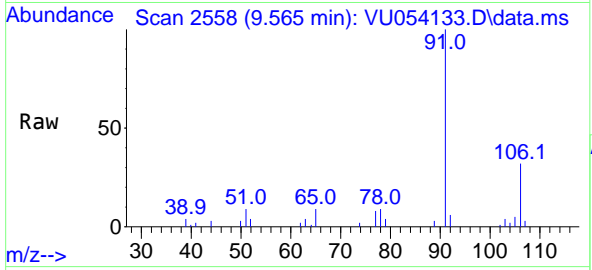

#53  
 m,p-Xylene  
 Concen: 6.647 ug/L  
 RT: 9.687 min Scan# 2596  
 Delta R.T. -0.003 min  
 Lab File: VU054133.D  
 Acq: 09 May 2023 20:08

Tgt Ion: 106 Resp: 17569  
 Ion Ratio Lower Upper  
 106 100  
 91 205.5 140.5 260.9


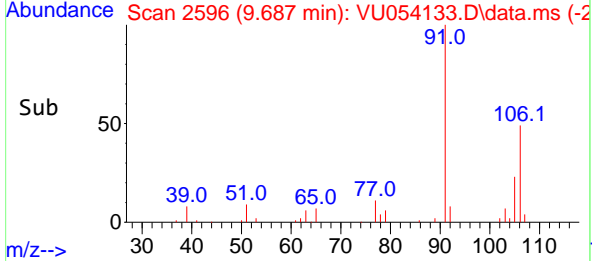
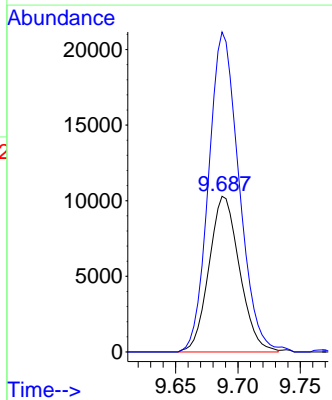
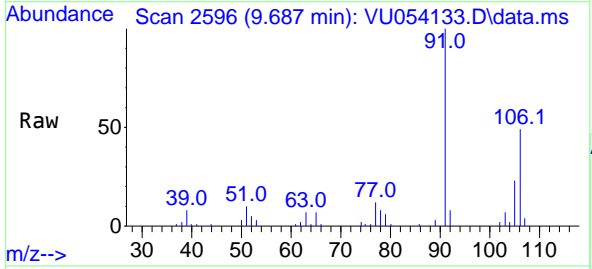


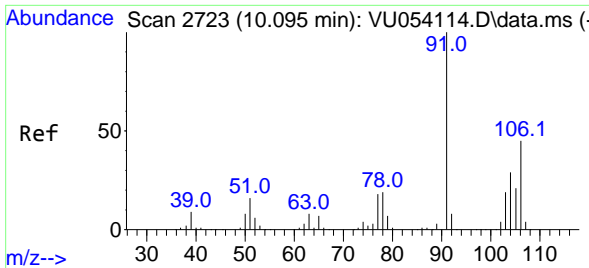

#54  
 o-Xylene  
 Concen: 3.870 ug/L  
 RT: 10.096 min Scan# 21  
 Delta R.T. 0.000 min  
 Lab File: VU054133.D  
 Acq: 09 May 2023 20:08

Instrument : MSVOA\_U  
 Client SampleId : JREN5

Tgt Ion:106 Resp: 10007  
 Ion Ratio Lower Upper  
 106 100  
 91 204.0 154.9 287.7

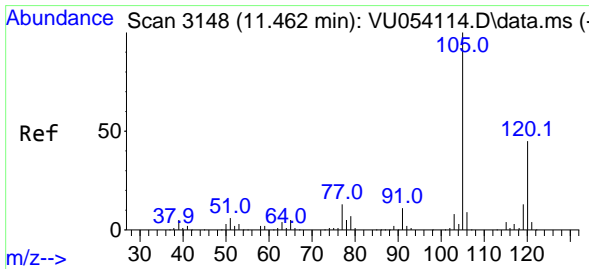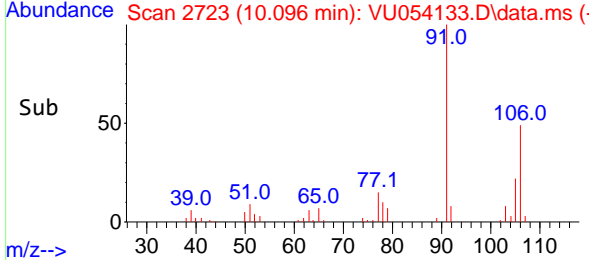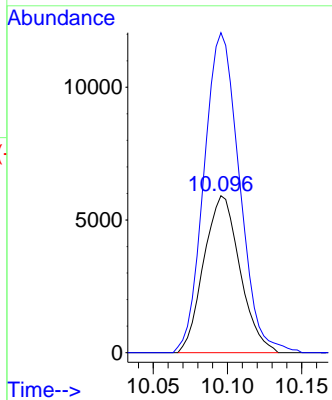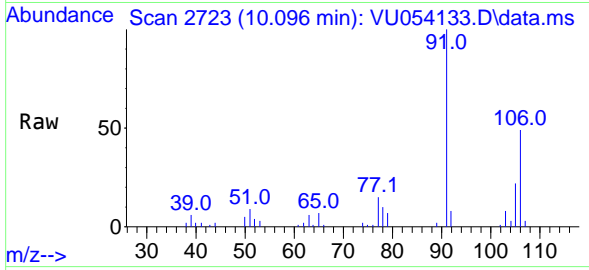

#63  
 1,2,4-Trimethylbenzene  
 Concen: 2.268 ug/L  
 RT: 11.462 min Scan# 3148  
 Delta R.T. 0.000 min  
 Lab File: VU054133.D  
 Acq: 09 May 2023 20:08

Tgt Ion:105 Resp: 12523  
 Ion Ratio Lower Upper  
 105 100  
 120 46.3 36.5 54.7

