

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050923\
 Data File : VU054125.D
 Acq On : 09 May 2023 17:00
 Operator : JC/MD
 Sample : 02694-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 JREL6

Quant Time: May 10 04:35:32 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat May 06 01:14:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.243	114	224575	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.411	117	215711	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.806	152	107624	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	56729	33.400	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	66.800%	
7) Chloroethane-d5	1.906	69	50138	44.970	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	89.940%	
11) 1,1-Dichloroethene-d2	2.562	63	87144	28.927	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	57.860%#	
21) 2-Butanone-d5	4.613	46	95796	98.890	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	98.890%	
24) Chloroform-d	5.054	84	137114	43.954	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	87.900%	
26) 1,2-Dichloroethane-d4	5.694	65	90233	45.051	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	90.100%	
32) Benzene-d6	5.719	84	256573	40.409	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	80.820%	
36) 1,2-Dichloropropane-d6	6.684	67	86039	42.924	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	85.840%	
41) Toluene-d8	7.893	98	230165	40.151	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	80.300%	
43) trans-1,3-Dichloroprop...	8.173	79	42096	42.437	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	84.880%	
47) 2-Hexanone-d5	8.626	63	62396	86.909	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	86.910%	
56) 1,1,2,2-Tetrachloroeth...	10.751	84	124147	47.020	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	94.040%	
66) 1,2-Dichlorobenzene-d4	12.189	152	100445	47.775	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	95.540%	
Target Compounds						
13) Acetone	2.629	43	2969	3.123	ug/L	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050923\
Data File : VU054125.D
Acq On : 09 May 2023 17:00
Operator : JC/MD
Sample : 02694-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
JREL6

Quant Time: May 10 04:35:32 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis
QLast Update : Sat May 06 01:14:00 2023
Response via : Initial Calibration

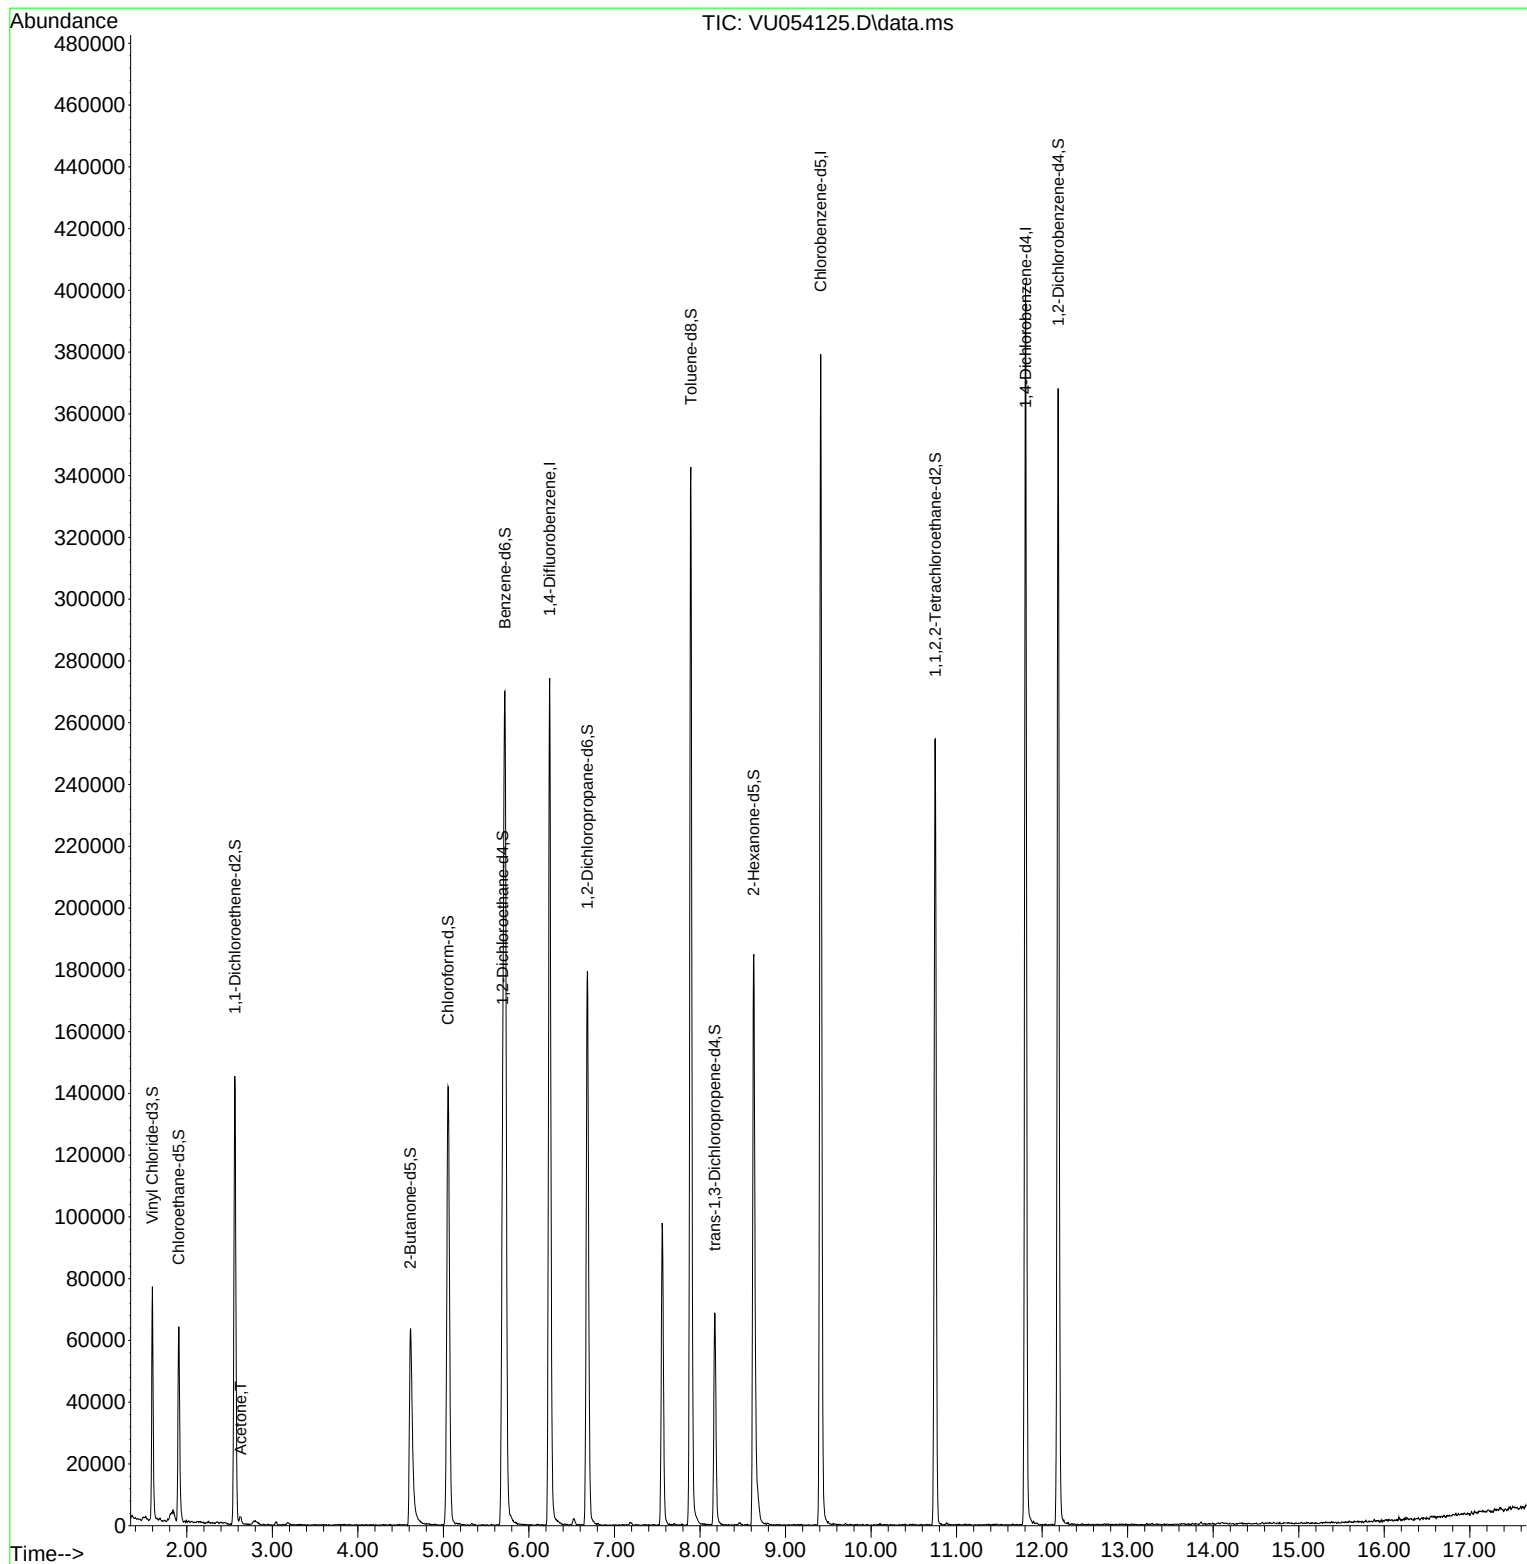

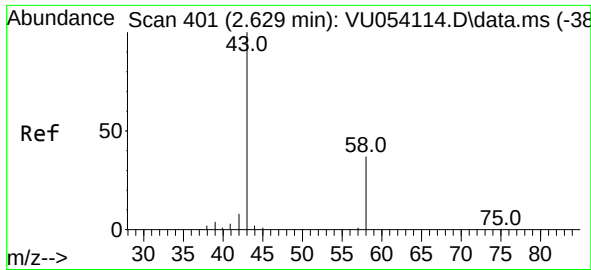

#13
 Acetone
 Concen: 3.123 ug/L
 RT: 2.629 min Scan# 401
 Delta R.T. -0.003 min
 Lab File: VU054125.D
 Acq: 09 May 2023 17:00

Instrument :
 MSVOA_U
 ClientSampleId :
 JREL6

Tgt Ion: 43 Resp: 2969
 Ion Ratio Lower Upper
 43 100
 58 36.1 0.0 67.4

