

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050923\
 Data File : VU054121.D
 Acq On : 09 May 2023 15:30
 Operator : JC/MD
 Sample : 02695-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

Signal : TIC: VU054121.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	97	rVB	86709	105232	12.84%	1.633%
2	1.909	169	177	194	rVB	70357	96850	11.81%	1.503%
3	2.562	368	380	396	rBV	162233	266235	32.48%	4.131%
4	2.678	413	416	420	rVB	654	405	0.05%	0.006%
5	2.700	420	423	424	rBV	390	238	0.03%	0.004%
6	2.732	431	433	434	rBV	190	82	0.01%	0.001%
7	2.742	434	436	438	rVB	294	118	0.01%	0.002%
8	2.774	439	446	448	rBV2	494	527	0.06%	0.008%
9	2.961	502	504	507	rBV	268	159	0.02%	0.002%
10	3.009	514	519	521	rBV2	216	196	0.02%	0.003%
11	3.041	524	529	530	rBV2	742	620	0.08%	0.010%
12	3.176	565	571	575	rBV2	867	1207	0.15%	0.019%
13	3.324	614	617	620	rBV	269	203	0.02%	0.003%
14	3.533	679	682	688	rVB	243	160	0.02%	0.002%
15	3.562	688	691	692	rBV	203	139	0.02%	0.002%
16	3.729	741	743	746	rBV	148	116	0.01%	0.002%
17	3.755	749	751	752	rBV	172	54	0.01%	0.001%
18	3.871	786	787	788	rBV	117	30	0.00%	0.000%
19	3.973	816	819	821	rBV	205	106	0.01%	0.002%
20	4.108	858	861	865	rBB	216	157	0.02%	0.002%
21	4.227	896	898	900	rBV	173	71	0.01%	0.001%
22	4.308	921	923	928	rVB2	207	121	0.01%	0.002%
23	4.353	934	937	940	rBV	148	95	0.01%	0.001%
24	4.375	940	944	946	rBV	190	163	0.02%	0.003%
25	4.498	979	982	986	rVB	322	249	0.03%	0.004%
26	4.520	986	989	990	rBV	237	122	0.01%	0.002%
27	4.543	993	996	999	rVV	164	98	0.01%	0.002%
28	4.620	1009	1020	1051	rBV	67414	171583	20.93%	2.662%
29	4.951	1121	1123	1125	rVB	167	69	0.01%	0.001%
30	4.964	1125	1127	1130	rBV	171	84	0.01%	0.001%
31	5.057	1140	1156	1177	rBV	154988	343124	41.86%	5.323%
32	5.289	1226	1228	1234	rVB	361	328	0.04%	0.005%
33	5.327	1236	1240	1247	rVV4	526	713	0.09%	0.011%
34	5.456	1277	1280	1282	rBV	165	138	0.02%	0.002%
35	5.485	1288	1289	1290	rBB	62	29	0.00%	0.000%
36	5.530	1302	1303	1304	rVB	124	24	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050923\
 Data File : VU054121.D
 Acq On : 09 May 2023 15:30
 Operator : JC/MD
 Sample : 02695-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

37	5.575	1314	1317	1318	rBV	174	104	0.01%	0.002%
38	5.636	1334	1336	1338	rBV	150	79	0.01%	0.001%
39	5.719	1341	1362	1386	rBV2	297626	819745	100.00%	12.718%
40	6.038	1458	1461	1464	rBV	396	219	0.03%	0.003%
41	6.067	1468	1470	1474	rVB2	177	109	0.01%	0.002%
42	6.128	1486	1489	1491	rBV	163	104	0.01%	0.002%
43	6.153	1495	1497	1499	rVB	153	64	0.01%	0.001%
44	6.243	1511	1525	1559	rBV	278752	537757	65.60%	8.343%
45	6.481	1597	1599	1601	rBV2	199	70	0.01%	0.001%
46	6.530	1607	1614	1623	rVB2	2560	3905	0.48%	0.061%
47	6.684	1649	1662	1690	rBV	194431	378017	46.11%	5.865%
48	6.851	1711	1714	1716	rBV	182	116	0.01%	0.002%
49	6.906	1727	1731	1735	rVB2	240	232	0.03%	0.004%
50	6.941	1740	1742	1747	rVB2	152	95	0.01%	0.001%
51	6.977	1750	1753	1755	rVB	274	166	0.02%	0.003%
52	6.993	1755	1758	1760	rBV2	153	92	0.01%	0.001%
53	7.015	1764	1765	1767	rVB2	243	67	0.01%	0.001%
54	7.034	1767	1771	1772	rBV2	256	154	0.02%	0.002%
55	7.086	1784	1787	1789	rBV	210	117	0.01%	0.002%
56	7.227	1829	1831	1833	rBV	168	61	0.01%	0.001%
57	7.243	1833	1836	1837	rBV	222	112	0.01%	0.002%
58	7.279	1844	1847	1851	rBV2	192	139	0.02%	0.002%
59	7.369	1872	1875	1876	rBV	315	180	0.02%	0.003%
60	7.472	1902	1907	1909	rBV	327	326	0.04%	0.005%
61	7.562	1922	1935	1955	rBV	106986	187749	22.90%	2.913%
62	7.790	2003	2006	2008	rBV2	326	211	0.03%	0.003%
63	7.893	2024	2038	2063	rBV	370866	642326	78.36%	9.966%
64	8.176	2115	2126	2141	rBV	74192	126538	15.44%	1.963%
65	8.404	2195	2197	2199	rBV	211	83	0.01%	0.001%
66	8.468	2211	2217	2227	rVB4	2061	2630	0.32%	0.041%
67	8.552	2239	2243	2245	rBV	353	248	0.03%	0.004%
68	8.629	2255	2267	2305	rBV2	192073	377252	46.02%	5.853%
69	9.356	2491	2493	2495	rBV	163	69	0.01%	0.001%
70	9.411	2498	2510	2534	rBV	378538	646246	78.84%	10.026%
71	9.552	2551	2554	2556	rBV2	471	265	0.03%	0.004%
72	9.629	2575	2578	2581	rBV	252	191	0.02%	0.003%
73	9.687	2592	2596	2597	rBV2	380	232	0.03%	0.004%
74	9.748	2612	2615	2619	rVB2	213	156	0.02%	0.002%
75	9.767	2619	2621	2625	rBV2	161	125	0.02%	0.002%
76	9.919	2664	2668	2674	rBV2	331	324	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050923\
 Data File : VU054121.D
 Acq On : 09 May 2023 15:30
 Operator : JC/MD
 Sample : 02695-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

77	10.047	2706	2708	2709	rBV	149	40	0.00%	0.001%
78	10.092	2721	2722	2723	rBV	206	68	0.01%	0.001%
79	10.295	2782	2785	2789	rVB	287	197	0.02%	0.003%
80	10.751	2914	2927	2950	rBV	269975	432489	52.76%	6.710%
81	10.886	2963	2969	2980	rVB4	1573	2104	0.26%	0.033%
82	11.021	3008	3011	3015	rBV	322	229	0.03%	0.004%
83	11.057	3018	3022	3024	rBV2	208	174	0.02%	0.003%
84	11.173	3056	3058	3062	rVB	183	61	0.01%	0.001%
85	11.465	3147	3149	3151	rBV2	391	259	0.03%	0.004%
86	11.745	3231	3236	3241	rBV4	580	540	0.07%	0.008%
87	11.806	3243	3255	3279	rBV	408641	644856	78.67%	10.005%
88	12.066	3326	3336	3354	rBV5	6082	16126	1.97%	0.250%
89	12.189	3362	3374	3400	rVB	384950	629159	76.75%	9.761%
90	12.520	3475	3477	3478	rBV	234	90	0.01%	0.001%
91	12.751	3546	3549	3551	rBV	379	221	0.03%	0.003%
92	12.893	3588	3593	3601	rBV5	919	1334	0.16%	0.021%
93	13.407	3750	3753	3757	rBV2	470	336	0.04%	0.005%
94	13.713	3844	3848	3855	rBV3	537	688	0.08%	0.011%




Sum of corrected areas: 6445491

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050923\
Data File : VU054121.D
Acq On : 09 May 2023 15:30
Operator : JC/MD
Sample : 02695-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

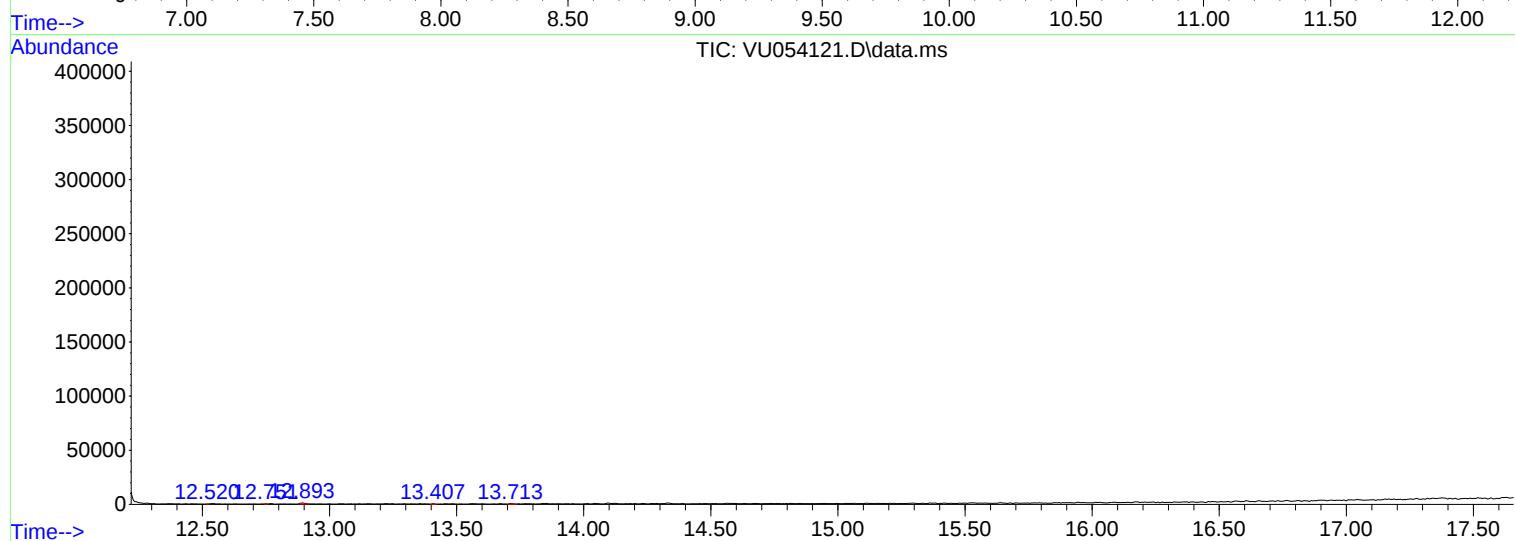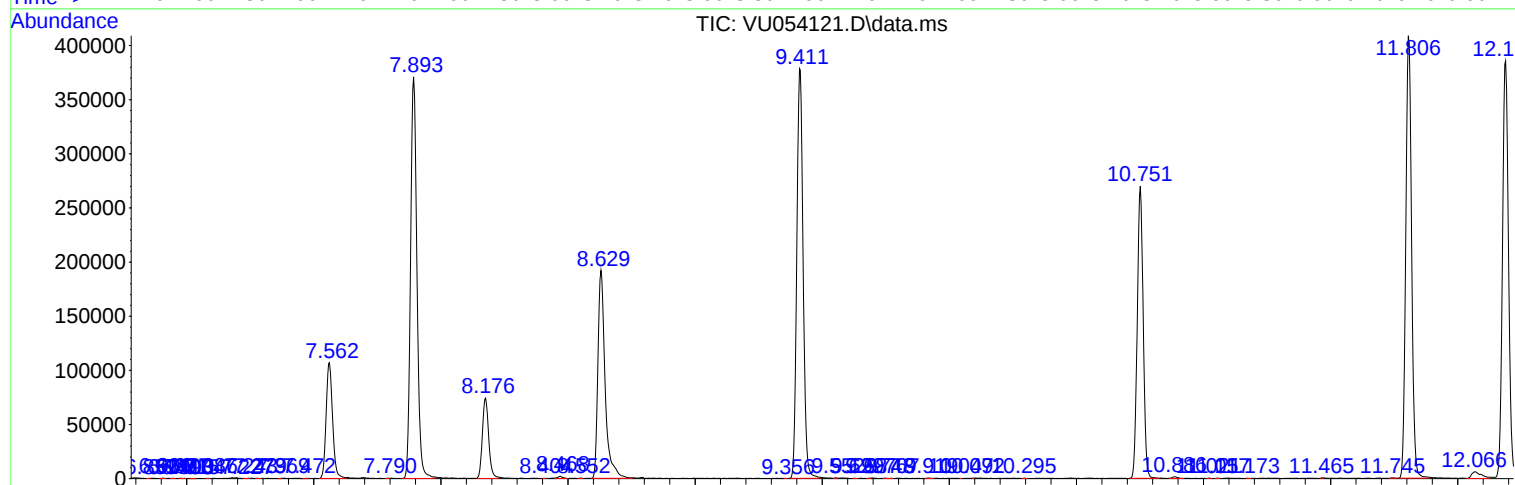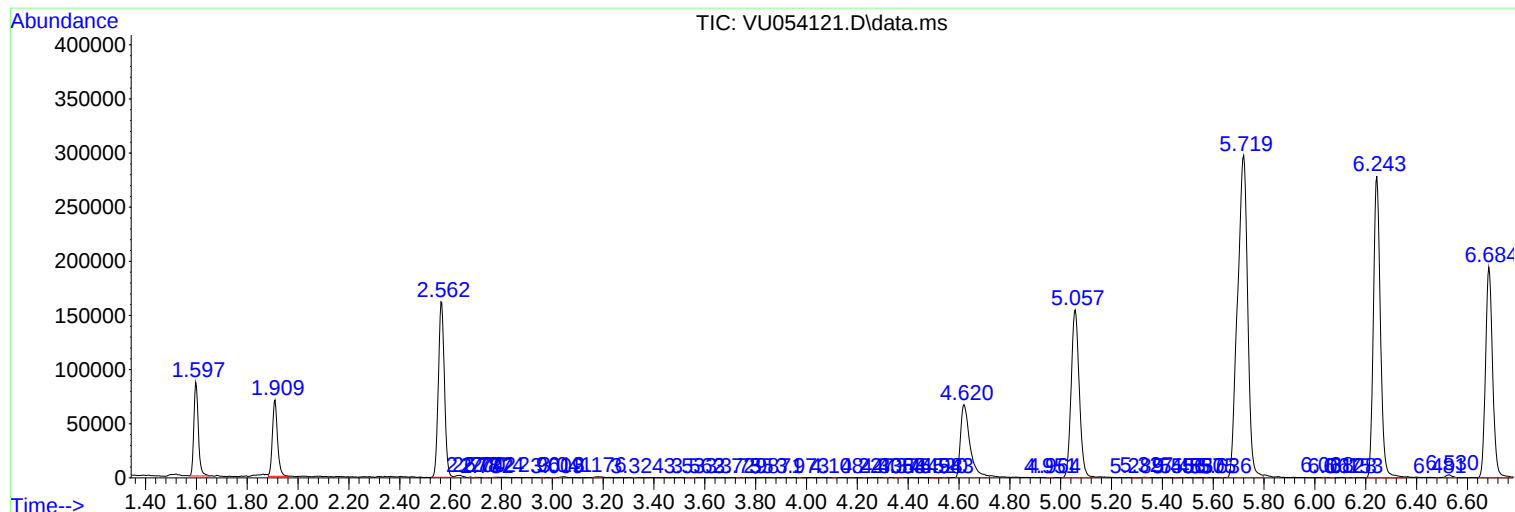

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050923\
Data File : VU054121.D
Acq On : 09 May 2023 15:30
Operator : JC/MD
Sample : 02695-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050923\
Data File : VU054121.D
Acq On : 09 May 2023 15:30
Operator : JC/MD
Sample : 02695-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------