

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050923\
 Data File : VU054122.D
 Acq On : 09 May 2023 15:53
 Operator : JC/MD
 Sample : 02694-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 JREL3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

Signal : TIC: VU054122.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	94	rBV	78248	94223	12.29%	1.548%
2	1.909	169	177	194	rVB	66498	93958	12.26%	1.544%
3	2.562	368	380	395	rBV	146972	243440	31.76%	4.001%
4	2.716	425	428	432	rBV2	345	307	0.04%	0.005%
5	3.038	523	528	530	rBV4	1010	974	0.13%	0.016%
6	3.118	550	553	559	rVB	207	184	0.02%	0.003%
7	3.182	562	573	583	rBV2	2188	4752	0.62%	0.078%
8	3.314	612	614	617	rBV	176	50	0.01%	0.001%
9	3.346	622	624	625	rBV	165	72	0.01%	0.001%
10	3.359	625	628	633	rVB	358	262	0.03%	0.004%
11	3.517	675	677	679	rVB	184	75	0.01%	0.001%
12	3.539	683	684	685	rBV	127	36	0.00%	0.001%
13	3.668	722	724	725	rBV	169	92	0.01%	0.002%
14	3.716	737	739	741	rBV	209	135	0.02%	0.002%
15	3.864	784	785	787	rVB	246	71	0.01%	0.001%
16	3.912	797	800	804	rBV2	194	160	0.02%	0.003%
17	3.938	805	808	811	rVV2	223	157	0.02%	0.003%
18	4.060	843	846	847	rBV	267	153	0.02%	0.003%
19	4.199	886	889	892	rBV2	205	143	0.02%	0.002%
20	4.234	896	900	903	rBV2	224	220	0.03%	0.004%
21	4.269	909	911	912	rBV2	148	64	0.01%	0.001%
22	4.372	938	943	946	rBV2	342	366	0.05%	0.006%
23	4.472	970	974	976	rVB	290	207	0.03%	0.003%
24	4.491	976	980	985	rBV	384	456	0.06%	0.007%
25	4.536	992	994	996	rVB2	140	72	0.01%	0.001%
26	4.552	996	999	1002	rBV2	247	186	0.02%	0.003%
27	4.616	1007	1019	1052	rBV	63648	164067	21.41%	2.696%
28	5.057	1140	1156	1179	rBV	142618	314753	41.07%	5.172%
29	5.379	1253	1256	1259	rBV	378	309	0.04%	0.005%
30	5.472	1283	1285	1287	rVB	138	60	0.01%	0.001%
31	5.501	1292	1294	1297	rBV	303	222	0.03%	0.004%
32	5.514	1297	1298	1301	rVB	206	72	0.01%	0.001%
33	5.552	1306	1310	1314	rBV	210	260	0.03%	0.004%
34	5.600	1323	1325	1326	rBV	138	36	0.00%	0.001%
35	5.719	1339	1362	1391	rBV2	277954	766397	100.00%	12.594%
36	5.970	1437	1440	1442	rBV2	159	102	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050923\
 Data File : VU054122.D
 Acq On : 09 May 2023 15:53
 Operator : JC/MD
 Sample : 02694-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 JREL3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

37	6.012	1451	1453	1459	rVB2	398	379	0.05%	0.006%
38	6.044	1459	1463	1465	rBV2	318	271	0.04%	0.004%
39	6.083	1473	1475	1477	rBV	160	110	0.01%	0.002%
40	6.115	1483	1485	1487	rBV	258	147	0.02%	0.002%
41	6.166	1497	1501	1504	rBV2	435	354	0.05%	0.006%
42	6.243	1510	1525	1546	rBV	268856	515570	67.27%	8.473%
43	6.385	1566	1569	1576	rBV2	496	510	0.07%	0.008%
44	6.462	1592	1593	1594	rVB2	95	18	0.00%	0.000%
45	6.475	1594	1597	1598	rBV	122	69	0.01%	0.001%
46	6.526	1606	1613	1622	rVB7	2281	4229	0.55%	0.069%
47	6.571	1625	1627	1629	rBV	154	85	0.01%	0.001%
48	6.620	1639	1642	1646	rBV	427	273	0.04%	0.004%
49	6.684	1648	1662	1684	rBV2	177627	354776	46.29%	5.830%
50	6.880	1721	1723	1725	rBV	166	117	0.02%	0.002%
51	6.896	1725	1728	1730	rVV	289	187	0.02%	0.003%
52	6.935	1737	1740	1742	rBV	188	153	0.02%	0.003%
53	6.986	1755	1756	1759	rVB	162	60	0.01%	0.001%
54	7.005	1759	1762	1763	rBV	141	90	0.01%	0.001%
55	7.086	1784	1787	1788	rBV	124	79	0.01%	0.001%
56	7.192	1812	1820	1827	rVV5	761	1147	0.15%	0.019%
57	7.221	1827	1829	1834	rVB2	250	170	0.02%	0.003%
58	7.266	1840	1843	1847	rVB2	324	236	0.03%	0.004%
59	7.311	1855	1857	1859	rVV	166	69	0.01%	0.001%
60	7.327	1859	1862	1865	rVB	261	192	0.03%	0.003%
61	7.362	1870	1873	1879	rBV2	194	229	0.03%	0.004%
62	7.562	1922	1935	1952	rBV	98070	172327	22.49%	2.832%
63	7.706	1973	1980	1985	rBV4	584	784	0.10%	0.013%
64	7.838	2017	2021	2022	rBV4	280	206	0.03%	0.003%
65	7.893	2025	2038	2056	rBV	349587	600004	78.29%	9.860%
66	8.176	2114	2126	2143	rBV	70174	120280	15.69%	1.977%
67	8.304	2164	2166	2167	rBV	167	54	0.01%	0.001%
68	8.423	2201	2203	2207	rBV	199	109	0.01%	0.002%
69	8.465	2207	2216	2223	rBV3	1152	1877	0.24%	0.031%
70	8.546	2237	2241	2252	rBV3	580	926	0.12%	0.015%
71	8.629	2255	2267	2302	rVV2	182039	356454	46.51%	5.858%
72	8.951	2364	2367	2368	rBV	186	80	0.01%	0.001%
73	8.980	2373	2376	2379	rVB	178	102	0.01%	0.002%
74	9.047	2394	2397	2400	rBV2	321	228	0.03%	0.004%
75	9.224	2450	2452	2455	rBB	145	40	0.01%	0.001%
76	9.411	2498	2510	2530	rBV	375792	628596	82.02%	10.330%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050923\
 Data File : VU054122.D
 Acq On : 09 May 2023 15:53
 Operator : JC/MD
 Sample : 02694-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 JREL3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

77	9.687	2592	2596	2604	rBV2	454	532	0.07%	0.009%
78	9.764	2615	2620	2623	rBV2	279	221	0.03%	0.004%
79	9.902	2660	2663	2665	rBV2	244	163	0.02%	0.003%
80	9.947	2674	2677	2680	rBV	204	104	0.01%	0.002%
81	10.083	2716	2719	2721	rBV	179	125	0.02%	0.002%
82	10.227	2763	2764	2767	rBV	154	94	0.01%	0.002%
83	10.340	2796	2799	2801	rBV	242	123	0.02%	0.002%
84	10.365	2805	2807	2812	rVB2	213	137	0.02%	0.002%
85	10.391	2813	2815	2818	rVB	258	119	0.02%	0.002%
86	10.407	2818	2820	2824	rBV	223	105	0.01%	0.002%
87	10.430	2824	2827	2833	rBV2	265	289	0.04%	0.005%
88	10.751	2914	2927	2945	rBV	250612	408298	53.27%	6.710%
89	11.066	3021	3025	3028	rBV2	312	216	0.03%	0.004%
90	11.086	3028	3031	3034	rVV2	395	250	0.03%	0.004%
91	11.806	3243	3255	3280	rBV	388785	626305	81.72%	10.292%
92	12.057	3331	3333	3335	rBV2	283	120	0.02%	0.002%
93	12.076	3337	3339	3341	rBV2	347	180	0.02%	0.003%
94	12.189	3361	3374	3401	rBV	370736	598416	78.08%	9.834%
95	13.227	3693	3697	3705	rBV3	588	586	0.08%	0.010%
96	13.902	3906	3907	3910	rBV	267	151	0.02%	0.002%




Sum of corrected areas: 6085214

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050923\
Data File : VU054122.D
Acq On : 09 May 2023 15:53
Operator : JC/MD
Sample : 02694-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
JREL3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

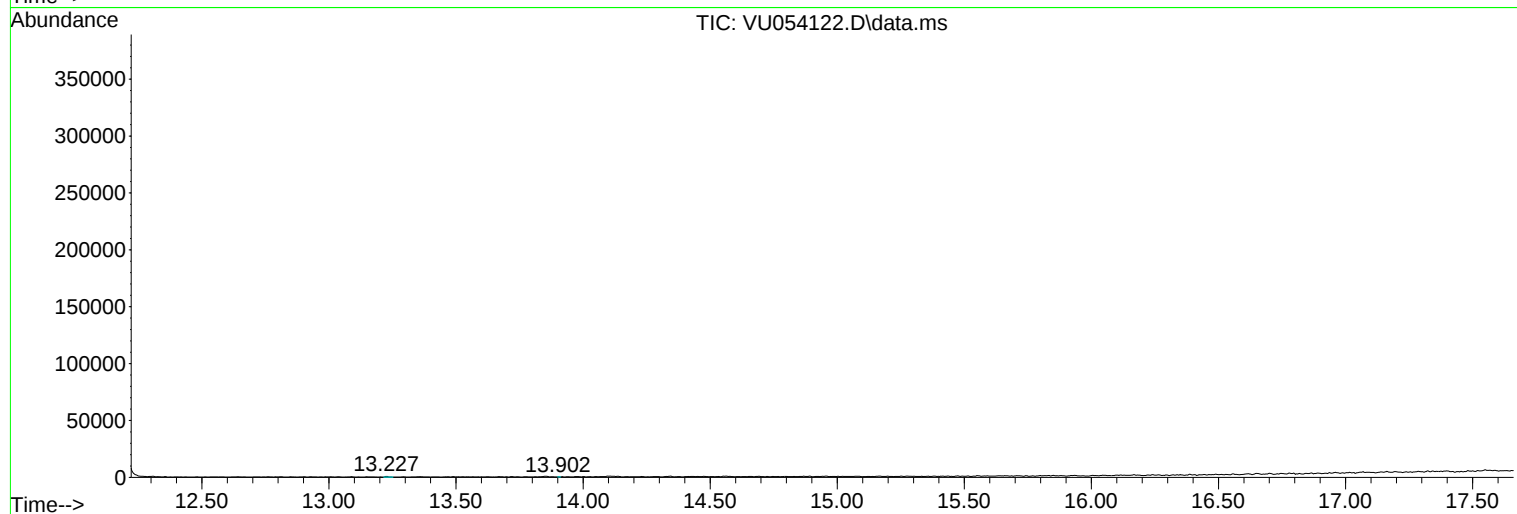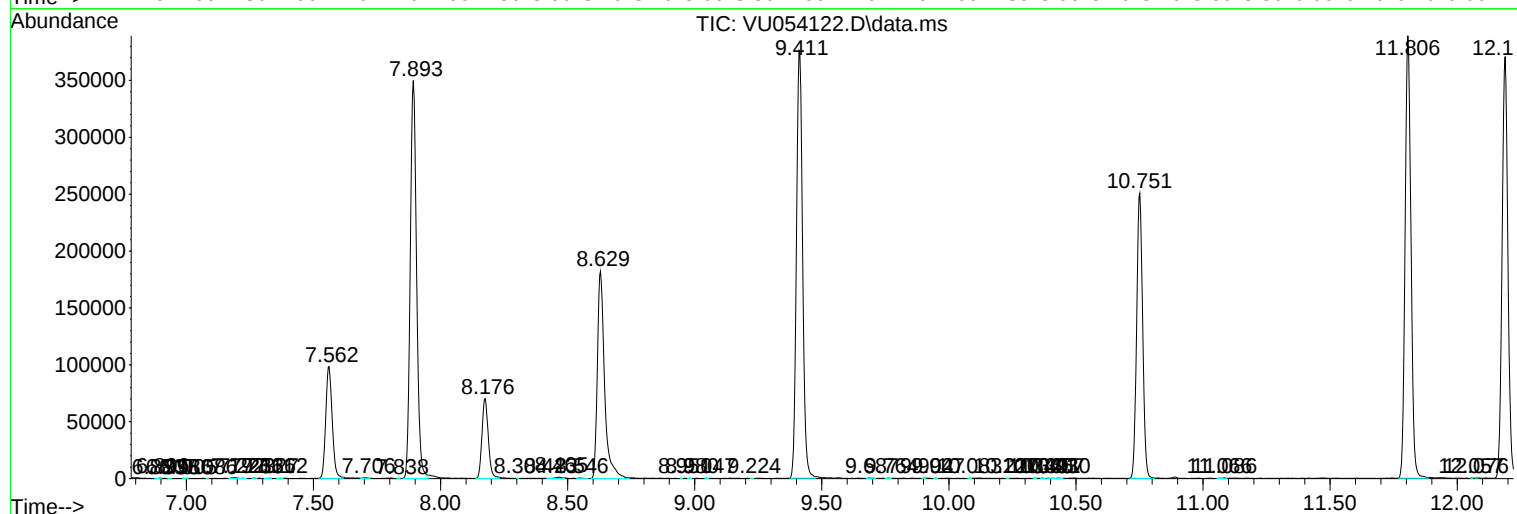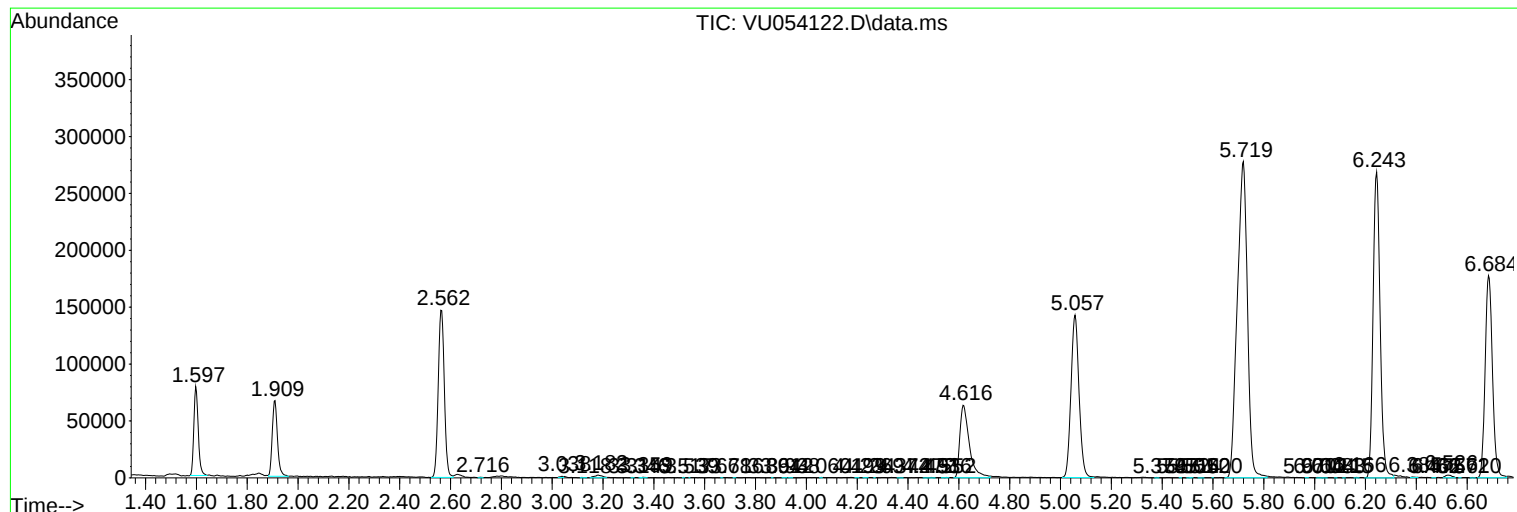

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050923\
Data File : VU054122.D
Acq On : 09 May 2023 15:53
Operator : JC/MD
Sample : 02694-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
JREL3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050923\
Data File : VU054122.D
Acq On : 09 May 2023 15:53
Operator : JC/MD
Sample : 02694-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
JREL3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc