

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050923\
 Data File : VU054125.D
 Acq On : 09 May 2023 17:00
 Operator : JC/MD
 Sample : 02694-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 JREL6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M

Title : VOC Analysis

Signal : TIC: VU054125.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	94	rVB	75087	88274	11.72%	1.460%
2	1.906	168	176	193	rVB	63299	90388	12.00%	1.495%
3	2.562	368	380	394	rBV	145107	233618	31.02%	3.863%
4	3.041	523	529	536	rBV3	1066	1520	0.20%	0.025%
5	3.118	550	553	556	rBV	249	196	0.03%	0.003%
6	3.234	587	589	592	rBV	151	63	0.01%	0.001%
7	3.311	611	613	615	rVB2	254	100	0.01%	0.002%
8	3.417	641	646	651	rVB2	230	266	0.04%	0.004%
9	3.559	687	690	693	rVB	222	152	0.02%	0.003%
10	3.774	752	757	761	rBV2	273	293	0.04%	0.005%
11	3.838	775	777	779	rVB	183	52	0.01%	0.001%
12	3.890	789	793	796	rBV	297	311	0.04%	0.005%
13	3.919	800	802	805	rVB	153	52	0.01%	0.001%
14	4.047	837	842	846	rBV2	256	261	0.03%	0.004%
15	4.092	854	856	859	rVB	209	112	0.01%	0.002%
16	4.109	859	861	863	rBV	186	103	0.01%	0.002%
17	4.160	875	877	880	rBV2	172	98	0.01%	0.002%
18	4.202	887	890	891	rBV	168	100	0.01%	0.002%
19	4.211	891	893	896	rVB2	145	90	0.01%	0.001%
20	4.253	903	906	909	rVB	197	111	0.01%	0.002%
21	4.311	923	924	925	rBV	124	41	0.01%	0.001%
22	4.372	939	943	947	rVB2	233	208	0.03%	0.003%
23	4.491	977	980	985	rBV	226	135	0.02%	0.002%
24	4.617	1008	1019	1054	rBV2	63829	161934	21.50%	2.677%
25	4.977	1129	1131	1134	rVB	221	90	0.01%	0.001%
26	5.054	1140	1155	1182	rBV	141879	315272	41.86%	5.213%
27	5.330	1233	1241	1249	rBV3	758	1377	0.18%	0.023%
28	5.369	1250	1253	1259	rVB	256	237	0.03%	0.004%
29	5.449	1276	1278	1280	rBV	174	54	0.01%	0.001%
30	5.533	1302	1304	1306	rBV	188	128	0.02%	0.002%
31	5.719	1341	1362	1381	rBV2	269864	753105	100.00%	12.452%
32	6.092	1473	1478	1482	rBV2	321	412	0.05%	0.007%
33	6.176	1502	1504	1505	rBV	287	139	0.02%	0.002%
34	6.243	1511	1525	1548	rBV	274288	520941	69.17%	8.613%
35	6.481	1595	1599	1602	rBV	304	286	0.04%	0.005%
36	6.520	1605	1611	1613	rBV3	1785	1762	0.23%	0.029%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050923\
 Data File : VU054125.D
 Acq On : 09 May 2023 17:00
 Operator : JC/MD
 Sample : 02694-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 JREL6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

37	6.575	1625	1628	1631	rBV2	247	208	0.03%	0.003%
38	6.684	1648	1662	1682	rBV	179419	349887	46.46%	5.785%
39	6.832	1707	1708	1710	rBV	124	67	0.01%	0.001%
40	6.906	1727	1731	1735	rVB	189	156	0.02%	0.003%
41	6.944	1741	1743	1746	rBV2	186	95	0.01%	0.002%
42	6.983	1753	1755	1759	rBV	170	137	0.02%	0.002%
43	7.015	1761	1765	1769	rVB2	203	195	0.03%	0.003%
44	7.047	1773	1775	1776	rBV2	130	37	0.00%	0.001%
45	7.096	1785	1790	1792	rBV	222	196	0.03%	0.003%
46	7.108	1793	1794	1797	rVB	142	77	0.01%	0.001%
47	7.250	1834	1838	1844	rBV2	272	283	0.04%	0.005%
48	7.272	1844	1845	1848	rBV2	136	85	0.01%	0.001%
49	7.340	1862	1866	1870	rBV2	193	184	0.02%	0.003%
50	7.446	1895	1899	1900	rBV2	274	222	0.03%	0.004%
51	7.559	1922	1934	1957	rBV	97664	172030	22.84%	2.844%
52	7.777	2001	2002	2003	rBV	153	51	0.01%	0.001%
53	7.793	2003	2007	2012	rVB3	374	402	0.05%	0.007%
54	7.845	2020	2023	2025	rBV	212	137	0.02%	0.002%
55	7.893	2025	2038	2075	rVV	342603	598035	79.41%	9.888%
56	8.173	2114	2125	2143	rBV	68700	118061	15.68%	1.952%
57	8.333	2172	2175	2178	rBV	257	195	0.03%	0.003%
58	8.378	2185	2189	2192	rVB2	237	219	0.03%	0.004%
59	8.404	2192	2197	2203	rBV2	334	438	0.06%	0.007%
60	8.459	2209	2214	2215	rBV2	614	533	0.07%	0.009%
61	8.520	2230	2233	2236	rBV2	214	168	0.02%	0.003%
62	8.555	2242	2244	2249	rVB2	344	220	0.03%	0.004%
63	8.584	2251	2253	2254	rBV	133	35	0.00%	0.001%
64	8.629	2255	2267	2304	rBV2	184854	357288	47.44%	5.907%
65	8.983	2376	2377	2382	rVB	158	92	0.01%	0.002%
66	9.031	2389	2392	2394	rBV2	199	115	0.02%	0.002%
67	9.169	2432	2435	2437	rBV	217	122	0.02%	0.002%
68	9.411	2498	2510	2535	rBV	378949	630281	83.69%	10.421%
69	9.748	2611	2615	2618	rBV2	289	272	0.04%	0.004%
70	9.899	2660	2662	2665	rVB	218	95	0.01%	0.002%
71	10.272	2775	2778	2784	rBV	217	183	0.02%	0.003%
72	10.751	2914	2927	2943	rBV	254588	411626	54.66%	6.806%
73	10.919	2976	2979	2982	rBV2	218	152	0.02%	0.003%
74	11.449	3142	3144	3147	rVB	234	110	0.01%	0.002%
75	11.806	3243	3255	3280	rBV	401885	637065	84.59%	10.533%
76	12.189	3361	3374	3392	rBV	367940	595478	79.07%	9.846%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050923\
Data File : VU054125.D
Acq On : 09 May 2023 17:00
Operator : JC/MD
Sample : 02694-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
JREL6

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Title : VOC Analysis

77	13.224	3692	3696	3699	rBV2	501	384	0.05%	0.006%
78	13.735	3852	3855	3858	rBV	227	145	0.02%	0.002%




Sum of corrected areas: 6048042

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050923\
Data File : VU054125.D
Acq On : 09 May 2023 17:00
Operator : JC/MD
Sample : 02694-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
JREL6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

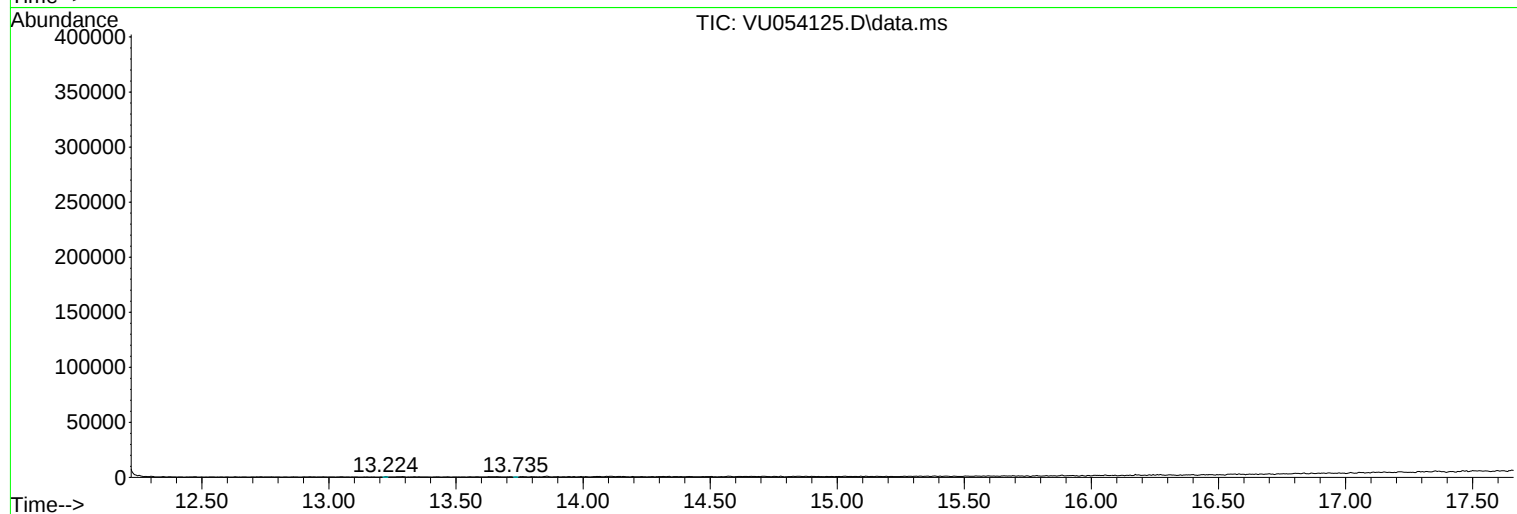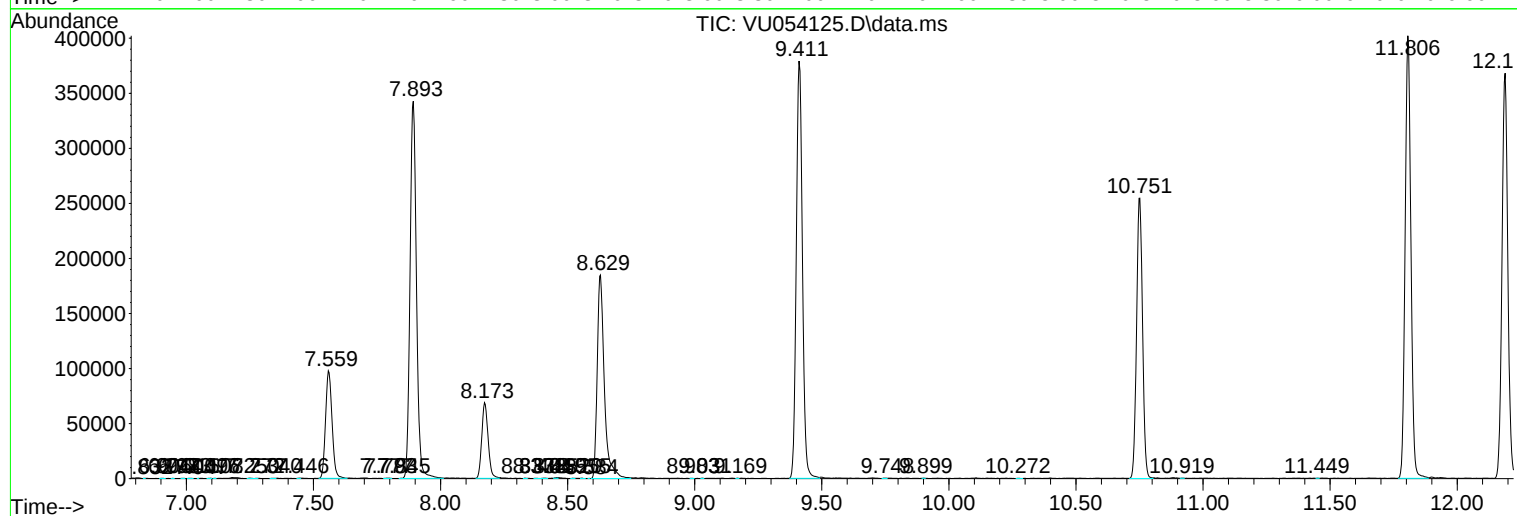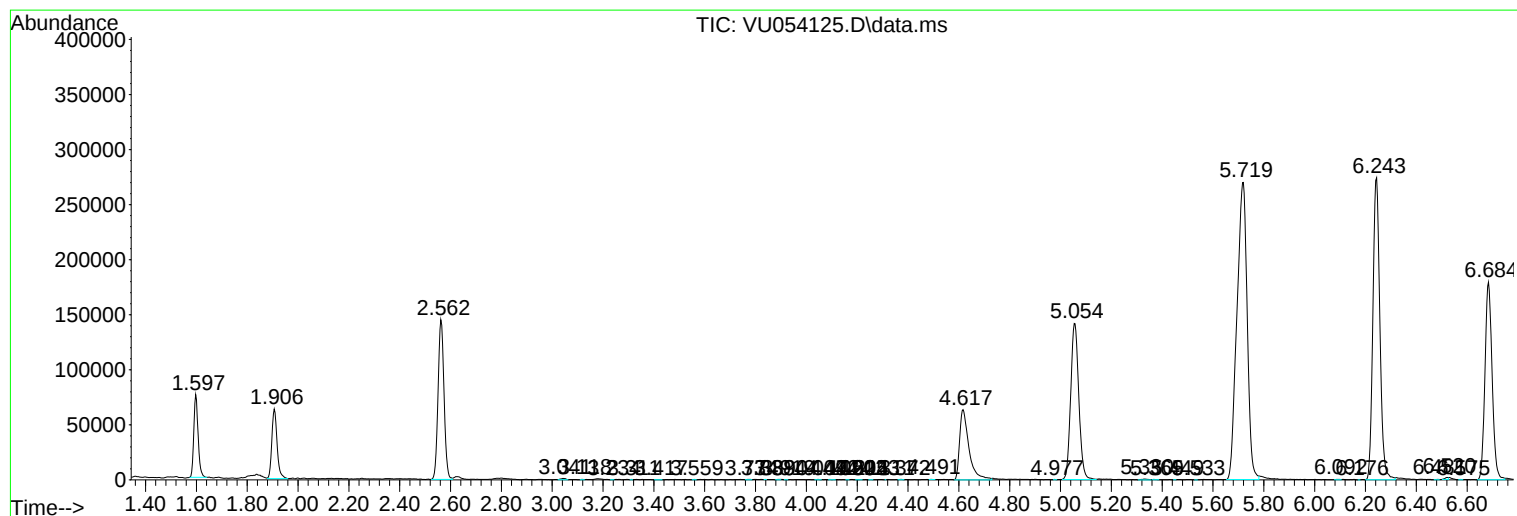

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050923\
Data File : VU054125.D
Acq On : 09 May 2023 17:00
Operator : JC/MD
Sample : 02694-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
JREL6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050923\
Data File : VU054125.D
Acq On : 09 May 2023 17:00
Operator : JC/MD
Sample : 02694-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
JREL6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc