

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050923\
 Data File : VU054126.D
 Acq On : 09 May 2023 17:23
 Operator : JC/MD
 Sample : 02694-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 JREM6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

Signal : TIC: VU054126.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	95	rVB	64840	76669	11.12%	1.379%
2	1.909	168	177	191	rBV	57911	78865	11.43%	1.419%
3	2.565	369	381	392	rBV	127237	205257	29.76%	3.693%
4	2.745	434	437	438	rBV2	507	304	0.04%	0.005%
5	2.938	495	497	501	rBV	250	187	0.03%	0.003%
6	3.179	563	572	585	rBV3	1773	3966	0.57%	0.071%
7	3.295	605	608	612	rVB	191	131	0.02%	0.002%
8	3.546	683	686	689	rVB2	228	181	0.03%	0.003%
9	3.581	692	697	698	rBV	326	293	0.04%	0.005%
10	3.665	719	723	728	rBV2	319	310	0.04%	0.006%
11	3.713	735	738	743	rBV2	297	309	0.04%	0.006%
12	3.855	780	782	785	rBV	310	224	0.03%	0.004%
13	4.002	826	828	831	rBV2	208	111	0.02%	0.002%
14	4.038	834	839	846	rVV2	230	262	0.04%	0.005%
15	4.096	854	857	859	rBV2	326	181	0.03%	0.003%
16	4.276	911	913	916	rVB	165	62	0.01%	0.001%
17	4.408	951	954	957	rBV2	245	191	0.03%	0.003%
18	4.453	964	968	971	rBV2	202	171	0.02%	0.003%
19	4.472	971	974	975	rBV	186	96	0.01%	0.002%
20	4.501	981	983	987	rVB	194	84	0.01%	0.002%
21	4.533	991	993	994	rBV	136	59	0.01%	0.001%
22	4.555	997	1000	1003	rVB	306	168	0.02%	0.003%
23	4.572	1003	1005	1008	rBV	155	58	0.01%	0.001%
24	4.617	1008	1019	1044	rBV	59196	151882	22.02%	2.733%
25	4.970	1125	1129	1131	rBV2	330	240	0.03%	0.004%
26	5.057	1140	1156	1176	rBV	128810	284970	41.32%	5.127%
27	5.337	1242	1243	1244	rBV	231	69	0.01%	0.001%
28	5.353	1244	1248	1251	rVB2	266	199	0.03%	0.004%
29	5.385	1251	1258	1261	rBV3	479	622	0.09%	0.011%
30	5.485	1286	1289	1294	rBV2	214	187	0.03%	0.003%
31	5.584	1319	1320	1321	rBV2	123	29	0.00%	0.001%
32	5.604	1324	1326	1330	rVV	155	81	0.01%	0.001%
33	5.719	1341	1362	1387	rBV2	246693	689740	100.00%	12.410%
34	5.957	1434	1436	1439	rBV	198	127	0.02%	0.002%
35	6.044	1461	1463	1467	rVB2	362	130	0.02%	0.002%
36	6.063	1467	1469	1471	rBV2	150	68	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050923\
 Data File : VU054126.D
 Acq On : 09 May 2023 17:23
 Operator : JC/MD
 Sample : 02694-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 JREM6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

37	6.089	1476	1477	1478	rBV2	161	41	0.01%	0.001%
38	6.115	1482	1485	1487	rBV2	168	151	0.02%	0.003%
39	6.179	1503	1505	1508	rVB	179	78	0.01%	0.001%
40	6.244	1512	1525	1543	rBV	248701	477122	69.17%	8.585%
41	6.488	1598	1601	1604	rBV2	204	179	0.03%	0.003%
42	6.530	1605	1614	1620	rBV6	2792	4176	0.61%	0.075%
43	6.684	1648	1662	1680	rBV	162044	315930	45.80%	5.684%
44	6.874	1717	1721	1722	rBV	258	165	0.02%	0.003%
45	6.887	1722	1725	1726	rBV2	294	190	0.03%	0.003%
46	6.986	1754	1756	1757	rBV2	217	93	0.01%	0.002%
47	7.102	1788	1792	1794	rVV3	411	322	0.05%	0.006%
48	7.125	1797	1799	1802	rVB	223	97	0.01%	0.002%
49	7.176	1811	1815	1818	rBV3	641	551	0.08%	0.010%
50	7.292	1848	1851	1853	rBV2	153	137	0.02%	0.002%
51	7.404	1884	1886	1889	rBV	197	128	0.02%	0.002%
52	7.430	1889	1894	1895	rBV2	170	124	0.02%	0.002%
53	7.485	1907	1911	1914	rBV	186	201	0.03%	0.004%
54	7.562	1922	1935	1957	rBV	88420	158618	23.00%	2.854%
55	7.687	1971	1974	1977	rBV	595	444	0.06%	0.008%
56	7.790	1998	2006	2016	rBV4	3965	6520	0.95%	0.117%
57	7.893	2025	2038	2052	rBV	307299	535706	77.67%	9.639%
58	8.124	2105	2110	2112	rBV	203	231	0.03%	0.004%
59	8.176	2115	2126	2142	rVV	64108	108483	15.73%	1.952%
60	8.317	2167	2170	2173	rBV2	225	159	0.02%	0.003%
61	8.459	2211	2214	2215	rBV	427	262	0.04%	0.005%
62	8.510	2228	2230	2233	rBV	160	97	0.01%	0.002%
63	8.549	2237	2242	2243	rBV	556	449	0.07%	0.008%
64	8.629	2255	2267	2300	rBV2	164977	323546	46.91%	5.821%
65	8.787	2310	2316	2330	rVB6	6385	10514	1.52%	0.189%
66	8.967	2369	2372	2374	rBV	336	134	0.02%	0.002%
67	9.095	2410	2412	2415	rBV	219	124	0.02%	0.002%
68	9.141	2423	2426	2430	rBV2	220	233	0.03%	0.004%
69	9.227	2450	2453	2455	rBV	238	143	0.02%	0.003%
70	9.411	2497	2510	2533	rBV	346821	588989	85.39%	10.597%
71	9.562	2553	2557	2558	rBV3	1122	794	0.12%	0.014%
72	9.694	2591	2598	2607	rVB2	2051	3210	0.47%	0.058%
73	9.883	2655	2657	2660	rBV	202	141	0.02%	0.003%
74	10.243	2766	2769	2773	rBV2	423	355	0.05%	0.006%
75	10.301	2784	2787	2790	rBV	219	145	0.02%	0.003%
76	10.439	2827	2830	2833	rBV	212	157	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050923\
 Data File : VU054126.D
 Acq On : 09 May 2023 17:23
 Operator : JC/MD
 Sample : 02694-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 JREM6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M

Title : VOC Analysis

77	10.677	2902	2904	2907	rBV2	213	138	0.02%	0.002%
78	10.751	2914	2927	2942	rBV	231047	375961	54.51%	6.764%
79	10.880	2964	2967	2969	rBV2	656	515	0.07%	0.009%
80	10.996	2998	3003	3009	rBV2	560	722	0.10%	0.013%
81	11.089	3026	3032	3039	rVB3	1078	1428	0.21%	0.026%
82	11.462	3144	3148	3160	rVB3	1714	2414	0.35%	0.043%
83	11.648	3202	3206	3212	rBV	307	232	0.03%	0.004%
84	11.745	3230	3236	3243	rBV3	1127	1500	0.22%	0.027%
85	11.806	3244	3255	3277	rBV	363841	588793	85.36%	10.594%
86	12.066	3334	3336	3340	rBV	207	139	0.02%	0.003%
87	12.189	3361	3374	3397	rBV	341484	550401	79.80%	9.903%

Sum of corrected areas: 5557865




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050923\
Data File : VU054126.D
Acq On : 09 May 2023 17:23
Operator : JC/MD
Sample : 02694-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
JREM6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

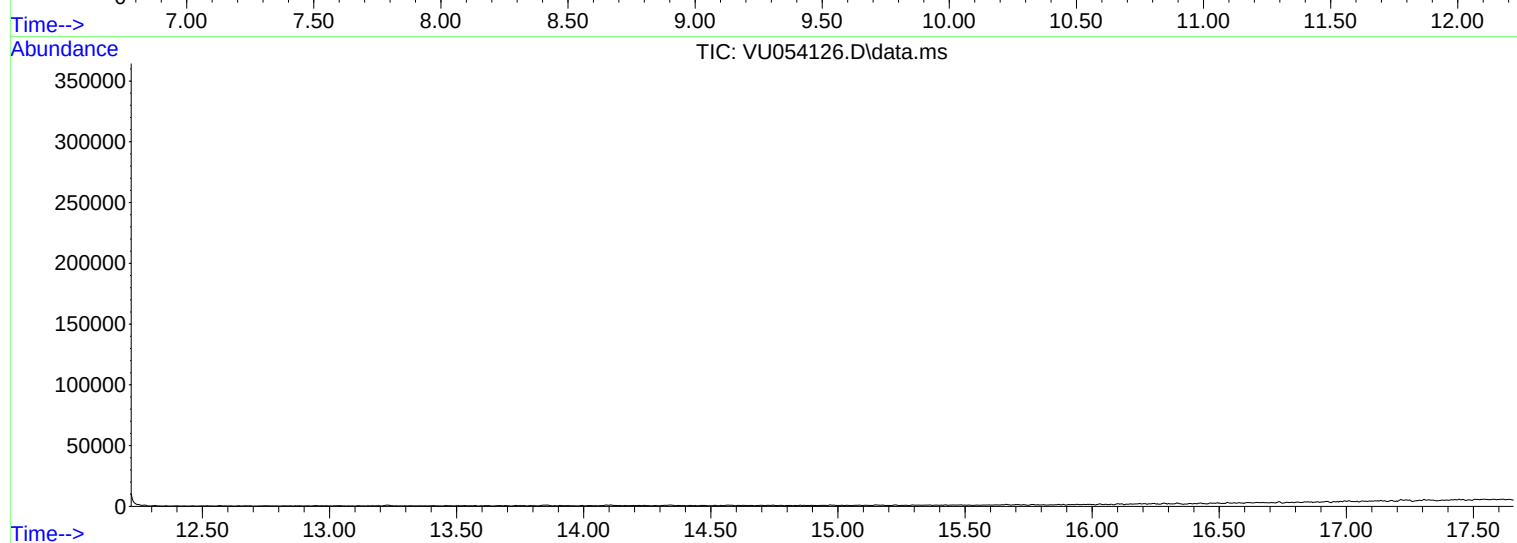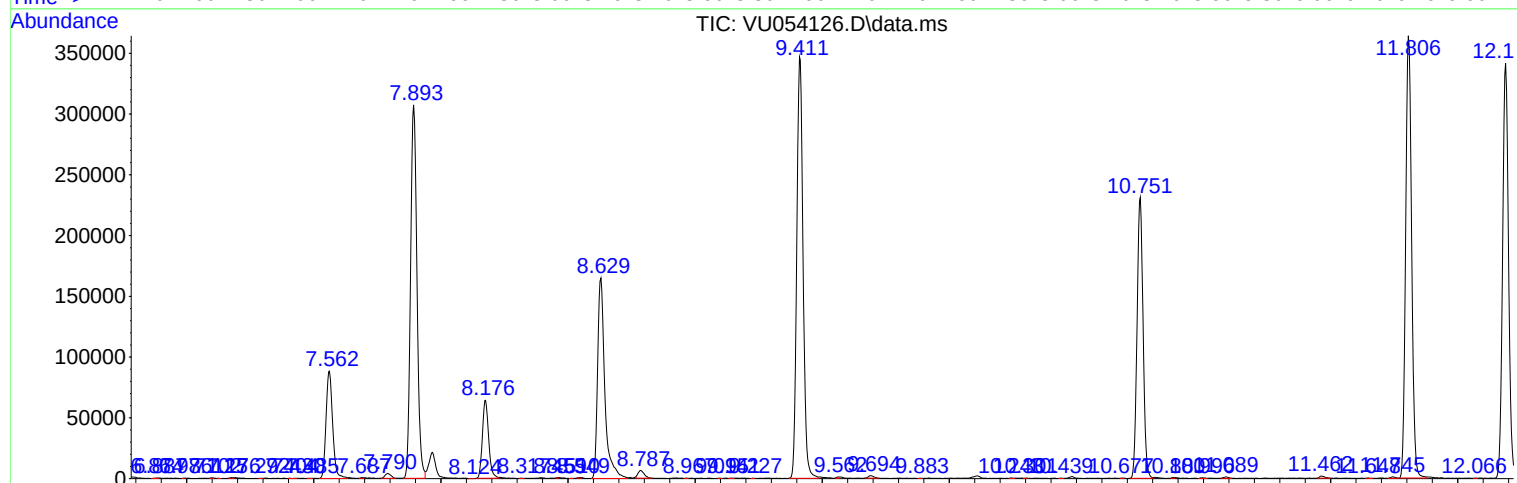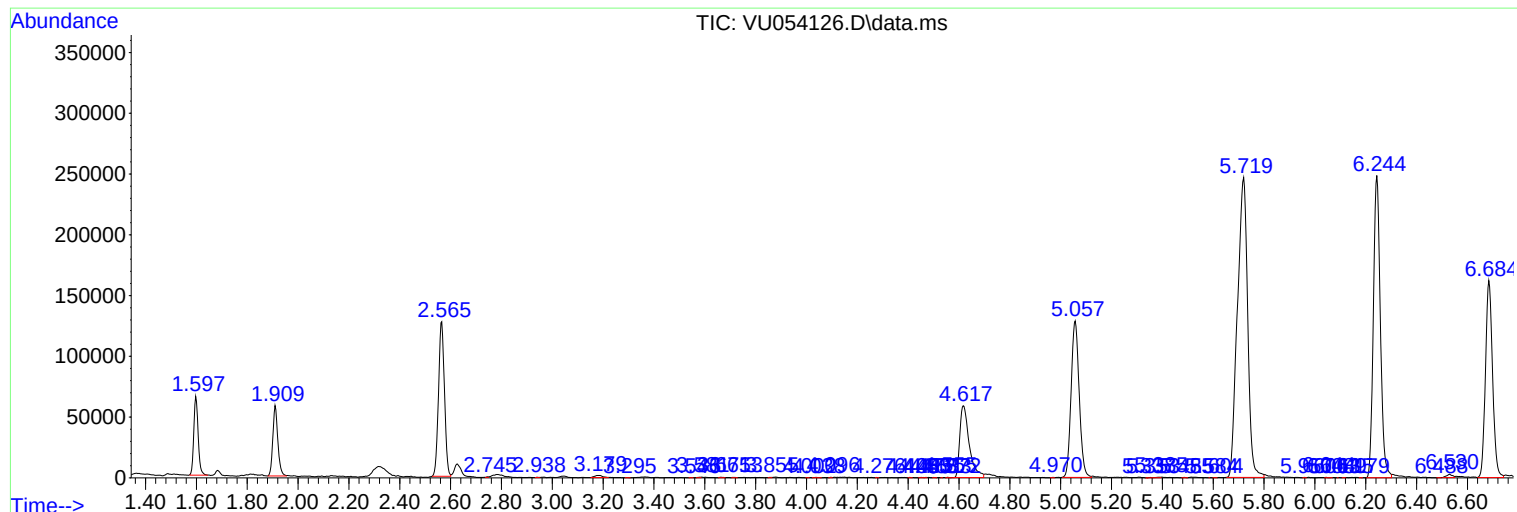

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050923\
Data File : VU054126.D
Acq On : 09 May 2023 17:23
Operator : JC/MD
Sample : 02694-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
JREM6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050923\
Data File : VU054126.D
Acq On : 09 May 2023 17:23
Operator : JC/MD
Sample : 02694-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
JREM6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------