

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050923\
 Data File : VU054131.D
 Acq On : 09 May 2023 19:21
 Operator : JC/MD
 Sample : 02694-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 JREN3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M

Title : VOC Analysis

Signal : TIC: VU054131.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	96	rVB	64566	78644	10.66%	1.357%
2	1.909	169	177	192	rVB	58109	82499	11.18%	1.423%
3	2.562	369	380	395	rBV	130949	212971	28.87%	3.674%
4	2.703	421	424	427	rBV2	361	339	0.05%	0.006%
5	2.758	436	441	442	rBV2	579	469	0.06%	0.008%
6	3.157	562	565	566	rBV2	417	224	0.03%	0.004%
7	3.321	614	616	618	rBV	234	111	0.02%	0.002%
8	3.401	637	641	643	rBV	293	178	0.02%	0.003%
9	3.472	660	663	666	rBV	157	117	0.02%	0.002%
10	3.536	679	683	686	rVB	299	166	0.02%	0.003%
11	3.755	747	751	752	rBV	297	202	0.03%	0.003%
12	3.848	777	780	783	rVB	244	128	0.02%	0.002%
13	4.137	868	870	873	rVB	215	138	0.02%	0.002%
14	4.170	877	880	881	rBV	125	72	0.01%	0.001%
15	4.240	899	902	908	rVV2	333	304	0.04%	0.005%
16	4.266	908	910	913	rVB2	173	93	0.01%	0.002%
17	4.340	931	933	934	rBV	168	92	0.01%	0.002%
18	4.456	968	969	970	rBV	112	34	0.00%	0.001%
19	4.530	989	992	999	rBV2	180	201	0.03%	0.003%
20	4.617	1006	1019	1042	rBV	61629	154156	20.90%	2.659%
21	4.925	1111	1115	1119	rBV2	347	327	0.04%	0.006%
22	4.983	1128	1133	1136	rBV2	181	167	0.02%	0.003%
23	5.057	1140	1156	1184	rVV	136890	304858	41.32%	5.259%
24	5.224	1206	1208	1210	rBV	346	193	0.03%	0.003%
25	5.250	1213	1216	1217	rVB	239	128	0.02%	0.002%
26	5.295	1226	1230	1233	rVB2	249	152	0.02%	0.003%
27	5.334	1240	1242	1243	rBV2	302	127	0.02%	0.002%
28	5.362	1249	1251	1254	rVB	144	60	0.01%	0.001%
29	5.411	1264	1266	1269	rBV2	144	86	0.01%	0.001%
30	5.440	1274	1275	1276	rBV2	106	25	0.00%	0.000%
31	5.520	1298	1300	1302	rBV2	155	81	0.01%	0.001%
32	5.620	1328	1331	1335	rBV2	210	238	0.03%	0.004%
33	5.719	1341	1362	1393	rBV2	266051	737739	100.00%	12.726%
34	6.031	1457	1459	1462	rBV	153	91	0.01%	0.002%
35	6.047	1462	1464	1466	rBV	146	46	0.01%	0.001%
36	6.086	1473	1476	1480	rBV	272	210	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050923\
 Data File : VU054131.D
 Acq On : 09 May 2023 19:21
 Operator : JC/MD
 Sample : 02694-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 JREN3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

37	6.125	1486	1488	1489	rBV	136	57	0.01%	0.001%
38	6.166	1498	1501	1503	rBV	204	164	0.02%	0.003%
39	6.243	1510	1525	1557	rBV	259311	494007	66.96%	8.521%
40	6.469	1592	1595	1599	rVV2	297	218	0.03%	0.004%
41	6.485	1599	1600	1602	rVB	147	57	0.01%	0.001%
42	6.523	1602	1612	1623	rBV8	2035	4069	0.55%	0.070%
43	6.568	1625	1626	1629	rVB	232	72	0.01%	0.001%
44	6.626	1642	1644	1647	rVB	160	56	0.01%	0.001%
45	6.684	1648	1662	1679	rBV	173653	339022	45.95%	5.848%
46	6.858	1715	1716	1717	rBV	126	35	0.00%	0.001%
47	6.960	1745	1748	1751	rVB2	203	118	0.02%	0.002%
48	7.022	1761	1767	1769	rBV	317	379	0.05%	0.007%
49	7.070	1779	1782	1785	rBV2	157	134	0.02%	0.002%
50	7.102	1787	1792	1799	rBV2	258	309	0.04%	0.005%
51	7.131	1799	1801	1804	rVB2	313	199	0.03%	0.003%
52	7.160	1804	1810	1812	rBV2	323	339	0.05%	0.006%
53	7.189	1812	1819	1826	rBV4	969	1313	0.18%	0.023%
54	7.324	1858	1861	1862	rBV	192	115	0.02%	0.002%
55	7.382	1877	1879	1881	rBV	138	77	0.01%	0.001%
56	7.427	1889	1893	1894	rBV	271	188	0.03%	0.003%
57	7.456	1899	1902	1908	rVB	342	361	0.05%	0.006%
58	7.504	1914	1917	1920	rVB2	179	118	0.02%	0.002%
59	7.559	1922	1934	1952	rBV	92776	164297	22.27%	2.834%
60	7.780	2000	2003	2004	rBV	372	172	0.02%	0.003%
61	7.893	2024	2038	2058	rBV	332043	578730	78.45%	9.983%
62	8.076	2091	2095	2098	rVB2	349	177	0.02%	0.003%
63	8.095	2098	2101	2105	rBV	238	148	0.02%	0.003%
64	8.173	2115	2125	2145	rBV	67324	115464	15.65%	1.992%
65	8.350	2177	2180	2186	rVB	222	144	0.02%	0.002%
66	8.411	2194	2199	2203	rBV2	274	286	0.04%	0.005%
67	8.427	2203	2204	2206	rBV	130	40	0.01%	0.001%
68	8.456	2211	2213	2215	rBV	227	149	0.02%	0.003%
69	8.549	2238	2242	2247	rBV3	696	612	0.08%	0.011%
70	8.629	2255	2267	2299	rBV2	179499	350860	47.56%	6.052%
71	9.018	2384	2388	2390	rBV2	192	127	0.02%	0.002%
72	9.411	2497	2510	2539	rBV	353957	593539	80.45%	10.238%
73	9.684	2592	2595	2596	rBV	362	182	0.02%	0.003%
74	9.951	2677	2678	2681	rBV	129	38	0.01%	0.001%
75	10.060	2710	2712	2714	rBV2	116	65	0.01%	0.001%
76	10.160	2741	2743	2746	rBV2	313	164	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050923\
 Data File : VU054131.D
 Acq On : 09 May 2023 19:21
 Operator : JC/MD
 Sample : 02694-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 JREN3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M

Title : VOC Analysis

77	10.275	2776	2779	2781	rBV	131	83	0.01%	0.001%
78	10.407	2817	2820	2825	rVB	229	168	0.02%	0.003%
79	10.549	2861	2864	2866	rBV	209	113	0.02%	0.002%
80	10.665	2896	2900	2902	rBV2	246	194	0.03%	0.003%
81	10.751	2911	2927	2942	rBV	245685	400924	54.34%	6.916%
82	10.880	2960	2967	2970	rBV3	336	415	0.06%	0.007%
83	10.928	2980	2982	2984	rBV	168	74	0.01%	0.001%
84	11.706	3222	3224	3225	rBV	157	50	0.01%	0.001%
85	11.806	3243	3255	3270	rBV	370913	586992	79.57%	10.125%
86	12.189	3361	3374	3398	rBV	359527	585330	79.34%	10.097%
87	13.012	3627	3630	3632	rBV	278	197	0.03%	0.003%
88	13.906	3905	3908	3914	rBV2	484	394	0.05%	0.007%




Sum of corrected areas: 5797201

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050923\
Data File : VU054131.D
Acq On : 09 May 2023 19:21
Operator : JC/MD
Sample : 02694-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
JREN3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

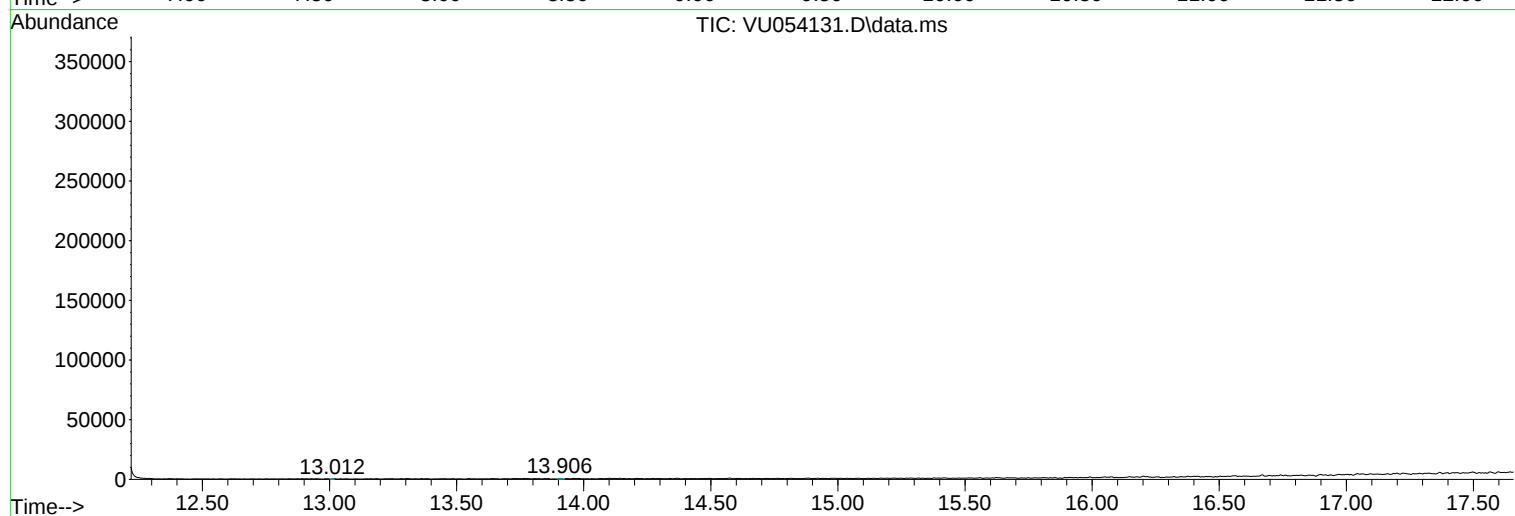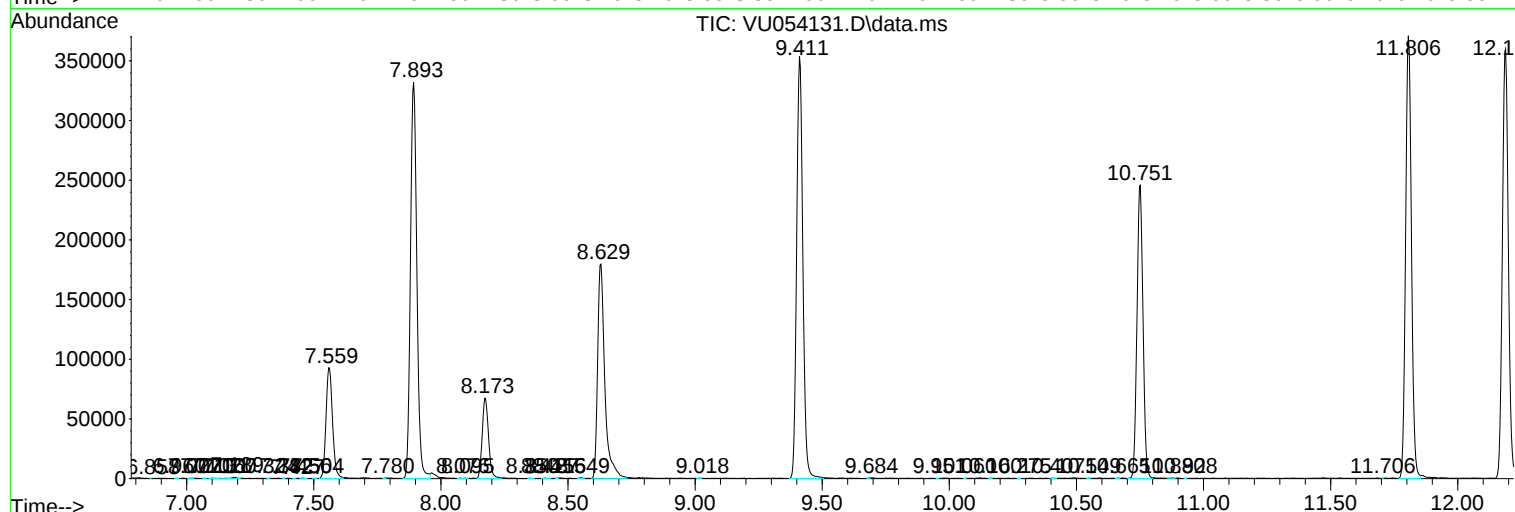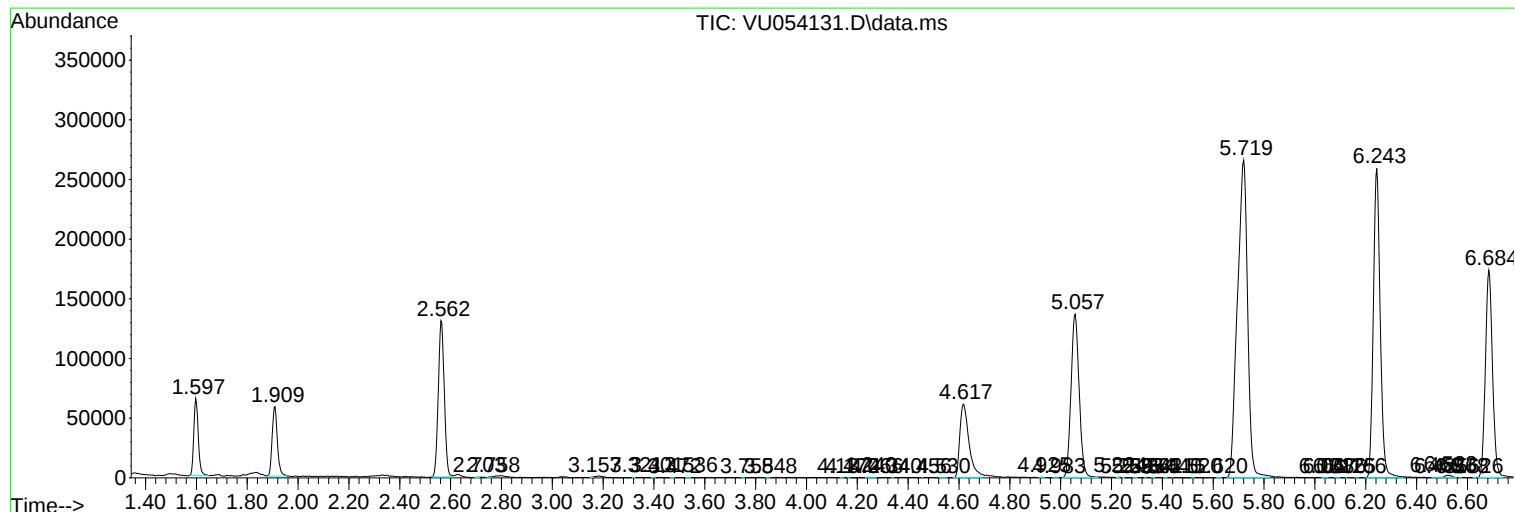

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050923\
Data File : VU054131.D
Acq On : 09 May 2023 19:21
Operator : JC/MD
Sample : 02694-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
JREN3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050923\
Data File : VU054131.D
Acq On : 09 May 2023 19:21
Operator : JC/MD
Sample : 02694-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
JREN3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------