


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050923\
Data File : VU054113.D
Acq On : 09 May 2023 09:08
Operator : JC/MD
Sample : BFB188
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB188

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Title : VOC Analysis
Last Update : Sat May 06 01:14:00 2023

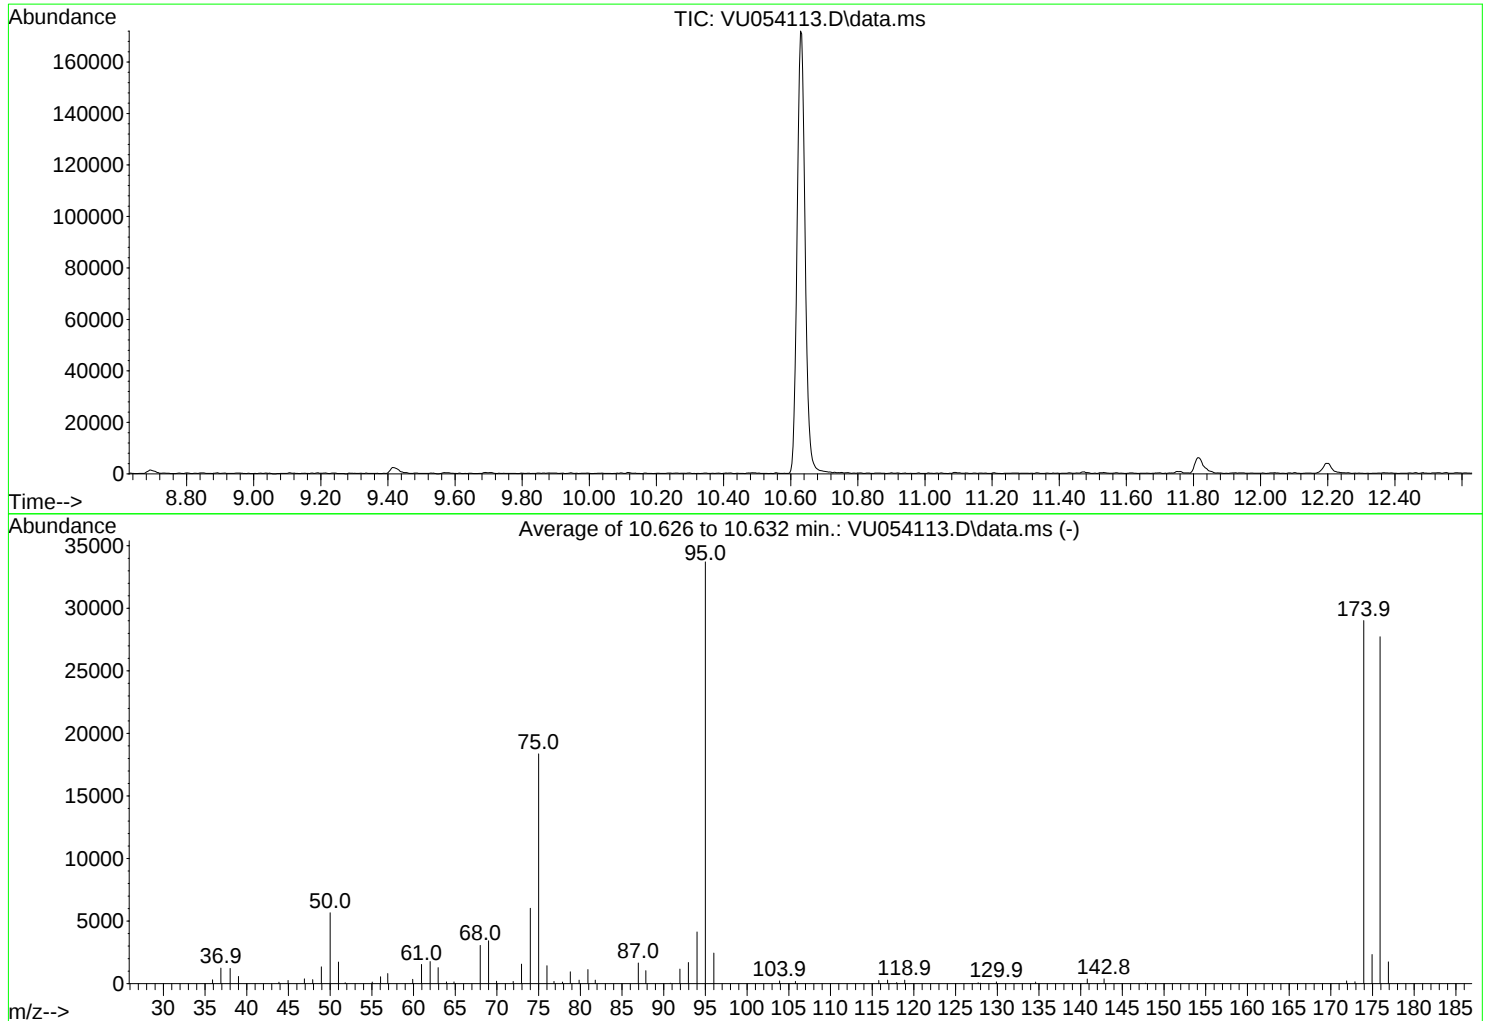

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	5672	PASS
75	95	30	80	54.5	18371	PASS
95	95	100	100	100.0	33715	PASS
96	95	5	9	7.2	2442	PASS
173	174	0.00	2	0.5	159	PASS
174	95	50	120	86.1	29021	PASS
175	174	5	9	8.0	2322	PASS
176	174	95	101	95.6	27733	PASS
177	176	5	9	6.3	1737	PASS

m/z	Abundance
43.90	174.0

Instrument :
MSVOA_U
ClientSampleId :
BFB188

m/z	Abundance
35.90	319.0
36.90	1113.0
38.00	1274.0
39.00	552.0
43.90	233.0
45.00	240.0
46.90	387.0
47.90	347.0
49.00	1192.0
50.00	5691.0
51.00	1663.0
51.80	117.0
55.10	112.0
56.00	509.0
56.90	744.0
59.90	321.0
60.90	1454.0
62.00	1638.0
62.90	1241.0
63.90	150.0
64.80	119.0
68.00	2967.0
69.00	3194.0
70.00	183.0
72.00	177.0
73.00	1418.0
74.00	5667.0
75.00	17664.0
76.00	1351.0
76.90	140.0
77.90	127.0
78.80	939.0
79.90	274.0
80.90	1018.0
81.80	215.0
86.90	1652.0
87.90	1052.0
91.90	998.0
93.00	1576.0
94.00	3926.0
95.00	32008.0
96.00	2402.0
103.90	235.0
105.80	169.0
115.80	195.0
116.80	244.0
117.90	155.0
118.80	244.0
128.00	117.0
129.90	136.0
134.60	105.0
140.80	355.0
142.80	352.0
171.90	207.0
173.90	27136.0
174.90	2268.0
175.90	25688.0
176.90	1723.0

Instrument :
MSVOA_U
ClientSampleId :
BFB188

m/z	Abundance
35.90	318.0
36.90	1288.0
38.00	1255.0
39.00	611.0
43.80	281.0
44.90	264.0
46.90	409.0
47.90	340.0
49.00	1353.0
50.00	5792.0
51.00	1795.0
51.80	130.0
55.10	156.0
56.10	579.0
56.90	825.0
59.90	333.0
60.90	1578.0
62.00	1808.0
63.00	1324.0
63.90	132.0
64.90	133.0
68.00	3103.0
69.00	3462.0
69.90	189.0
71.90	179.0
73.00	1588.0
74.00	6158.0
75.00	18952.0
76.00	1477.0
76.80	168.0
77.80	131.0
78.80	951.0
79.90	289.0
80.90	1145.0
81.80	300.0
86.90	1746.0
87.90	998.0
92.00	1229.0
92.90	1749.0
94.00	4220.0
95.00	34784.0
96.00	2523.0
103.90	247.0
105.80	174.0
115.80	293.0
116.80	282.0
118.00	127.0
118.90	288.0
127.70	107.0
129.90	157.0
134.60	136.0
140.80	404.0
142.80	376.0
147.80	108.0
171.90	227.0
172.90	477.0
173.90	29928.0
175.00	2369.0
175.90	28456.0
176.90	1807.0

Instrument :
MSVOA_U
ClientSampleId :
BFB188

m/z	Abundance
35.90	292.0
36.90	1330.0
38.00	1103.0
39.00	587.0
43.80	348.0
44.90	275.0
46.90	372.0
47.90	278.0
48.90	1484.0
50.00	5532.0
51.00	1724.0
55.00	136.0
56.10	583.0
56.90	835.0
59.90	367.0
61.00	1567.0
62.00	1844.0
63.00	1289.0
64.00	130.0
64.90	160.0
68.00	3105.0
69.00	3628.0
69.90	196.0
71.90	176.0
72.90	1695.0
74.00	6239.0
75.00	18496.0
76.00	1457.0
76.90	215.0
77.80	123.0
78.80	937.0
79.80	287.0
80.90	1220.0
81.80	348.0
87.00	1573.0
87.80	1069.0
90.80	136.0
92.00	1251.0
92.90	1734.0
94.00	4242.0
95.00	34352.0
96.00	2400.0
103.90	190.0
105.80	194.0
115.80	293.0
116.90	302.0
119.00	335.0
127.70	120.0
129.90	143.0
134.60	126.0
140.80	363.0
142.80	425.0
171.90	225.0
174.00	30000.0
175.00	2329.0
175.90	29056.0
176.90	1680.0

Instrument :
MSVOA_U
ClientSampleId :
BFB188