

Data File : VU031899.D
Acq On : 10 May 2019 19:32
Operator : JC/SP
Sample : K2742-01DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0C26DL

Quant Time: May 11 02:49:20 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis
QLast Update : Sat May 11 02:45:36 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	1001160	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	1002780	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	388135	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	372317	44.43	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	88.86%
7) Chloroethane-d5	1.94	69	224	0.03	ug/L	0.27
Spiked Amount	50.000	Range	70 - 130	Recovery	=	0.06%#
11) 1,1-Dichloroethene-d2	2.26	63	522257	31.30	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	62.60%
21) 2-Butanone-d5	4.17	46	671318	88.43	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	88.43%
24) Chloroform-d	4.64	84	689064	44.90	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.80%
26) 1,2-Dichloroethane-d4	5.30	65	463649	46.25	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.50%
32) Benzene-d6	5.33	84	1414794	45.95	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.90%
36) 1,2-Dichloropropane-d6	6.32	67	483509	44.63	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	89.26%
41) Toluene-d8	7.56	98	1185202	44.19	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	88.38%
43) trans-1,3-Dichloropropene-	7.85	79	198593	42.70	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	85.40%
47) 2-Hexanone-d5	8.31	63	469157	100.05	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	100.05%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	695312	47.82	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	95.64%
64) 1,2-Dichlorobenzene-d4	11.85	152	420556	51.52	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	103.04%

Target Compounds


					Qvalue
13) Acetone	2.32	43	20872	2.441 ug/L	96
44) trans-1,3-Dichloropropene	7.85	75	7835	0.625 ug/L #	76
51) Chlorobenzene	9.12	112	98455	4.537 ug/L	97
62) 1,3-Dichlorobenzene	11.42	146	10217	0.795 ug/L	92
63) 1,4-Dichlorobenzene	11.50	146	85575	6.431 ug/L	95
65) 1,2-Dichlorobenzene	11.87	146	516979	37.861 ug/L	97
67) 1,3,5-Trichlorobenzene	13.50	180	51767	5.380 ug/L	94
68) 1,2,4-trichlorobenzene	13.50	180	51767	6.795 ug/L	91
70) 1,2,3-Trichlorobenzene	13.99	180	46054	5.310 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VU031899.D
Acq On : 10 May 2019 19:32
Operator : JC/SP
Sample : K2742-01DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0C26DL

Quant Time: May 11 02:49:20 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis
QLast Update : Sat May 11 02:45:36 2019
Response via : Initial Calibration

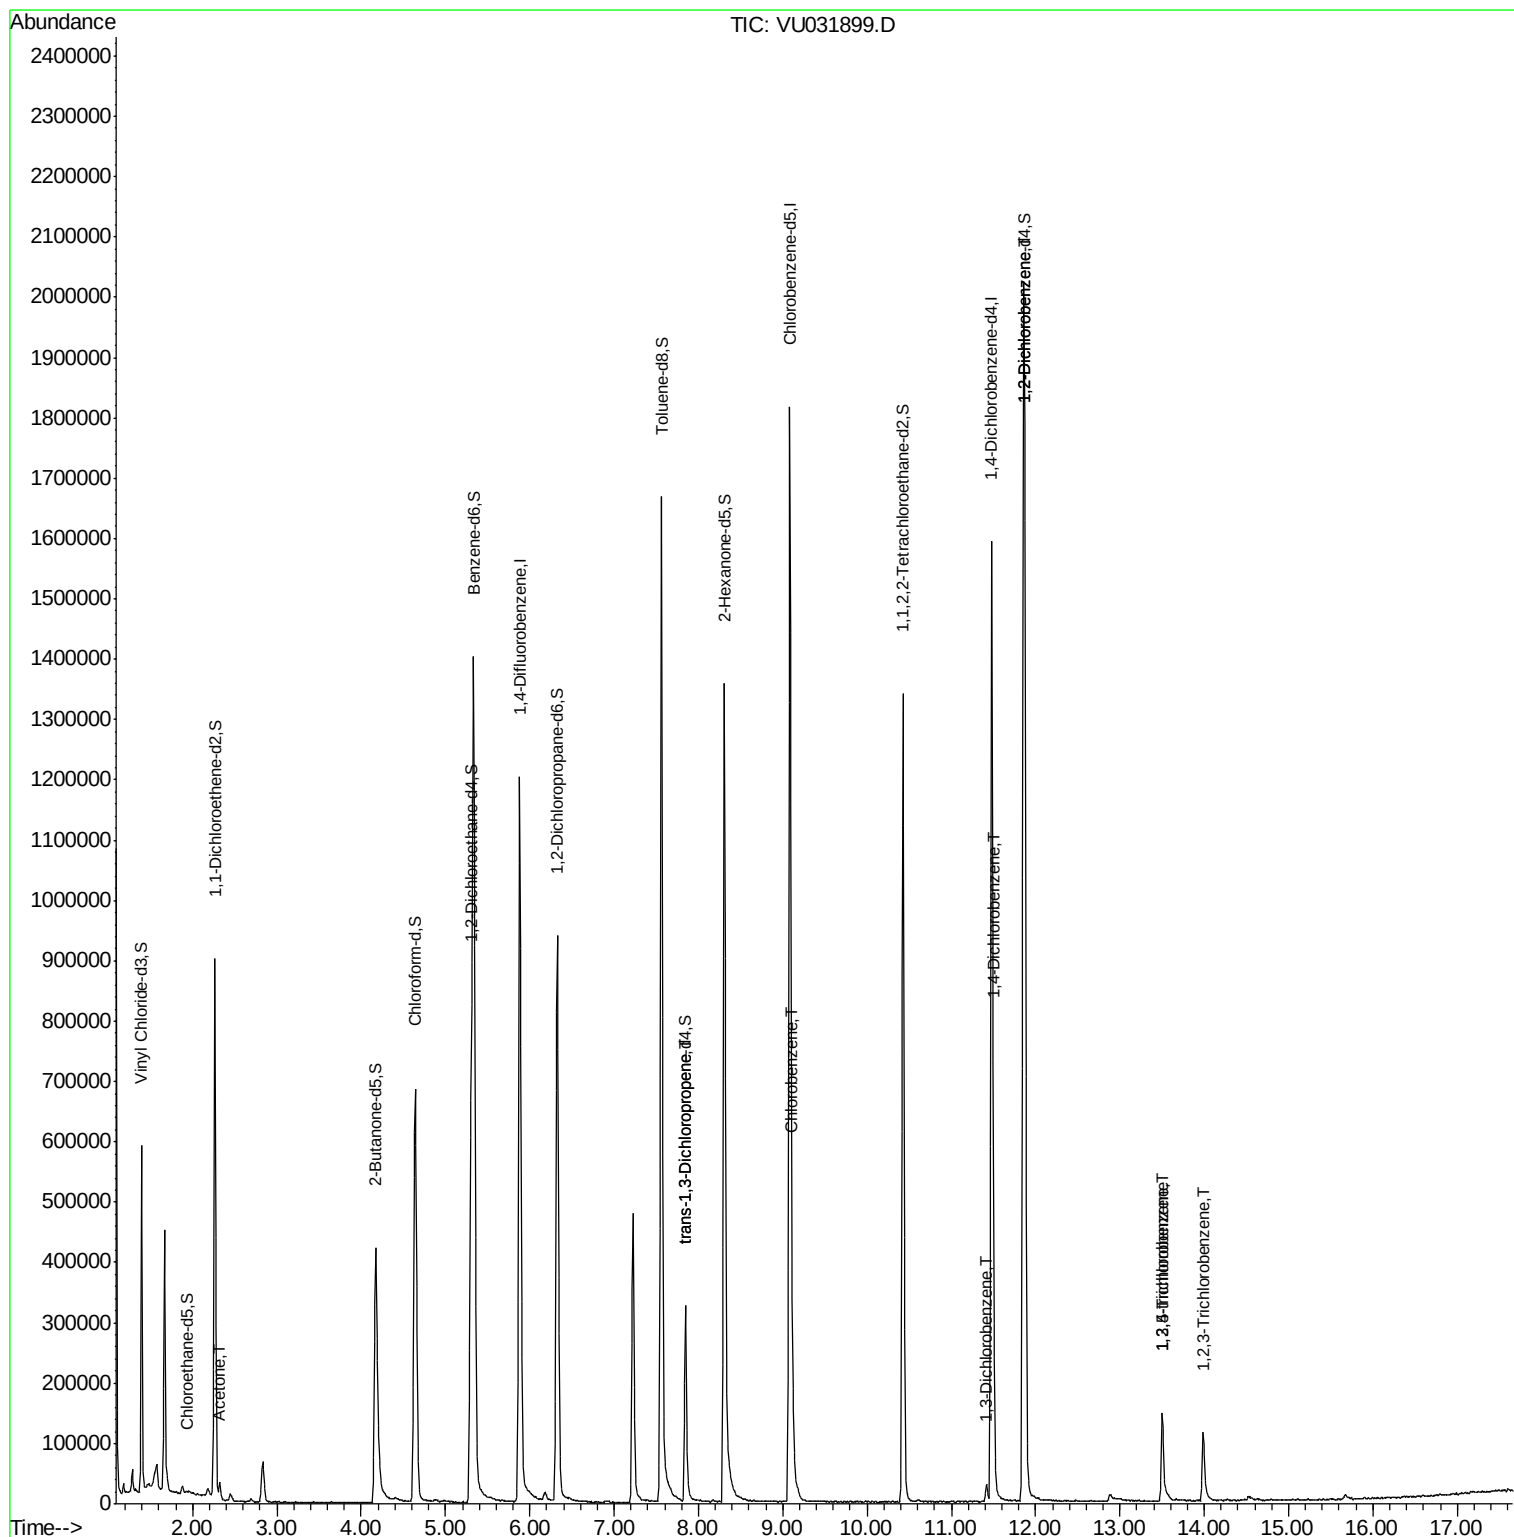

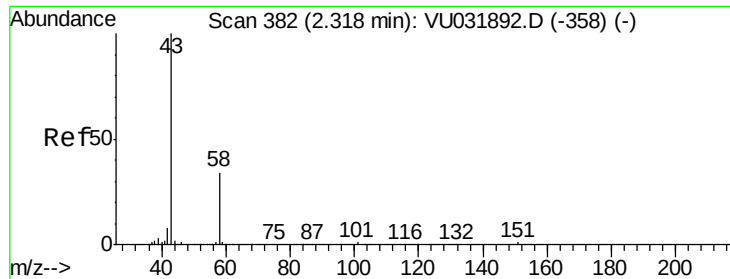

#13

Acetone

Concen: 2.441 ug/L

RT: 2.32 min Scan# 383

Delta R.T. 0.00 min

Lab File: VU031899.D

Acq: 10 May 2019 19:32

Instrument :

MSVOA_U

ClientSampleId :


C0C26DL

Tgt Ion: 43 Resp: 20872

Ion Ratio Lower Upper

43 100

58 34.5 0.0 64.4

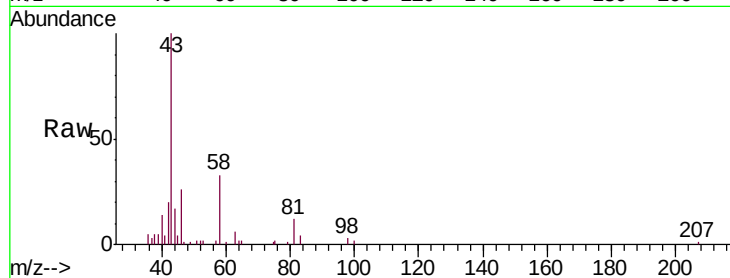

Abundance Ion 43.00 (42.70 to 43.70): VU031899.D (-289) (-)

Ion 58.00 (57.70 to 58.70): VU031899.D (-289) (-)

15000



10000

5000

2.32

2.25 2.30 2.35 2.40

Time-->

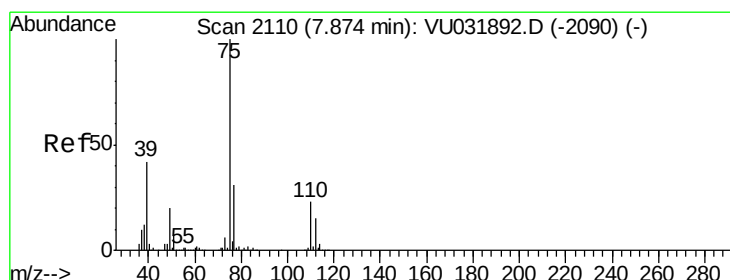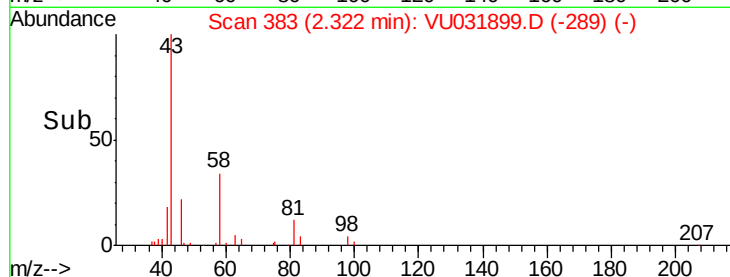

#44

trans-1,3-Dichloropropene

Concen: 0.625 ug/L

RT: 7.85 min Scan# 2101

Delta R.T. -0.03 min

Lab File: VU031899.D


Acq: 10 May 2019 19:32

Tgt Ion: 75 Resp: 7835

Ion Ratio Lower Upper

75 100

77 45.1 22.1 41.1#

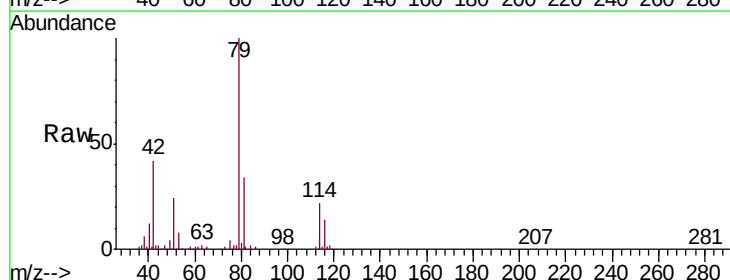

Abundance Ion 75.00 (74.70 to 75.70): VU031899.D (-2017) (-)

Ion 77.00 (76.70 to 77.70): VU031899.D (-2017) (-)

5000

4000

3000


2000


1000

7.85

7.80 7.85 7.90

Time-->




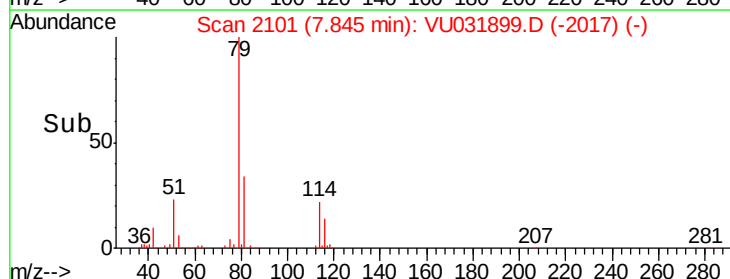


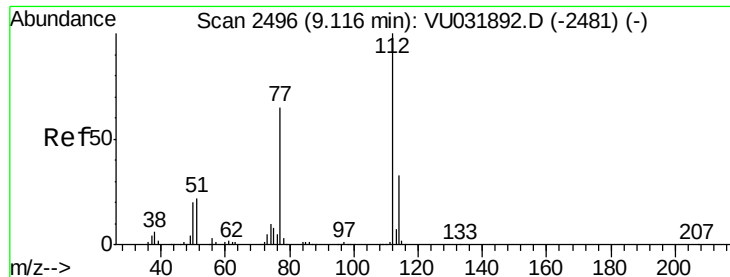

#51
Chlorobenzene
Concen: 4.537 ug/L
RT: 9.12 min Scan# 2496
Delta R.T. -0.00 min
Lab File: VU031899.D
Acq: 10 May 2019 19:32




Instrument :
MSVOA_U
ClientSampleId :
C0C26DL


Tgt Ion	Ratio	Lower	Upper
112	100		
114	29.5	23.3	43.3
77	64.9	53.0	79.4

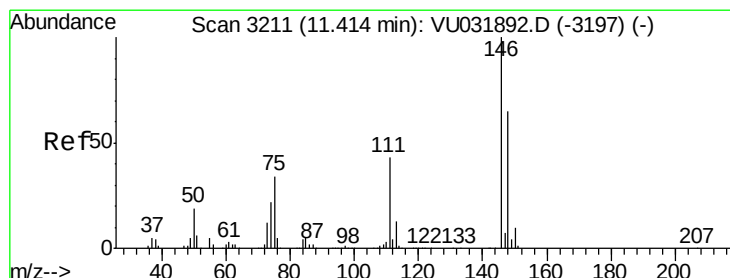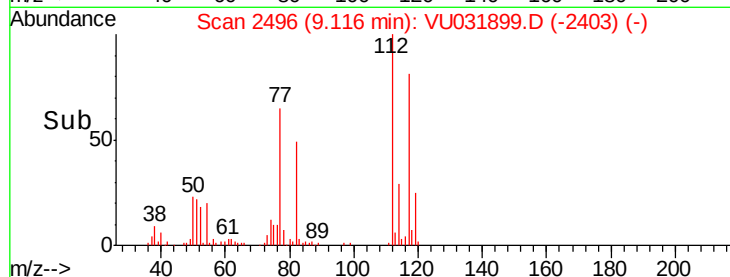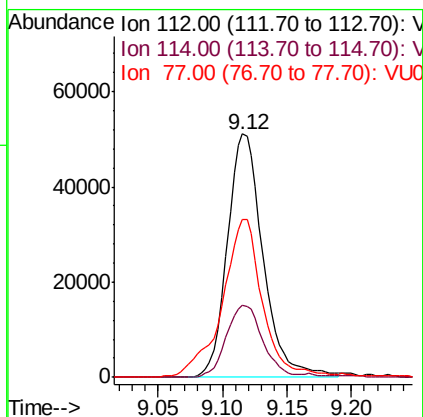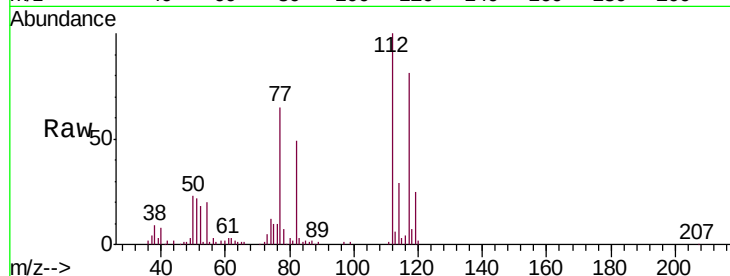

#62
1,3-Dichlorobenzene
Concen: 0.795 ug/L
RT: 11.42 min Scan# 3213
Delta R.T. 0.01 min
Lab File: VU031899.D
Acq: 10 May 2019 19:32

Tgt Ion	Ratio	Lower	Upper
146	100		
111	52.9	29.8	55.4
148	66.0	45.1	83.9


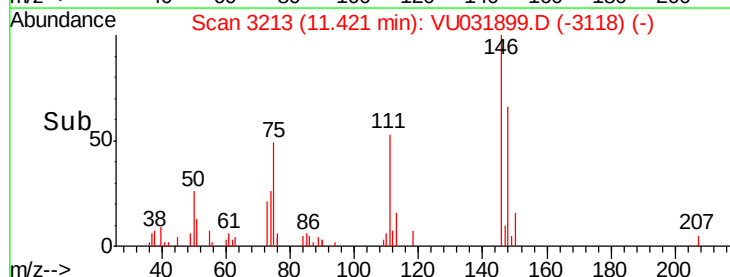
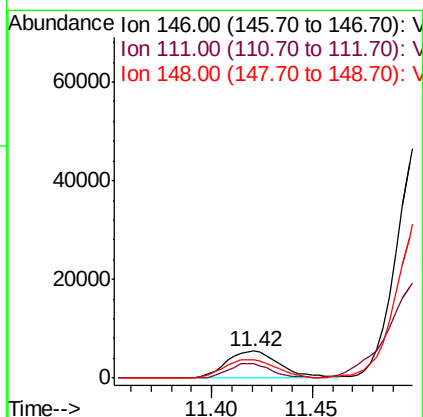
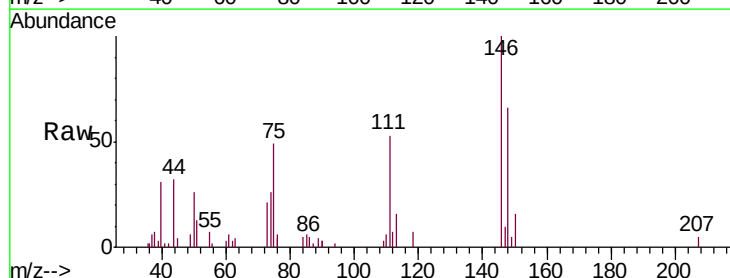


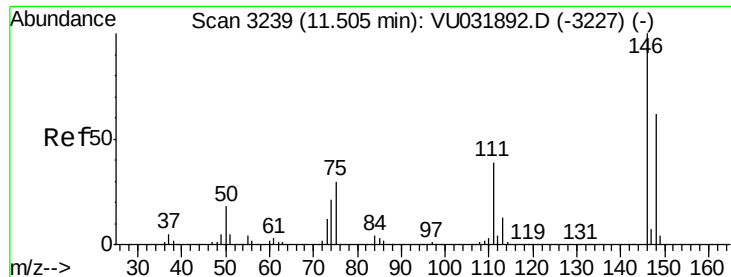

#63
 1,4-Dichlorobenzene
 Concen: 6.431 ug/L
 RT: 11.50 min Scan# 3239
 Delta R.T. -0.00 min
 Lab File: VU031899.D
 Acq: 10 May 2019 19:32




Instrument :
 MSVOA_U
 ClientSampleId :
 C0C26DL


Tgt Ion:146 Resp: 85575
 Ion Ratio Lower Upper
 146 100
 111 41.2 28.2 52.4
 148 70.3 45.4 84.4

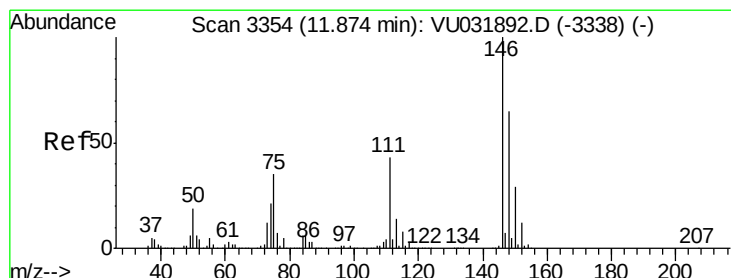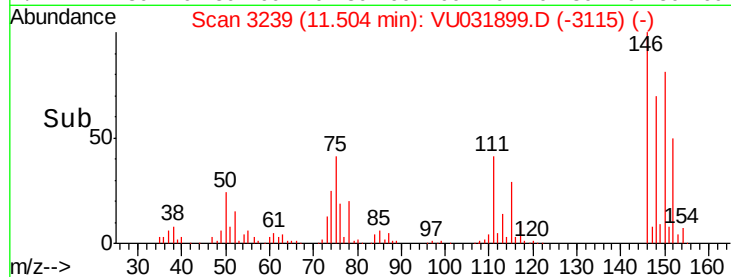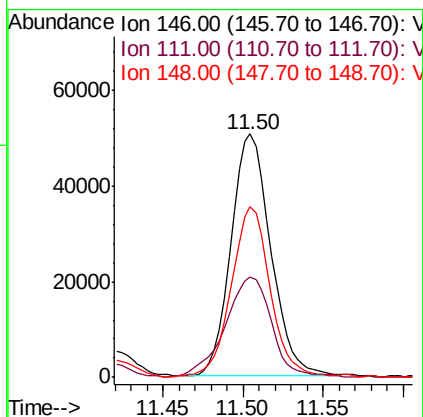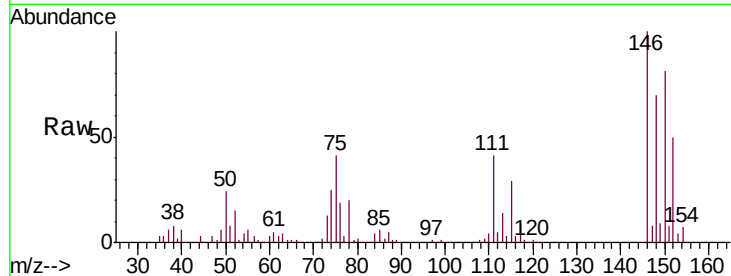

#65
 1,2-Dichlorobenzene
 Concen: 37.861 ug/L
 RT: 11.87 min Scan# 3354
 Delta R.T. -0.00 min
 Lab File: VU031899.D
 Acq: 10 May 2019 19:32

Tgt Ion:146 Resp: 516979
 Ion Ratio Lower Upper
 146 100
 111 43.6 35.9 53.9
 148 60.4 50.5 75.7


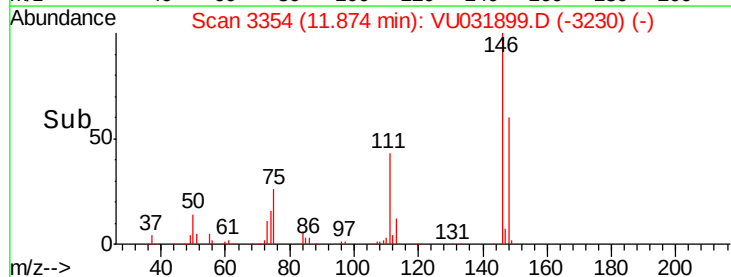
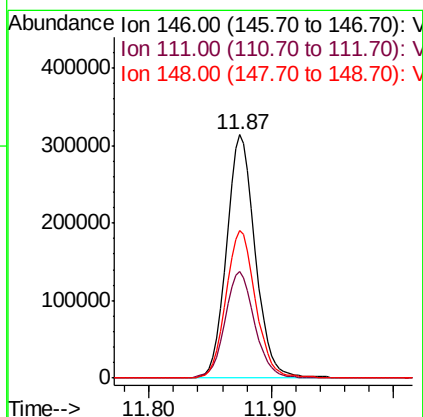
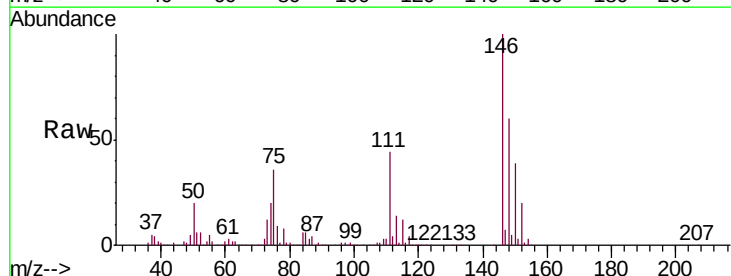


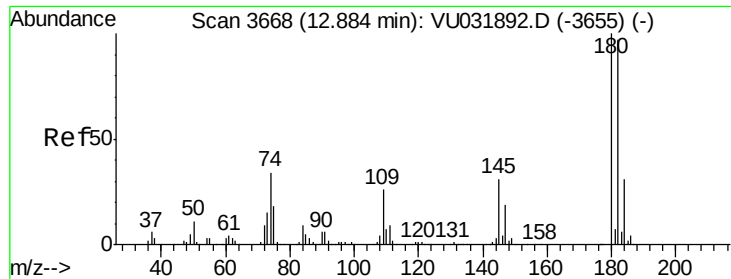

#67
 1,3,5-Trichlorobenzene
 Concen: 5.380 ug/L
 RT: 13.50 min Scan# 3861
 Delta R.T. 0.62 min
 Lab File: VU031899.D
 Acq: 10 May 2019 19:32




Instrument :
 MSVOA_U
 ClientSampleId :
 C0C26DL


Tgt Ion:	180	Resp:	51767
Ion	Ratio	Lower	Upper
180	100		
182	104.0	77.3	115.9
184	32.5	24.4	36.6
145	27.4	23.8	35.8

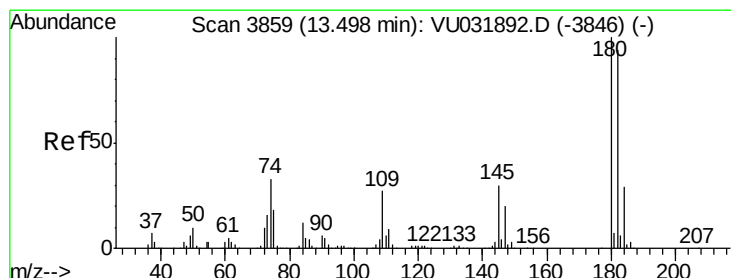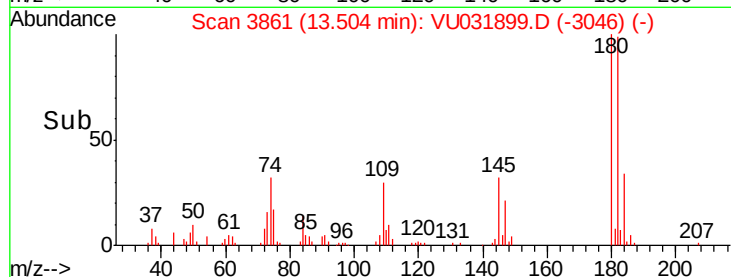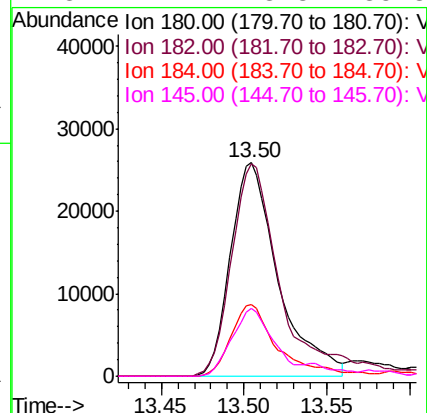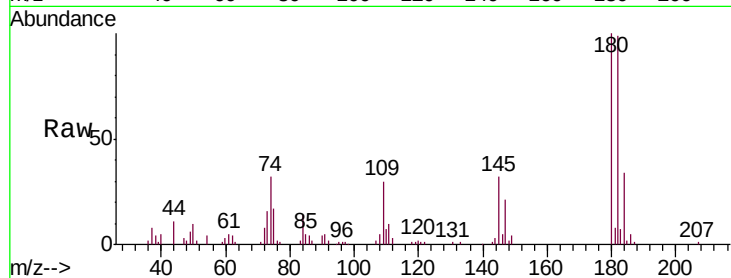

#68
 1,2,4-trichlorobenzene
 Concen: 6.795 ug/L
 RT: 13.50 min Scan# 3861
 Delta R.T. 0.01 min
 Lab File: VU031899.D
 Acq: 10 May 2019 19:32

Tgt Ion:	180	Resp:	51767
Ion	Ratio	Lower	Upper
180	100		
182	104.0	75.8	113.8
145	27.4	24.5	36.7

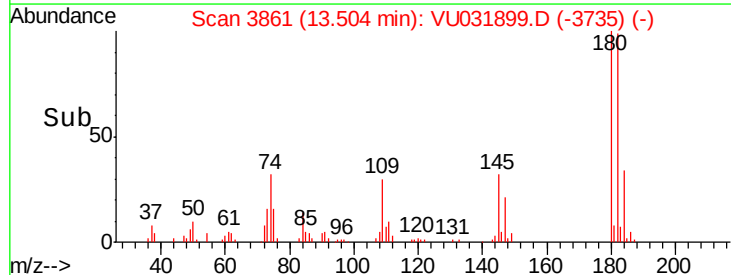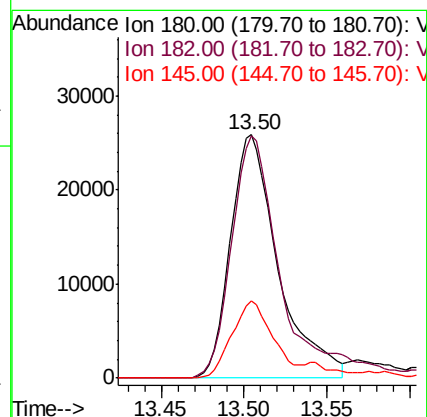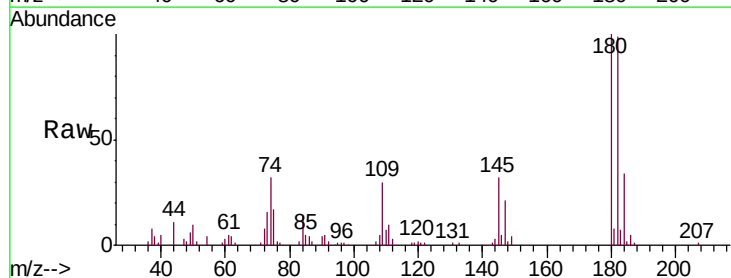

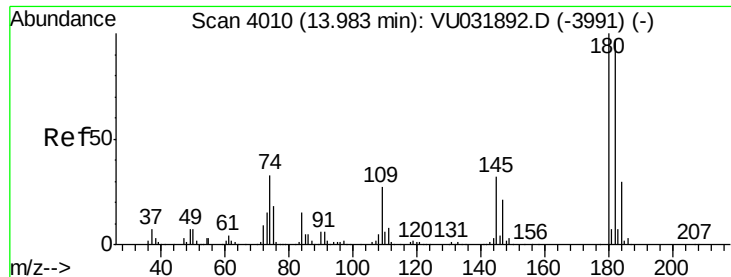

#70
 1,2,3-Trichlorobenzene
 Concen: 5.310 ug/L
 RT: 13.99 min Scan# 4011
 Delta R.T. 0.00 min
 Lab File: VU031899.D
 Acq: 10 May 2019 19:32

Instrument :
 MSVOA_U
 ClientSampleId :
 C0C26DL

Tgt Ion:180 Resp: 46054
 Ion Ratio Lower Upper
 180 100
 182 88.7 76.1 114.1
 145 30.4 26.0 39.0

