

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU051019\
Quantitation Report (QT/LSC Reviewed)


Data File : VU031882.D
Acq On : 10 May 2019 12:40
Operator : JC/SP
Sample : K2690-19ME
Misc : 5.43g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A5165ME

Manual Integrations
APPROVED

MMDadoda
5/11/2019 11:48:40 AM

Quant Time: May 11 01:48:08 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis
QLast Update : Sat May 11 00:57:57 2019
Response via : Initial Calibration

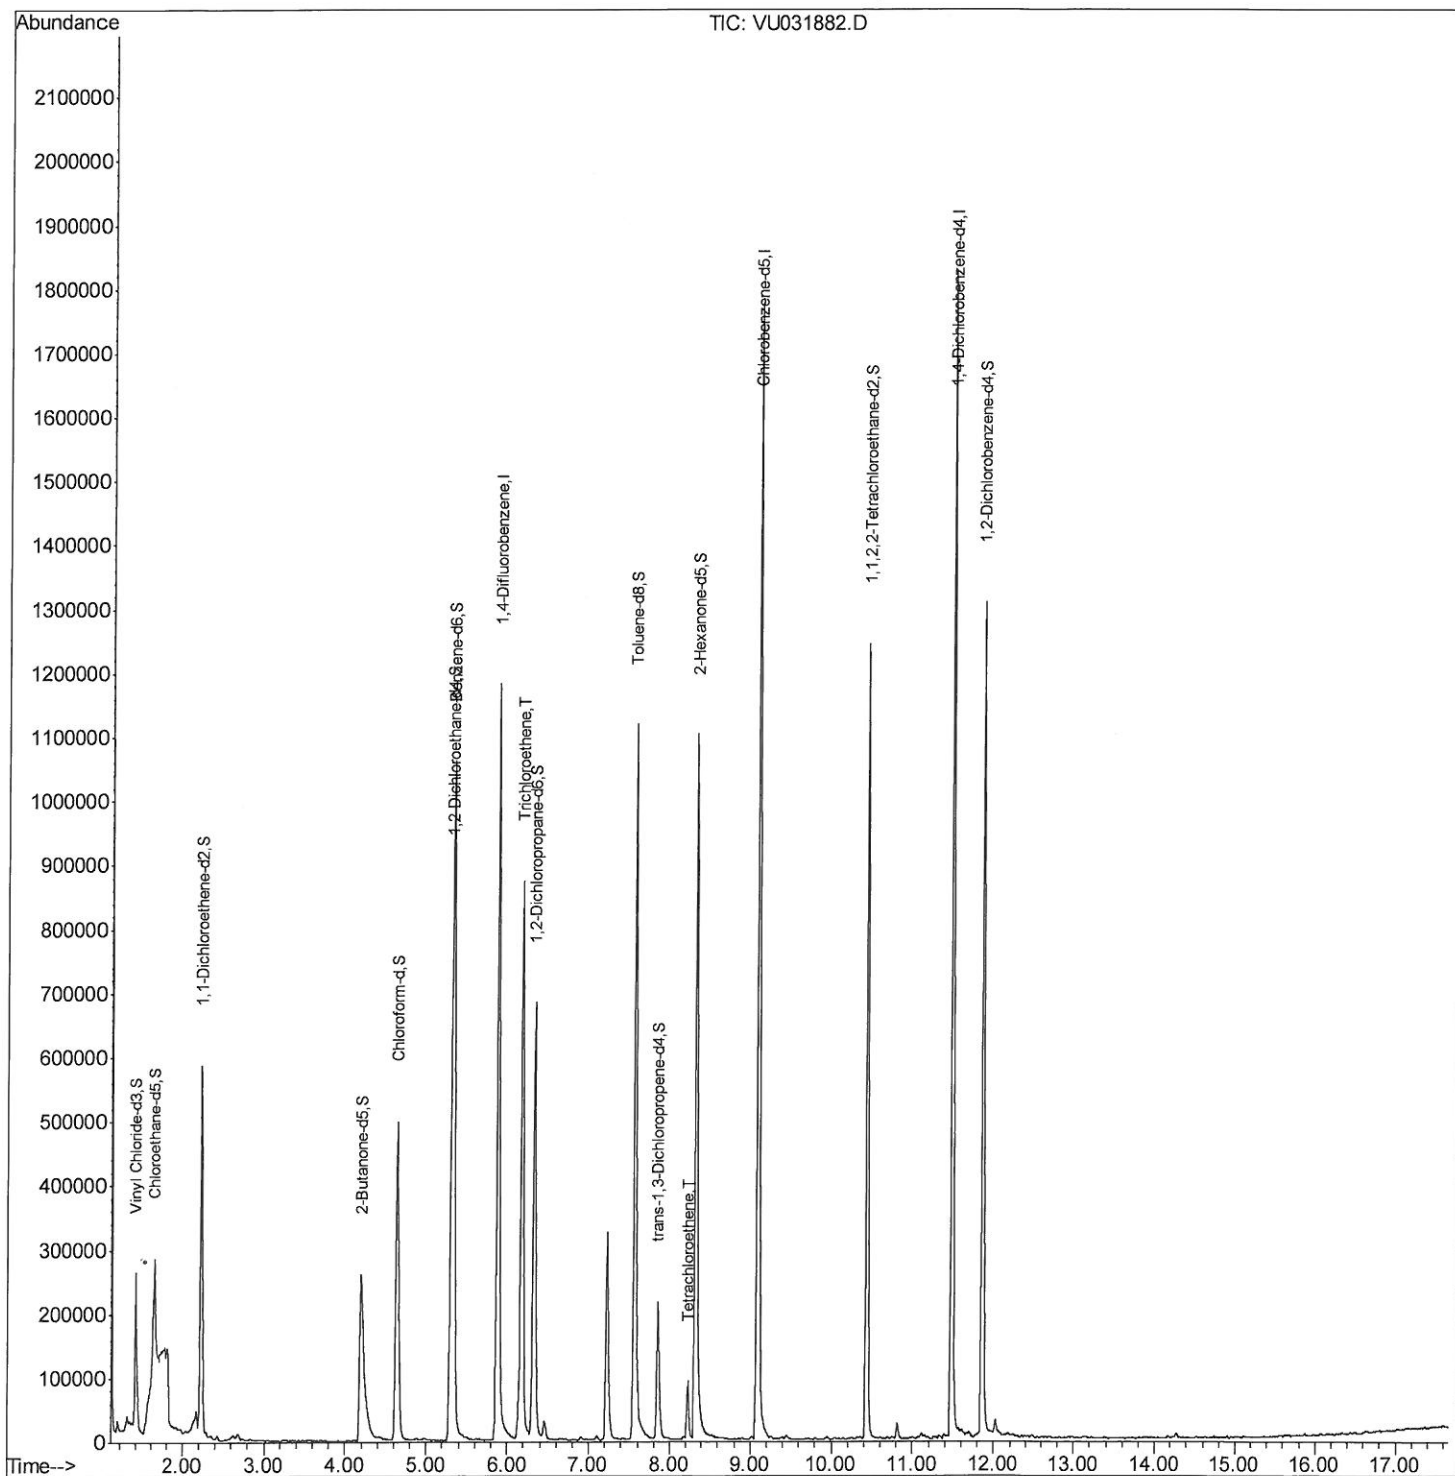

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU051019\
Quantitation Report (Qedit)




Data File : VU031882.D
Acq On : 10 May 2019 12:40
Operator : JC/SP
Sample : K2690-19ME
Misc : 5.43g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A5165ME

Manual Integrations
APPROVED

MMDadoda
5/11/2019 11:48:40 AM

Quant Time: May 11 01:01:20 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis
QLast Update : Sat May 11 00:57:57 2019
Response via : Initial Calibration

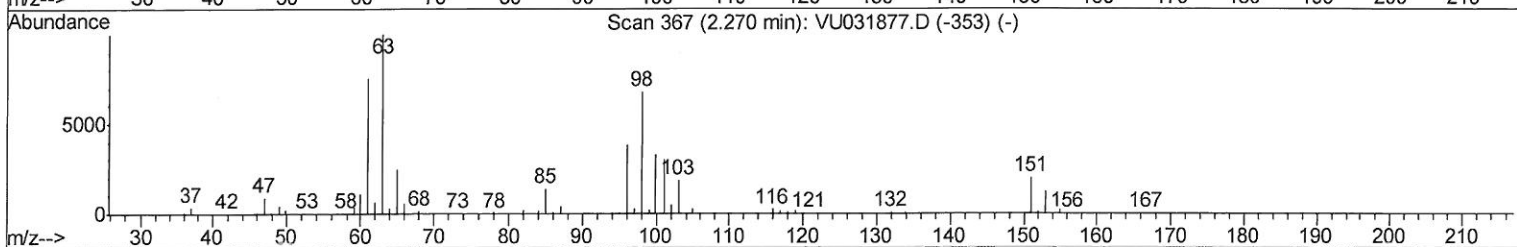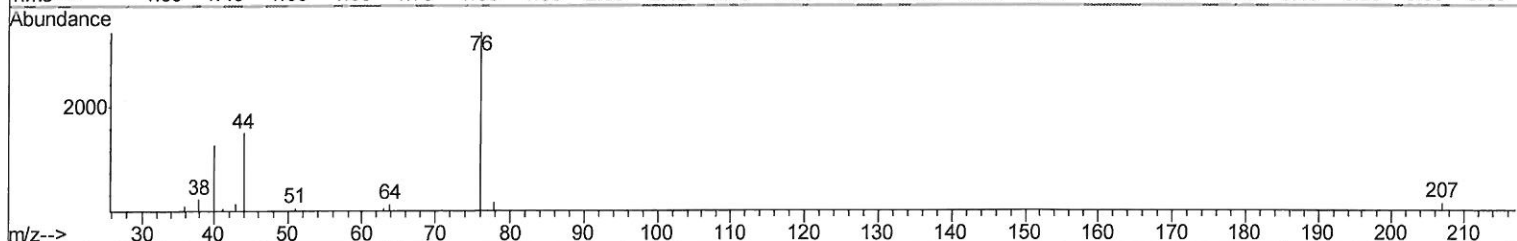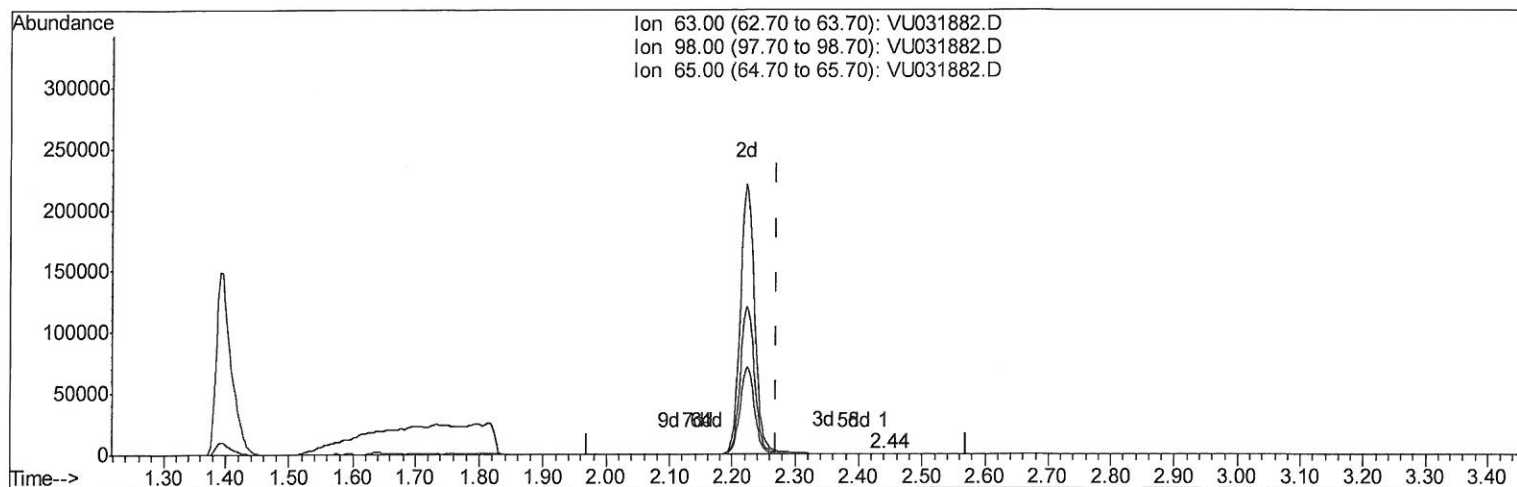

TIC: VU031882.D

(11) 1,1-Dichloroethene-d2 (S)

2.441min (+0.171) 0.00ug/L

response 80

Ion	Exp%	Act%
63.00	100	100
98.00	66.60	81.25
65.00	23.40	26.25
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU051019\
Quantitation Report (Qedit)




Data File : VU031882.D
Acq On : 10 May 2019 12:40
Operator : JC/SP
Sample : K2690-19ME
Misc : 5.43g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A5165ME

Manual Integrations
APPROVED

MMDadoda
5/11/2019 11:48:40 AM

Quant Time: May 11 01:01:20 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis
QLast Update : Sat May 11 00:57:57 2019
Response via : Initial Calibration

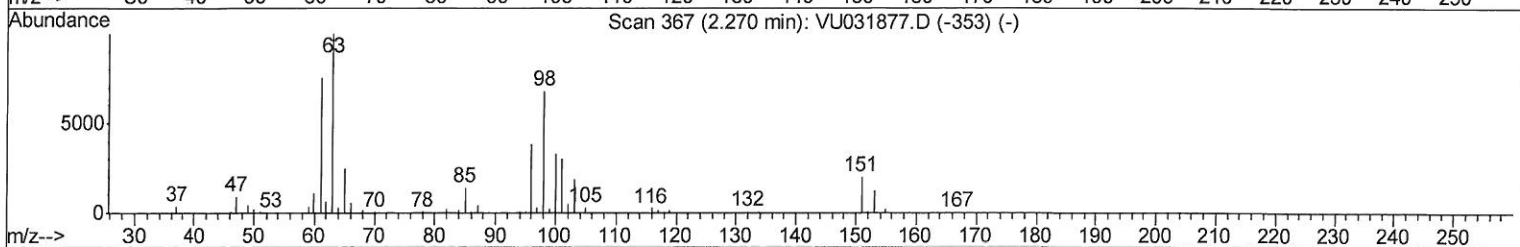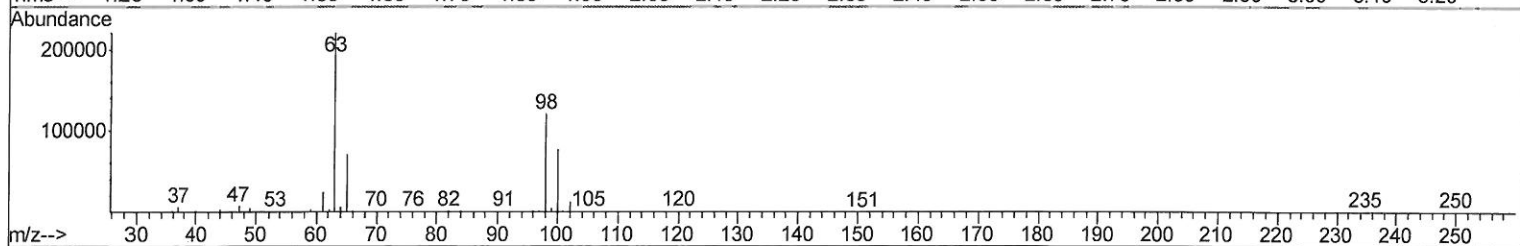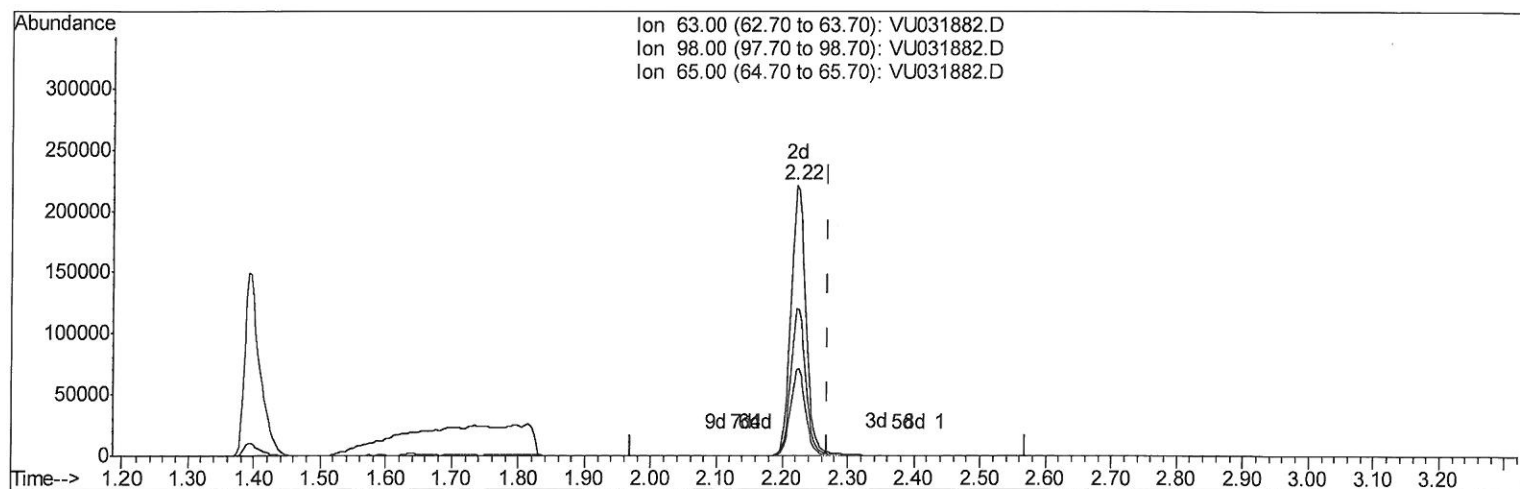

TIC: VU031882.D

(11) 1,1-Dichloroethene-d2 (S)

2.222min (-0.048) 19.34ug/L m

response 350263

Ion Exp% Act%

63.00 100 100

98.00 66.60 0.02#

65.00 23.40 0.01#

0.00 0.00 0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU051019\

Quantitation Report (QT/LSC Reviewed)

Data File : VU031882.D

Acq On : 10 May 2019 12:40

Operator : JC/SP

Sample : K2690-19ME

Misc : 5.43g/5mL/100uL/5.0mL/MSVOA_U/MEOH

ALS Vial : 7 Sample Multiplier: 1

Instrument :

MSVOA_U

ClientSampleId :

A5165ME

Manual Integrations
APPROVEDMMDadoda
5/11/2019 11:48:40 AM

Quant Time: May 11 01:48:08 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M

Quant Title : VOC Analysis

QLast Update : Sat May 11 00:57:57 2019

Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	1086442	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	1109007	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	458173	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	234296	25.77	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	51.54%#
7) Chloroethane-d5	1.64	69	139296	19.82	ug/L	-0.03
Spiked Amount	50.000	Range	70 - 130	Recovery	=	39.64%#
11) 1,1-Dichloroethene-d2	2.22	63	350263m	19.34	ug/L	-0.05
Spiked Amount	50.000	Range	60 - 125	Recovery	=	38.68%#
21) 2-Butanone-d5	4.20	46	602469	73.13	ug/L	0.03
Spiked Amount	100.000	Range	40 - 130	Recovery	=	73.13%#
24) Chloroform-d	4.64	84	540471	32.46	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	64.92%#
26) 1,2-Dichloroethane-d4	5.30	65	374908	34.46	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	68.92%#
32) Benzene-d6	5.33	84	1009516	29.64	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	59.28%#
36) 1,2-Dichloropropane-d6	6.32	67	377216	31.48	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	62.96%#
41) Toluene-d8	7.56	98	820274	27.65	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	55.30%#
43) trans-1,3-Dichloropropene-	7.85	79	150042	29.17	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	58.34%#
47) 2-Hexanone-d5	8.32	63	452159	87.19	ug/L	0.02
Spiked Amount	100.000	Range	45 - 130	Recovery	=	87.19%#
57) 1,1,2,2-Tetrachloroethane-	10.43	84	654844	40.73	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	81.46%#
64) 1,2-Dichlorobenzene-d4	11.86	152	341027	35.39	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	70.78%#

7MA
5/15/19

Target Compounds

Target Compounds				Qvalue
34) Trichloroethene	6.18	95	326637	33.048 ug/L 98
46) Tetrachloroethene	8.22	164	22283	3.307 ug/L 92

(#)=qualifier out of range (m)=manual integration (+)=signals summed